




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030491.D
Acq On : 25 Mar 2024 21:11
Operator : MA/JU
Sample : P1841-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK4

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

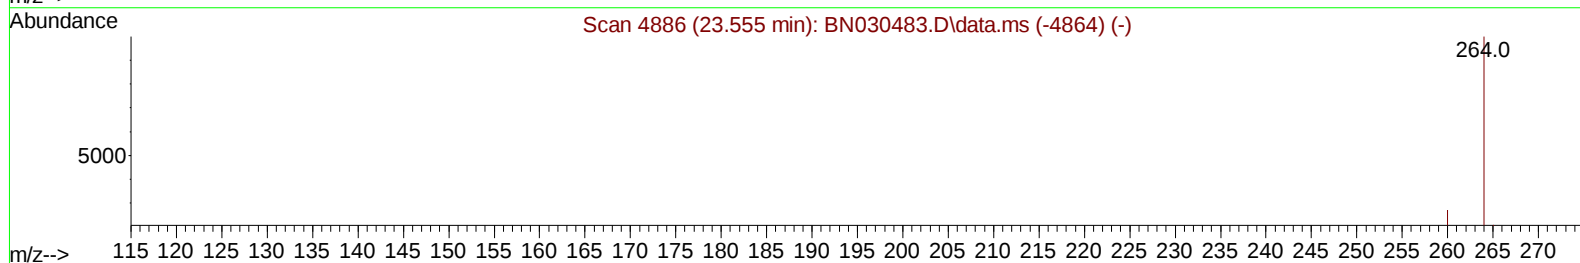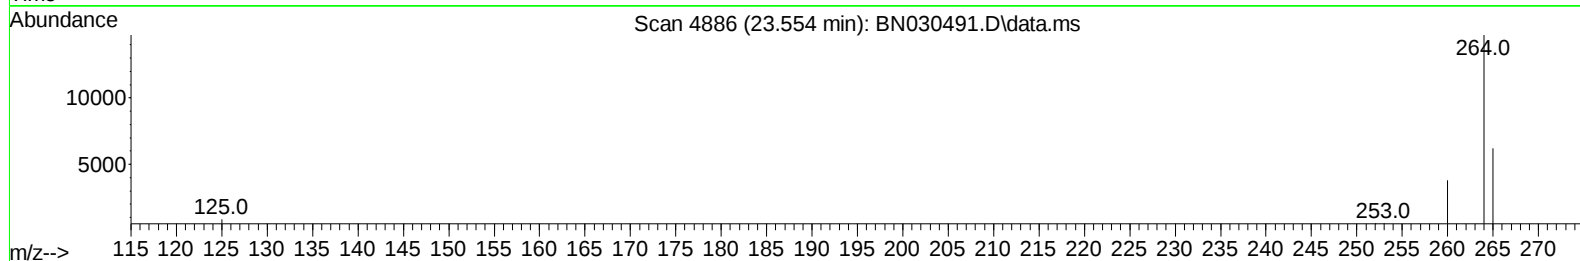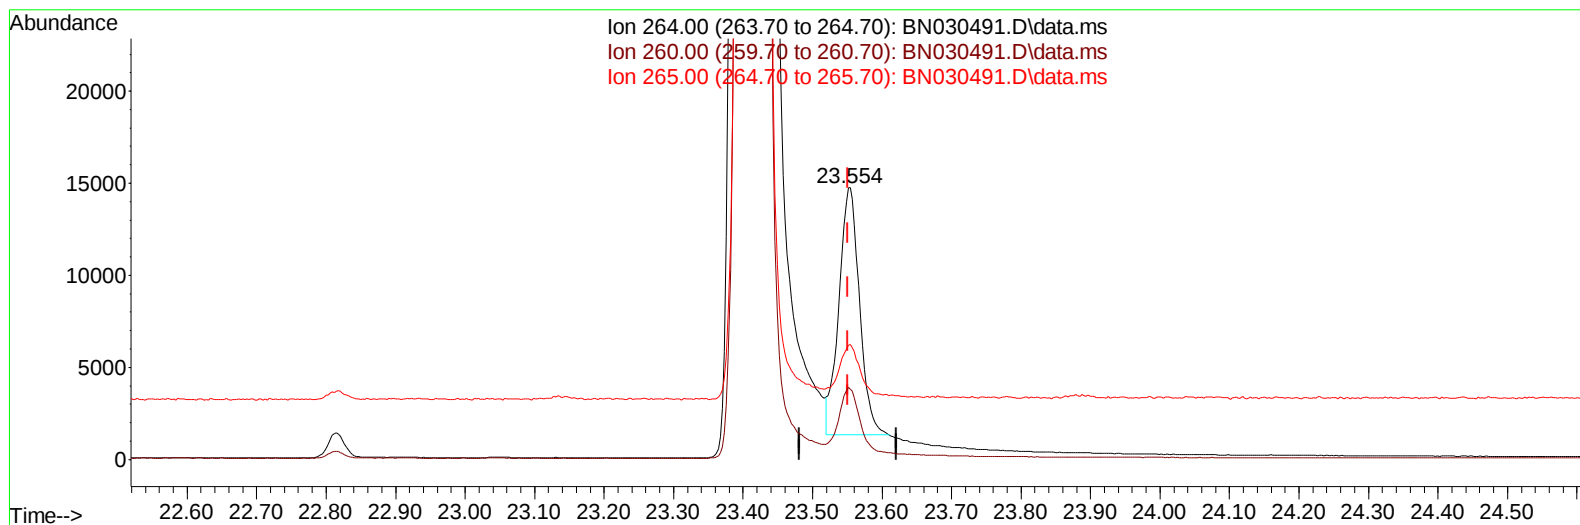

TIC: BN030491.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/u1

response 27699

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	25.86
265.00	41.20	42.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030491.D
Acq On : 25 Mar 2024 21:11
Operator : MA/JU
Sample : P1841-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK4

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

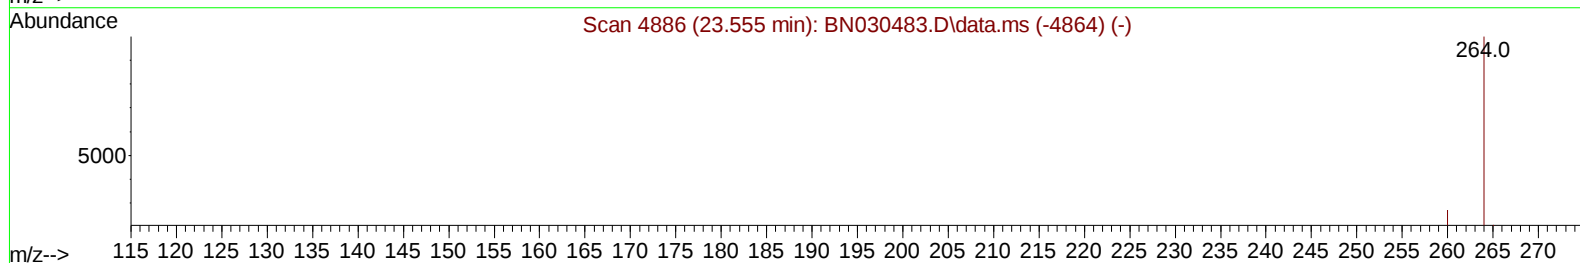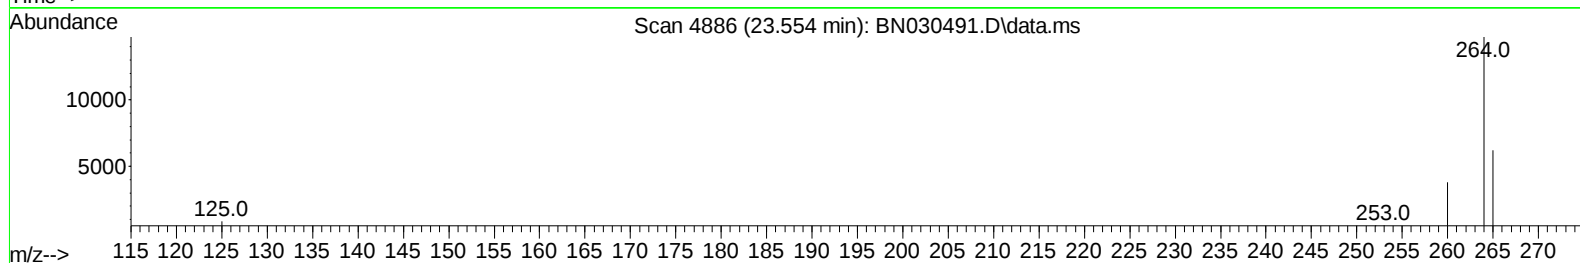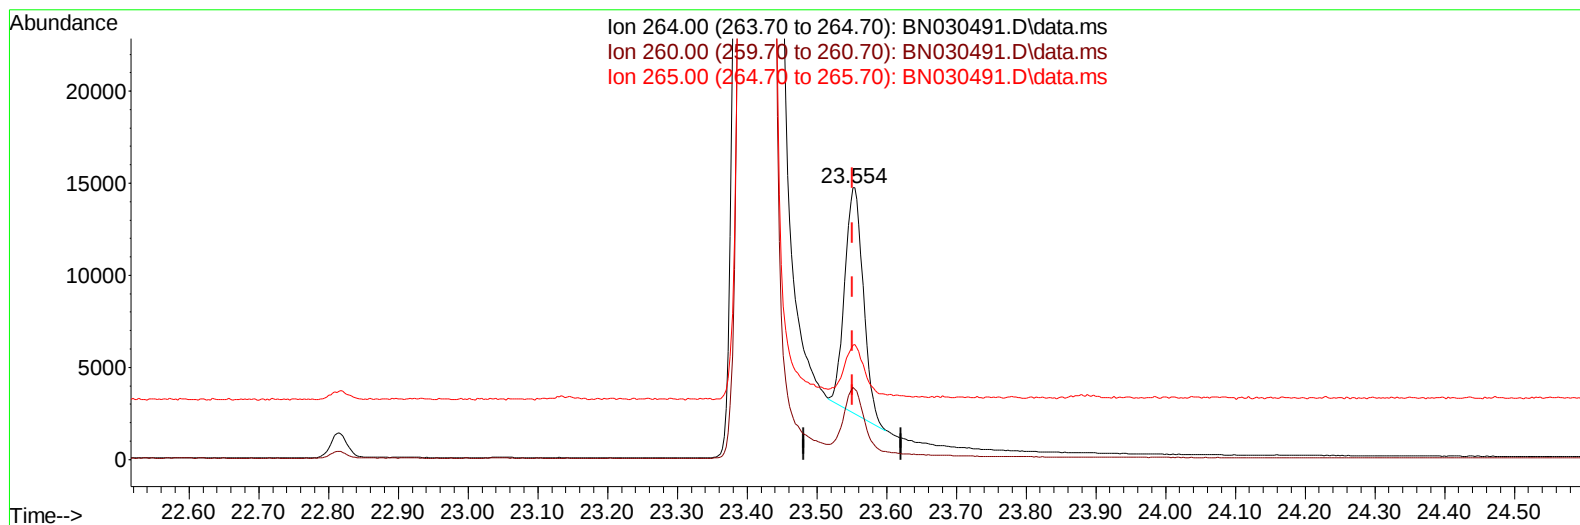

TIC: BN030491.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul m

response 22718

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	25.86
265.00	41.20	42.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030491.D
 Acq On : 25 Mar 2024 21:11
 Operator : MA/JU
 Sample : P1841-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.728	152		8871	0.400	ng/ul	0.00
4) Naphthalene-d8	10.507	136		27910	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164		16788	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.108	188		40273	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240		27240	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264		22718m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.218	96		50239	4.820	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152		13121	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.142	212		34953	0.411	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.252	88		14048	1.304	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030491.D
Acq On : 25 Mar 2024 21:11
Operator : MA/JU
Sample : P1841-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK4

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

