




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030492.D
Acq On : 25 Mar 2024 21:47
Operator : MA/JU
Sample : P1841-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

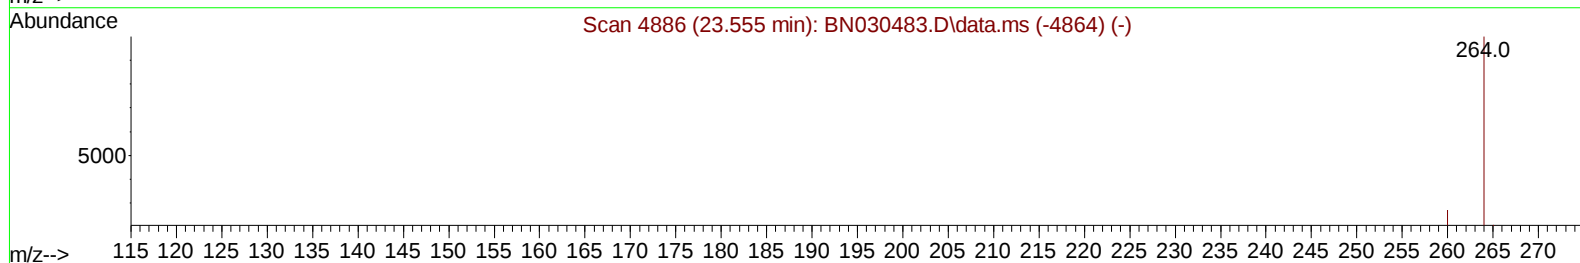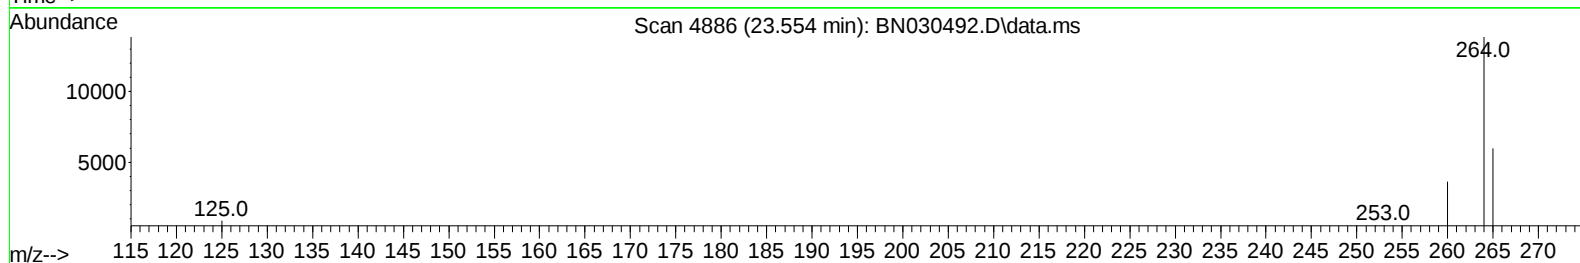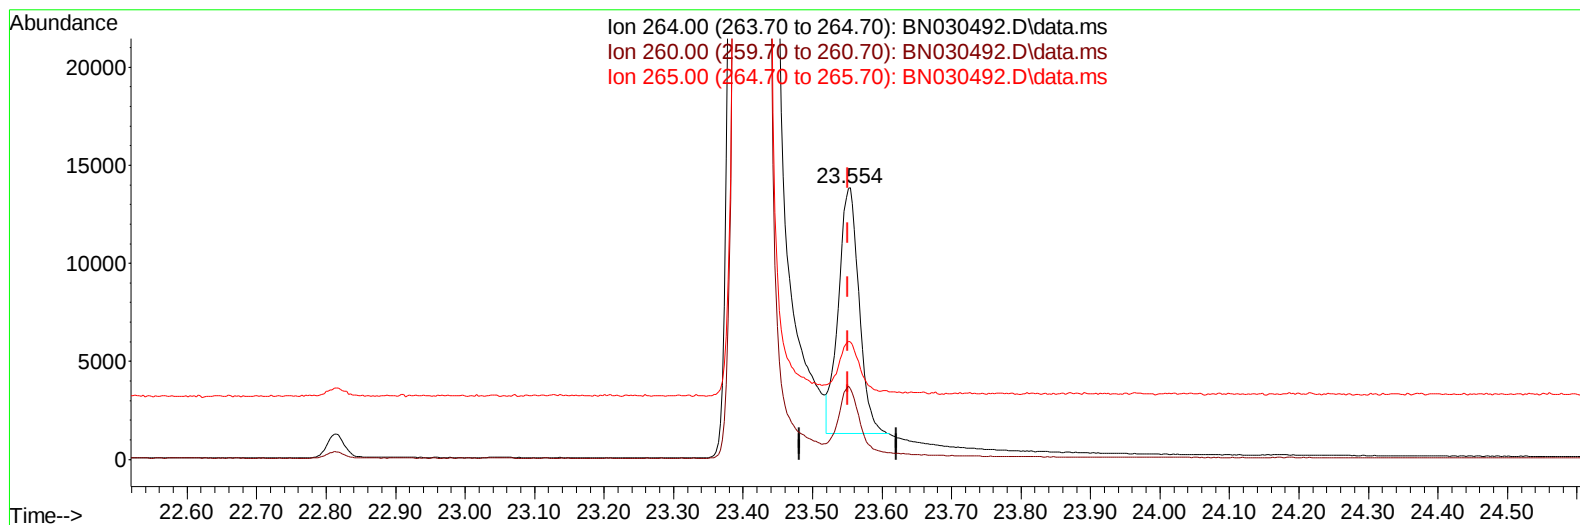

TIC: BN030492.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/u1

response 26040

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.12
265.00	41.20	43.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030492.D
Acq On : 25 Mar 2024 21:47
Operator : MA/JU
Sample : P1841-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

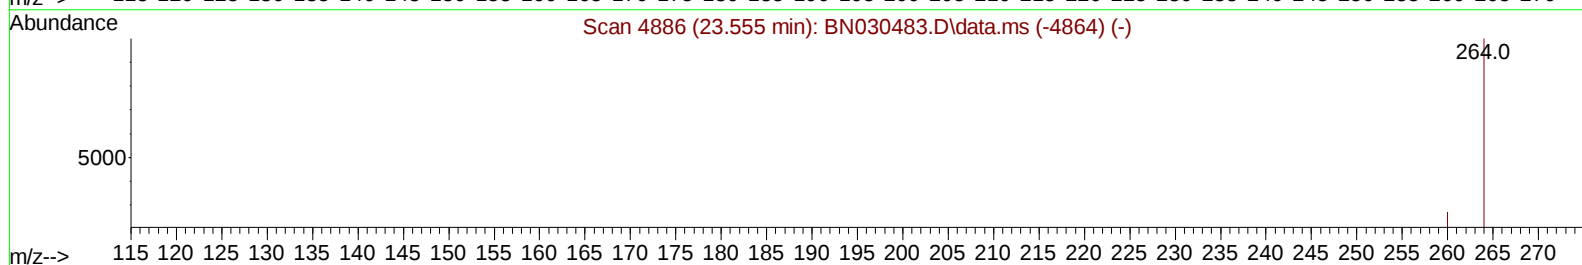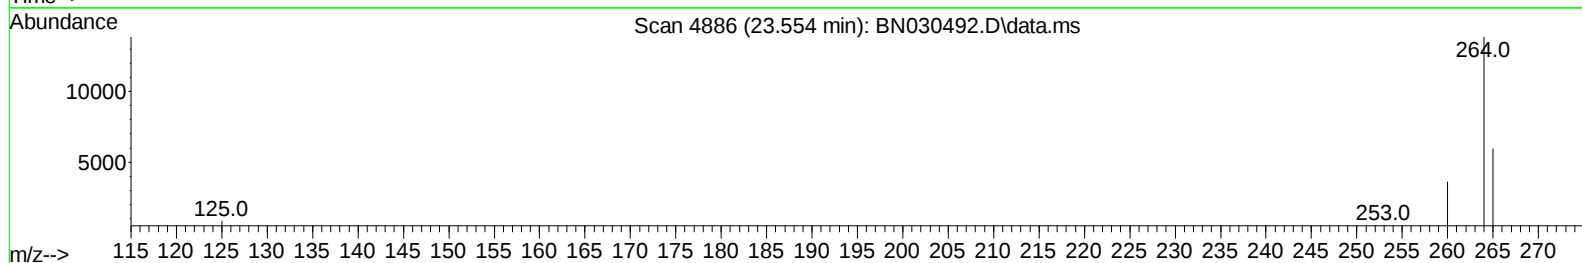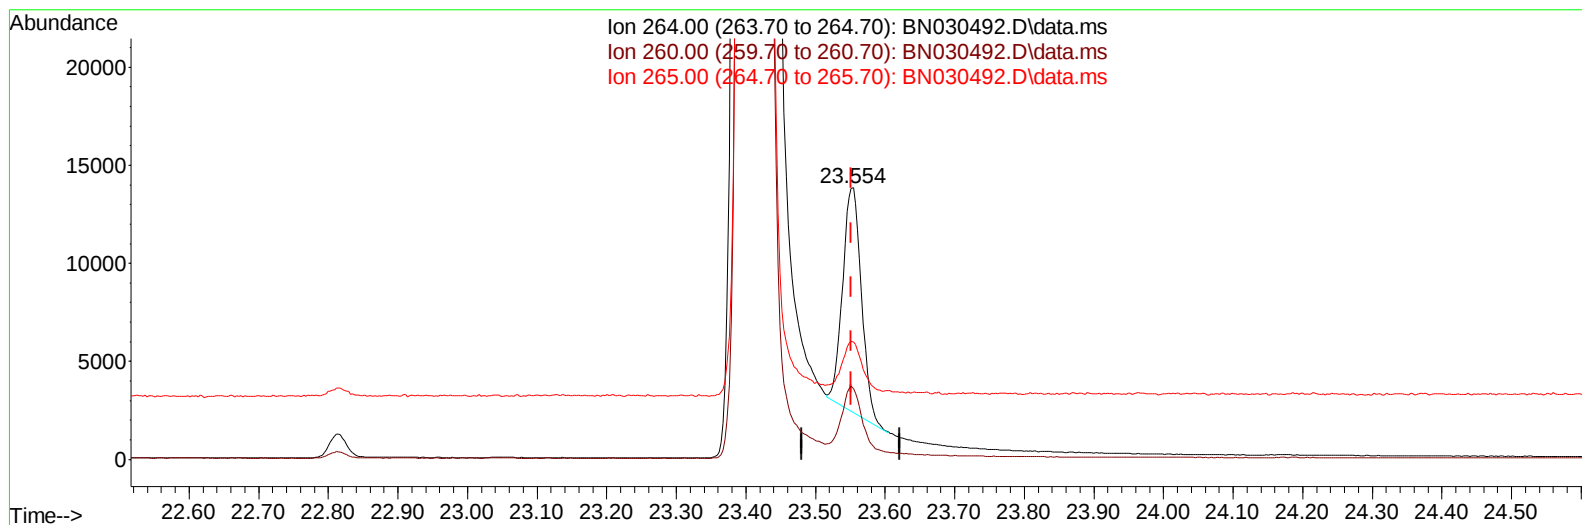

TIC: BN030492.D\data.ms

(23) Perylene-d12 (I)

23.554min (+ 0.003) 0.40 ng/ul m

response 21290

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	26.12
265.00	41.20	43.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030492.D
 Acq On : 25 Mar 2024 21:47
 Operator : MA/JU
 Sample : P1841-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.728	152		8690	0.400	ng/ul	0.00
4) Naphthalene-d8	10.507	136		27096	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164		16243	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.108	188		38663	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240		25860	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264		21290m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.218	96		43901	4.299	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152		13291	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.142	212		33521	0.415	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.256	88		11581	1.097	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030492.D
Acq On : 25 Mar 2024 21:47
Operator : MA/JU
Sample : P1841-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:32:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

