

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030487.D
 Acq On : 25 Mar 2024 18:46
 Operator : MA/JU
 Sample : P1813-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0LX9

Quant Time: Mar 28 01:41:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.729	152	11285	0.400	ng/ul	0.00
4) Naphthalene-d8	10.513	136	36030	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.363	164	23431	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.112	188	49539	0.400	ng/ul #	0.00
17) Chrysene-d12	21.304	240	34100	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264	25973m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	52920	3.991	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	17074	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	40259	0.378	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.256	88	2994	0.218	ng/ul#	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030487.D
Acq On : 25 Mar 2024 18:46
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0LX9


Quant Time: Mar 28 01:41:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

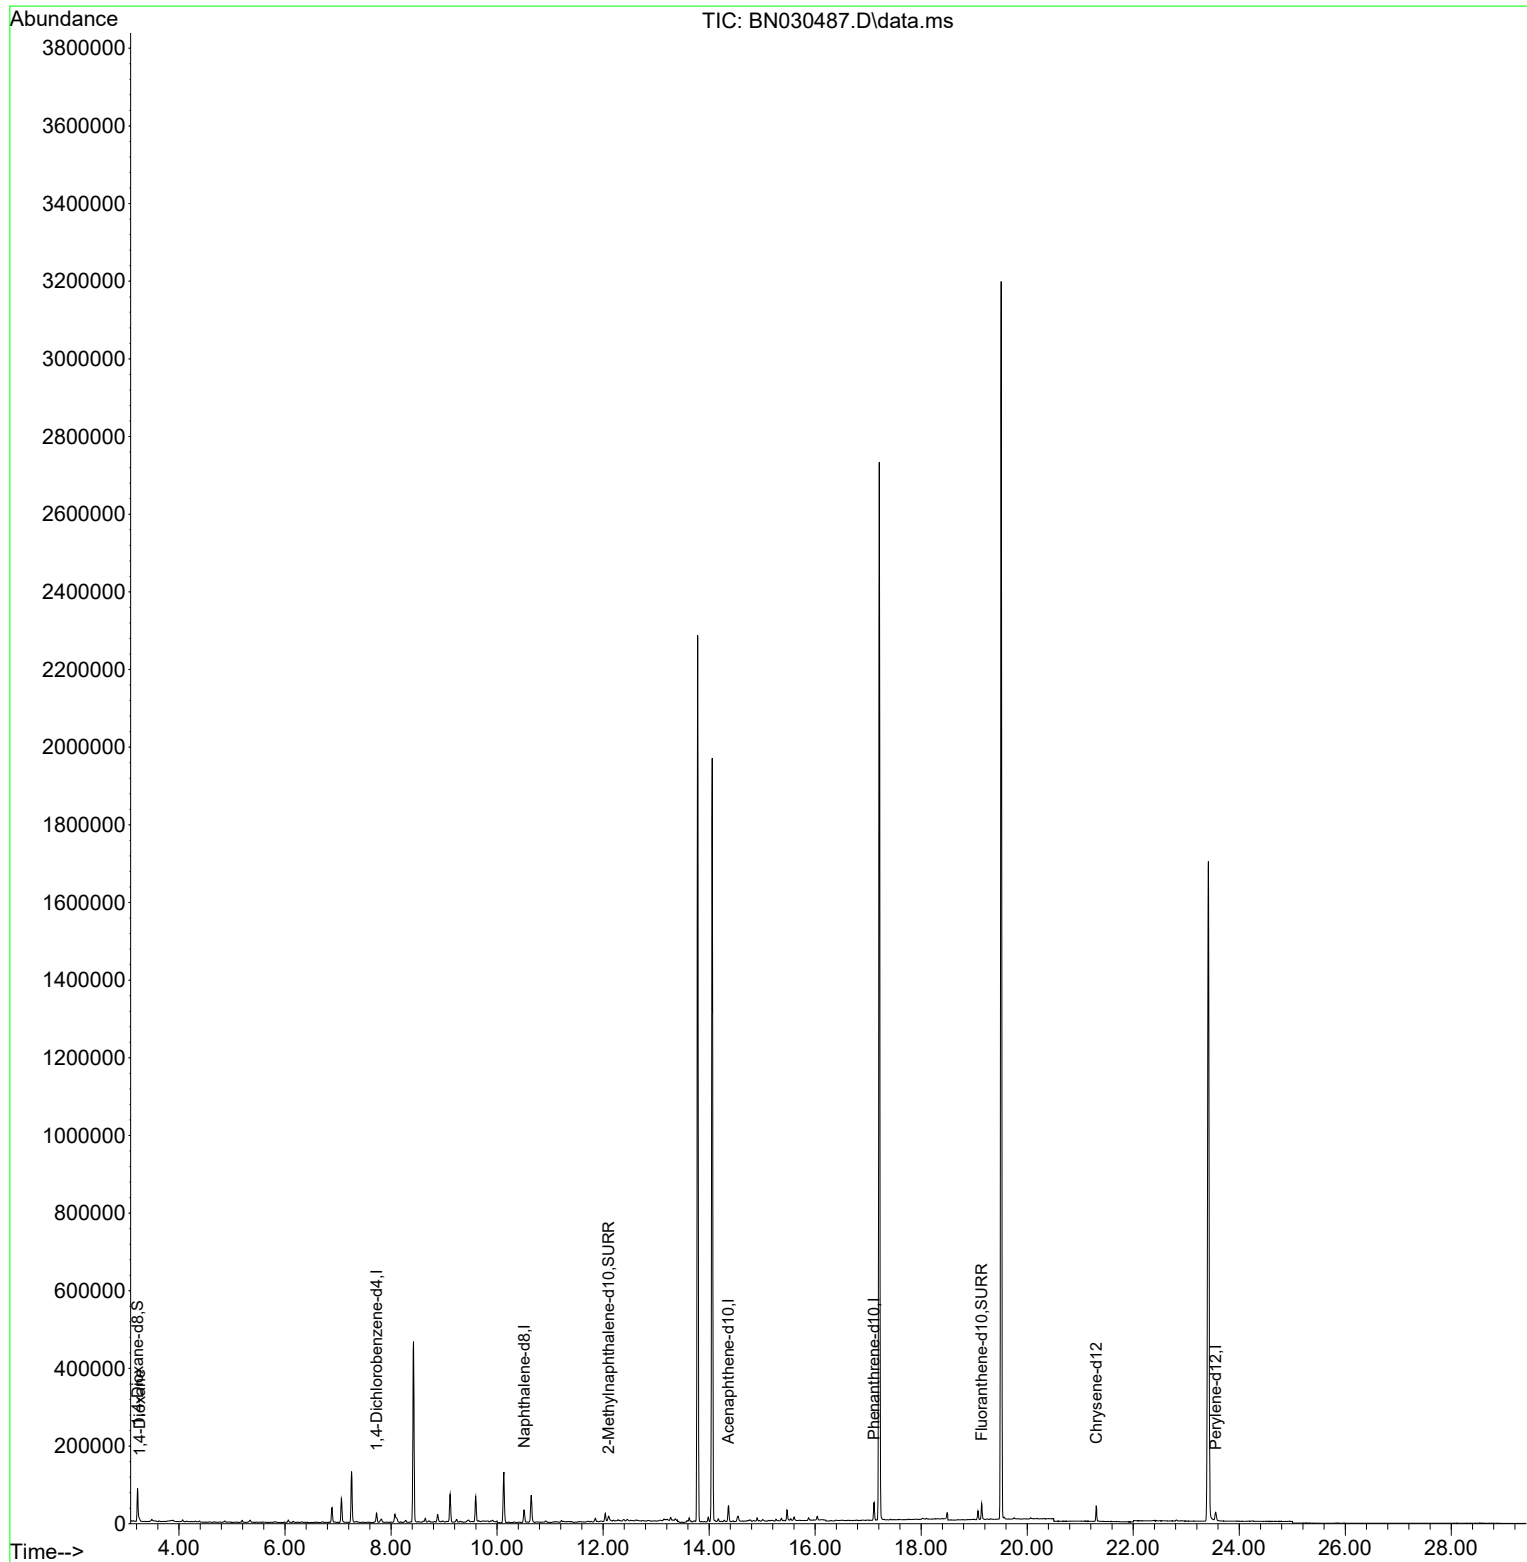

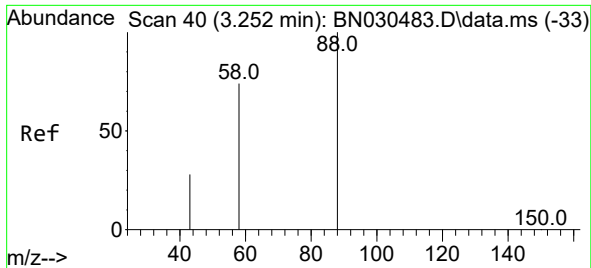

#2
 1,4-Dioxane
 Concen: 0.218 ng/ul
 RT: 3.256 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BN030487.D
 Acq: 25 Mar 2024 18:46

Instrument :
 BNA_N
 ClientSampleId :
 E0LX9

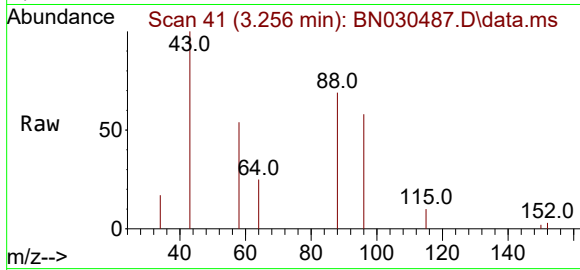

Tgt Ion: 88 Resp: 2994
 Ion Ratio Lower Upper
 88 100
 43 144.4 29.2 43.8#
 58 77.3 46.3 69.5#

