

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030490.D
 Acq On : 25 Mar 2024 20:35
 Operator : MA/JU
 Sample : P1841-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.729	152	9107	0.400	ng/u1	0.00
4) Naphthalene-d8	10.513	136	28534	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.363	164	17145	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.108	188	39930	0.400	ng/u1	0.00
17) Chrysene-d12	21.301	240	27654	0.400	ng/u1	0.00
23) Perylene-d12	23.552	264	24041m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	63293m	5.915	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.102	152	13240	0.329	ng/u1	0.00
18) Fluoranthene-d10	19.142	212	34701	0.402	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	14050	1.270	ng/u1	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030490.D
Acq On : 25 Mar 2024 20:35
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024


Quant Time: Mar 25 23:32:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

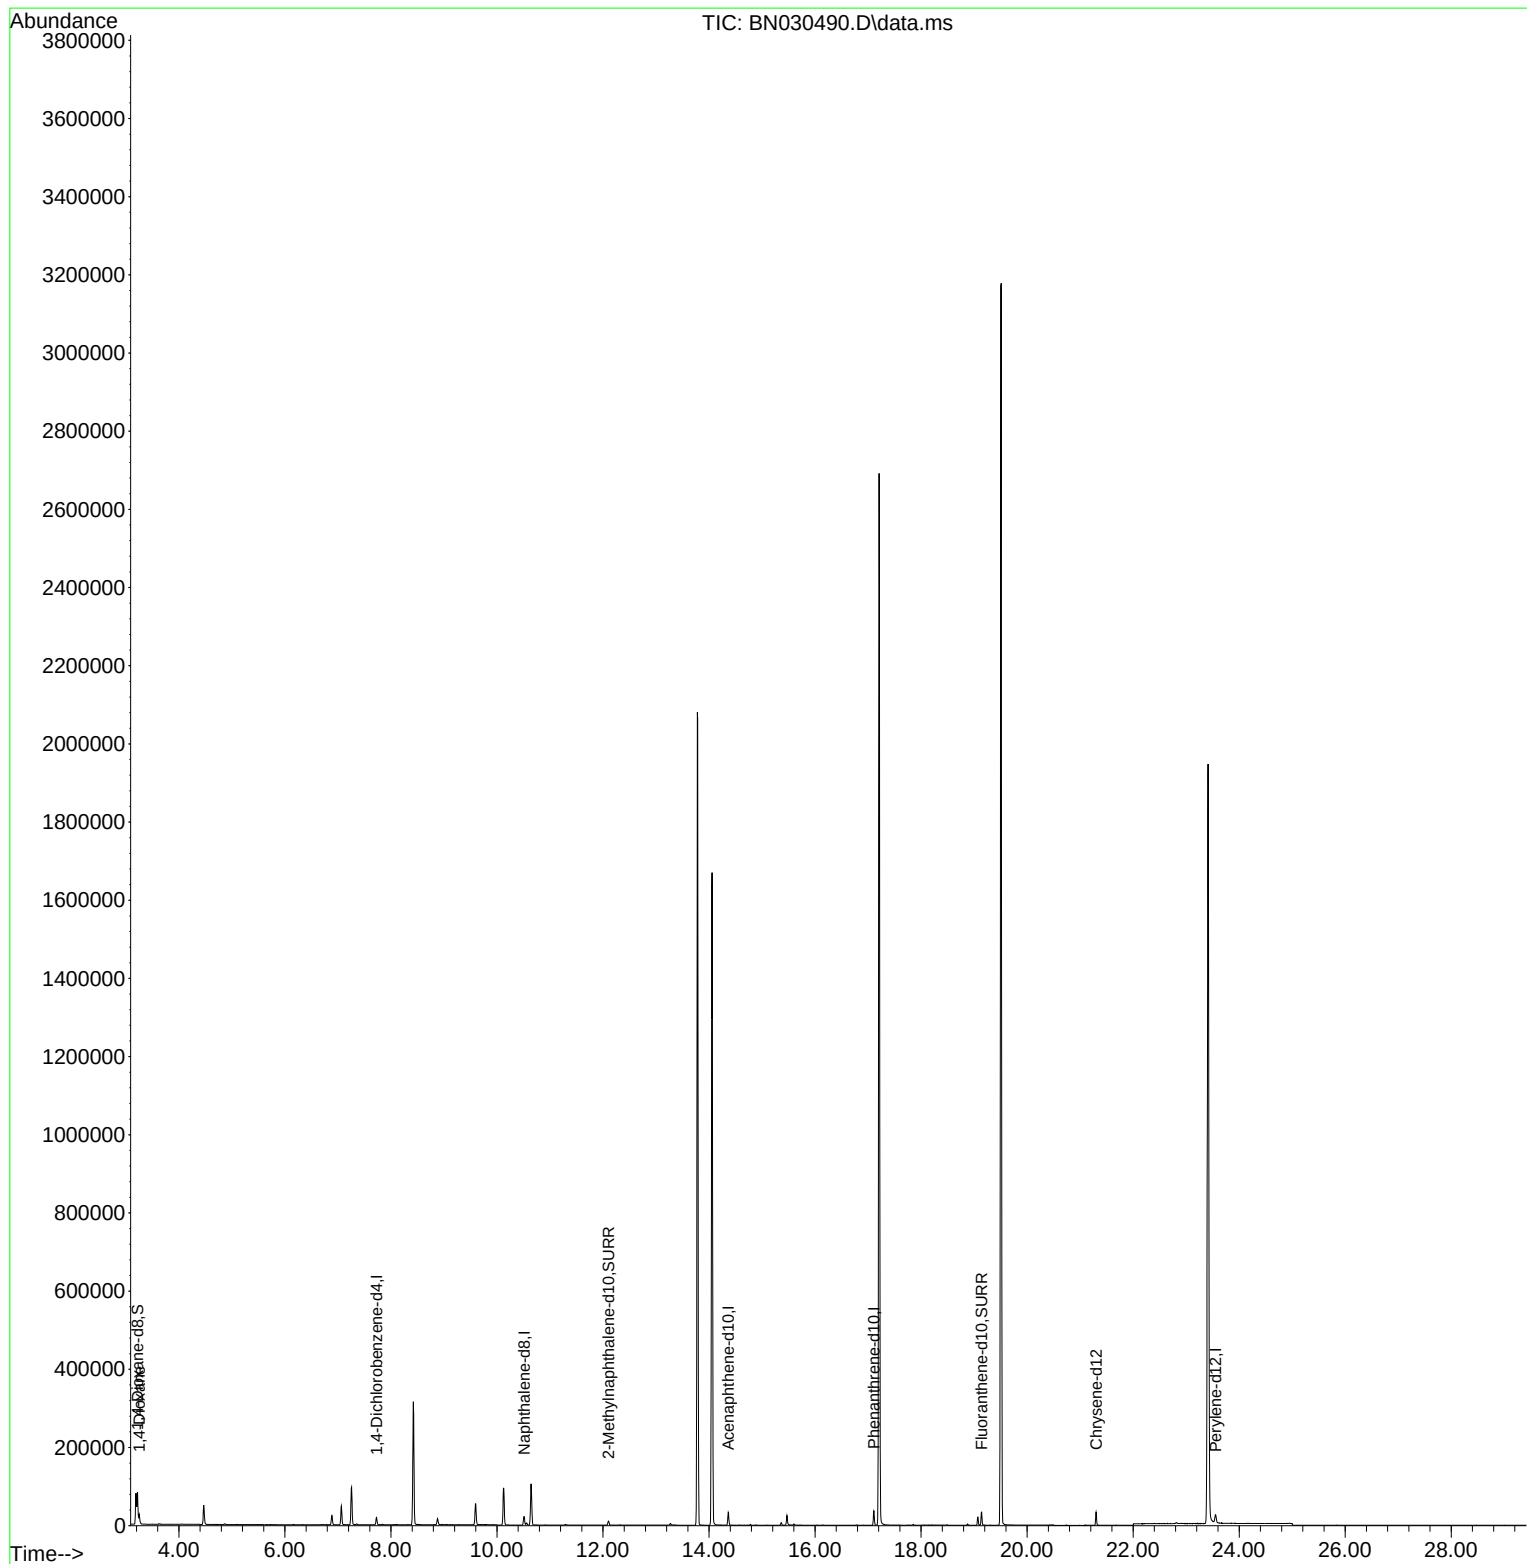

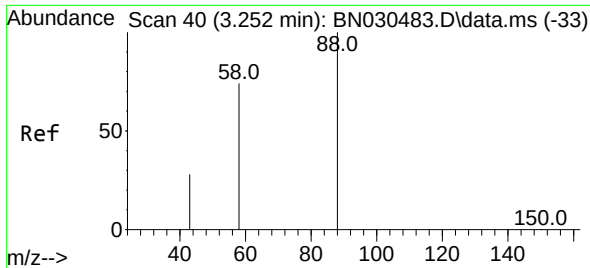

#2
 1,4-Dioxane
 Concen: 1.270 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.008 min
 Lab File: BN030490.D
 Acq: 25 Mar 2024 20:35

Instrument :
 BNA_N
 ClientSampleId :
 C0AK3

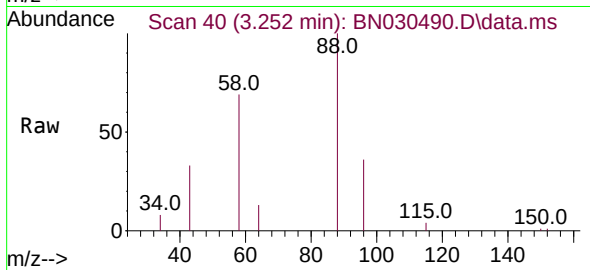

Tgt Ion: 88 Resp: 14050
 Ion Ratio Lower Upper
 88 100
 43 32.9 29.2 43.8
 58 68.8 46.3 69.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

