

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
 Data File : BN030491.D
 Acq On : 25 Mar 2024 21:11
 Operator : MA/JU
 Sample : P1841-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 25 23:32:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 25 13:38:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	8871	0.400	ng/ul	0.00
4) Naphthalene-d8	10.507	136	27910	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.363	164	16788	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.108	188	40273	0.400	ng/ul	0.00
17) Chrysene-d12	21.304	240	27240	0.400	ng/ul	0.00
23) Perylene-d12	23.554	264	22718m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	50239	4.820	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.102	152	13121	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.142	212	34953	0.411	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	14048	1.304	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032524\
Data File : BN030491.D
Acq On : 25 Mar 2024 21:11
Operator : MA/JU
Sample : P1841-02
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AK4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024


Quant Time: Mar 25 23:32:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 25 13:38:40 2024
Response via : Initial Calibration

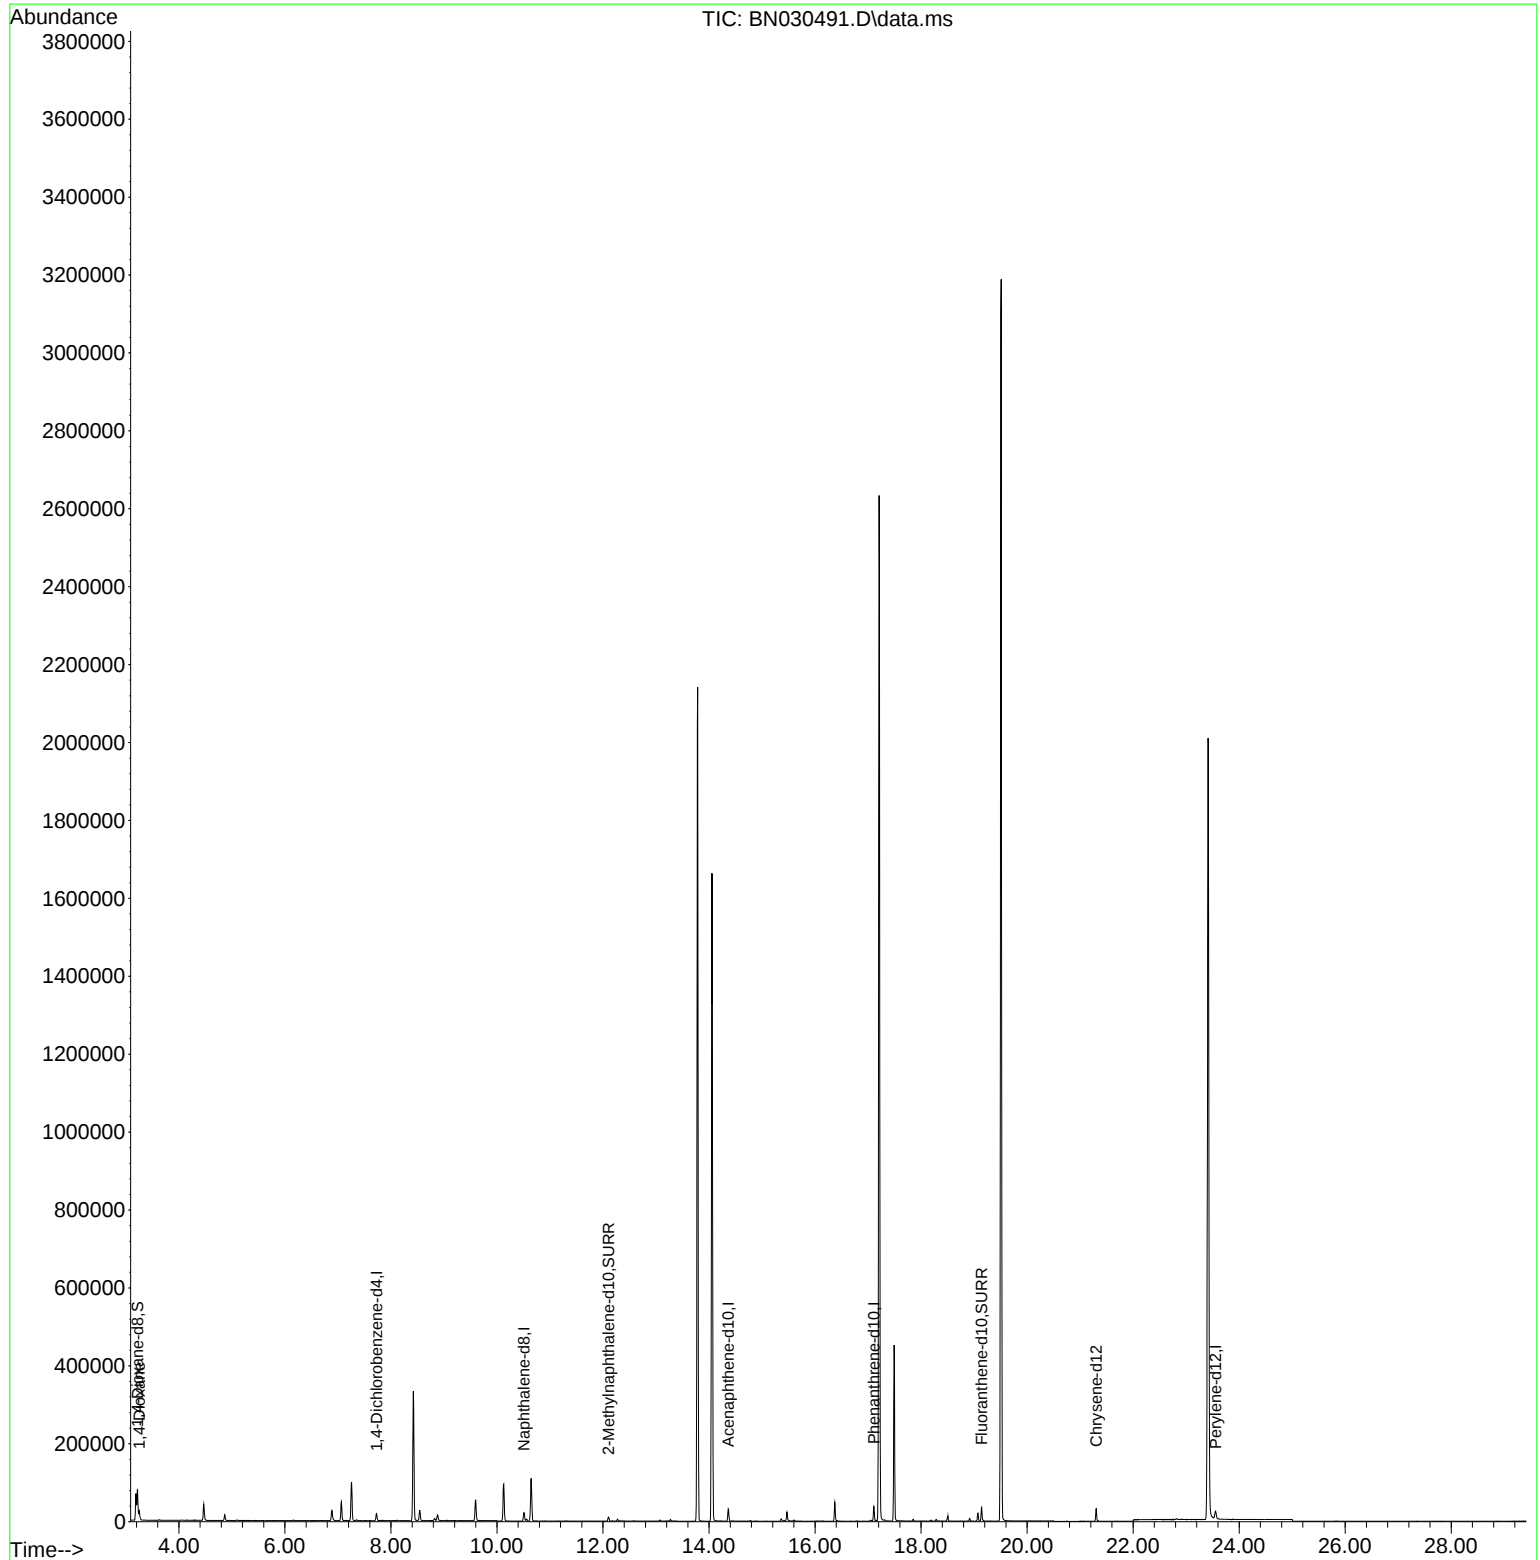

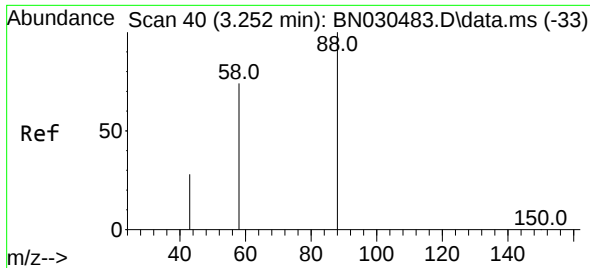

#2
 1,4-Dioxane
 Concen: 1.304 ng/ul
 RT: 3.252 min Scan# 40
 Delta R.T. -0.008 min
 Lab File: BN030491.D
 Acq: 25 Mar 2024 21:11

Instrument :
 BNA_N
 ClientSampleId :
 C0AK4

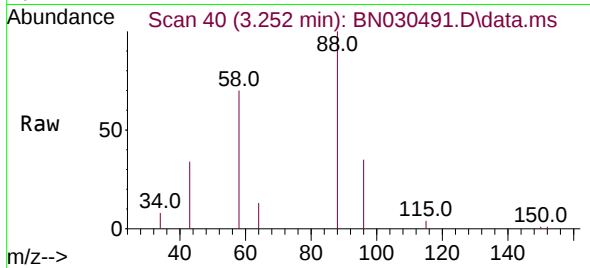

Tgt Ion: 88 Resp: 14048

Ion	Ratio	Lower	Upper
88	100		
43	33.6	29.2	43.8
58	69.9	46.3	69.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

