
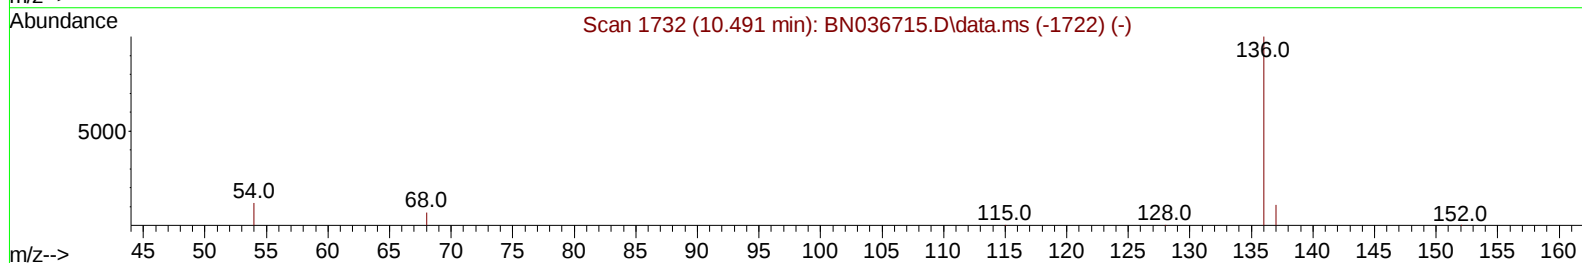
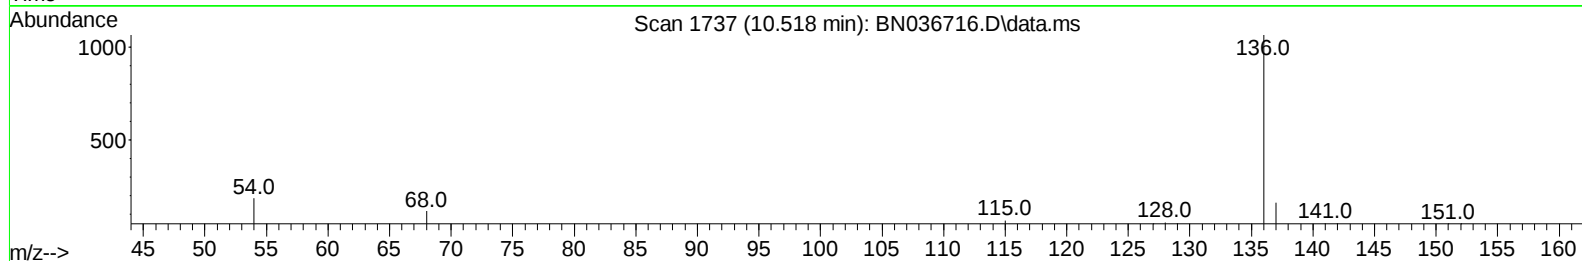


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
Data File : BN036716.D
Acq On : 25 Mar 2025 09:50
Operator : RC/JU
Sample : PB167176BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 24 17:31:03 2025
Response via : Initial Calibration

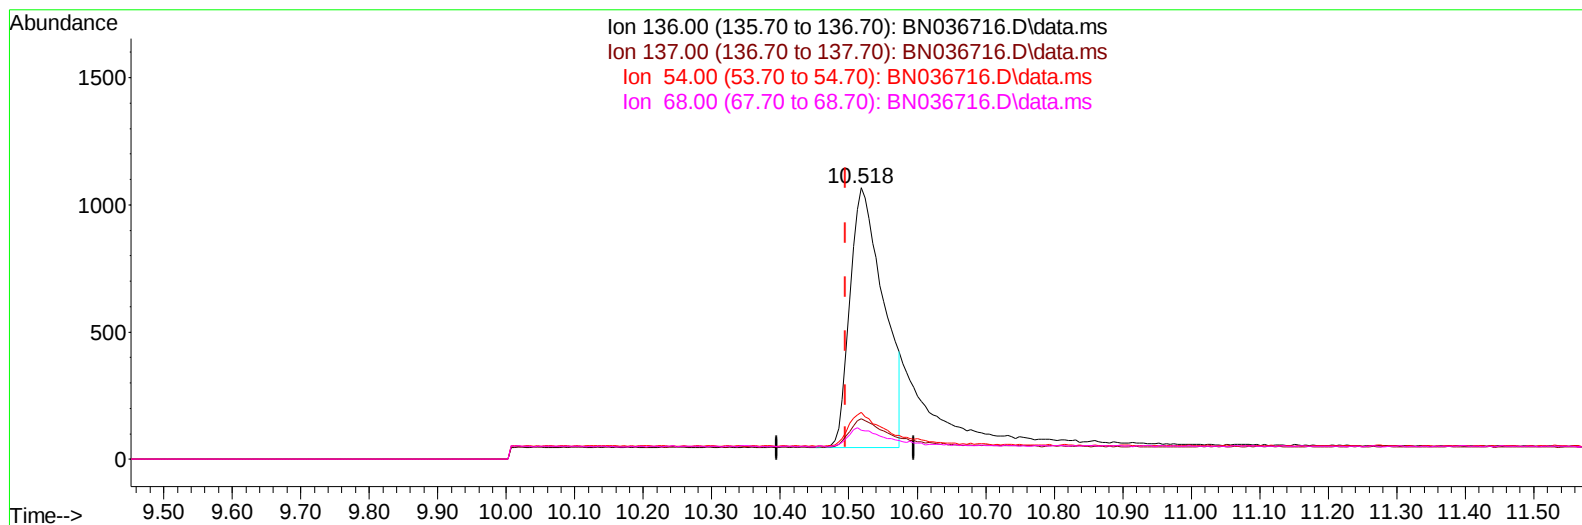

TIC: BN036716.D\data.ms

(4) Naphthalene-d8 (I)




10.518min (+ 0.023) 0.40 ng/u1

response 3438

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.60	15.09
54.00	13.90	17.24#
68.00	8.40	10.78#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
Data File : BN036716.D
Acq On : 25 Mar 2025 09:50
Operator : RC/JU
Sample : PB167176BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 24 17:31:03 2025
Response via : Initial Calibration

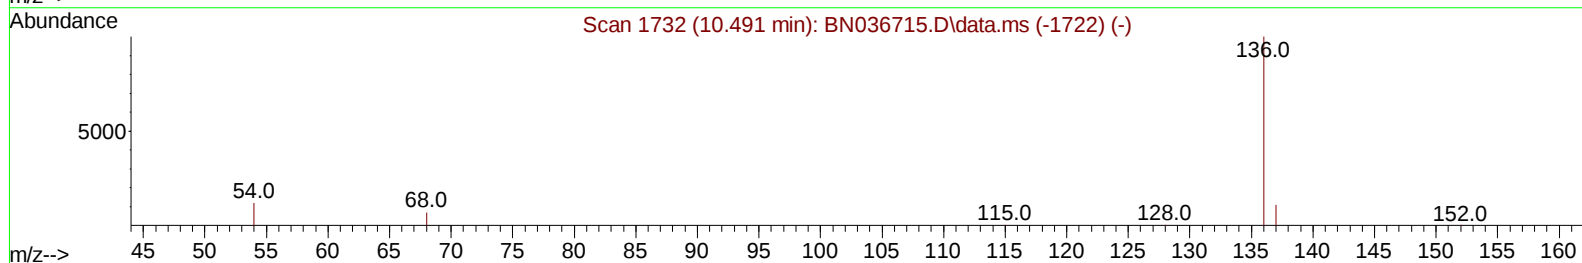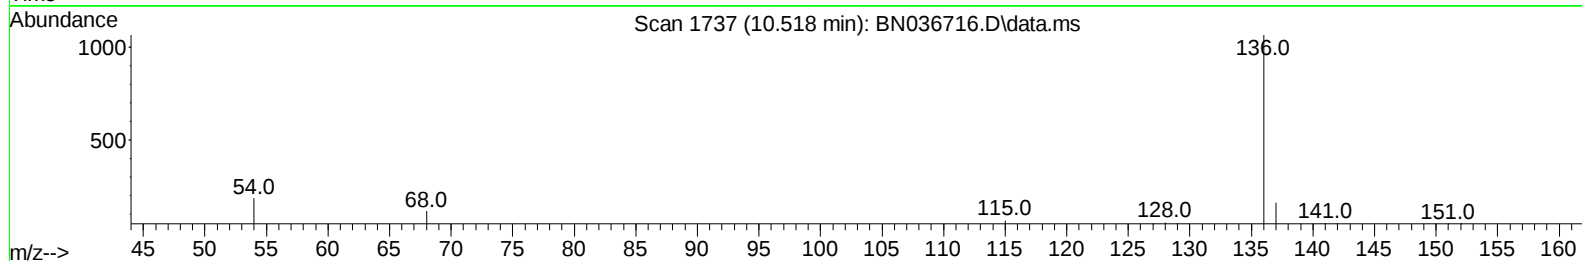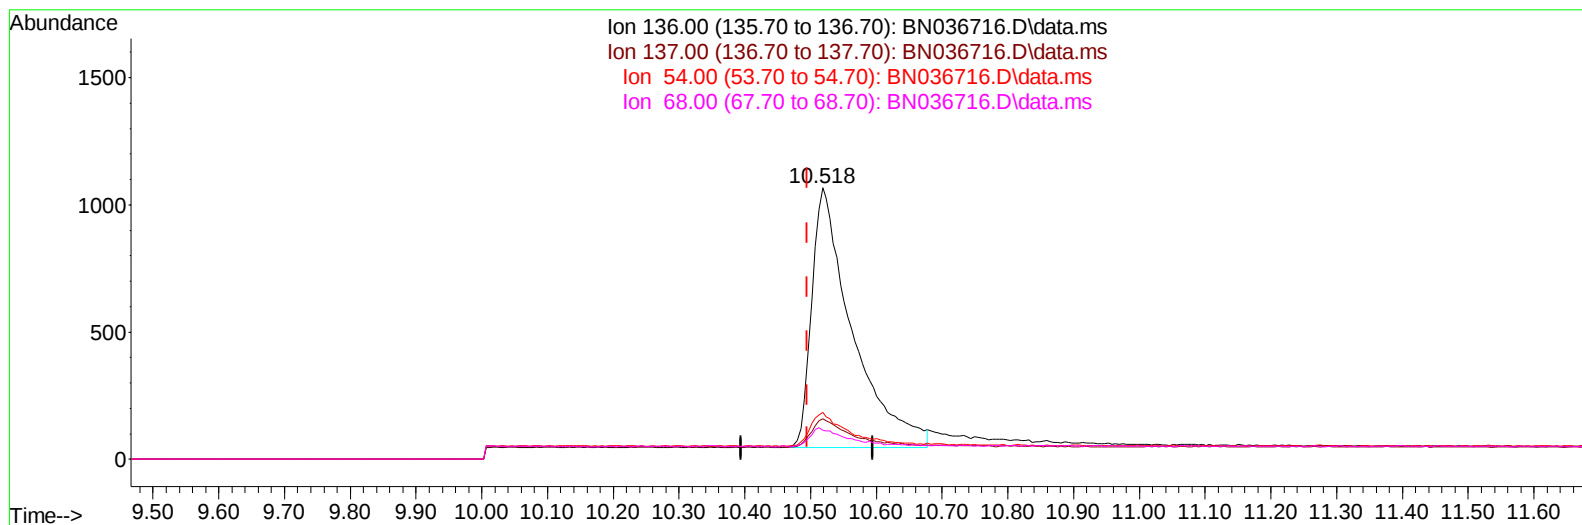

TIC: BN036716.D\data.ms

(4) Naphthalene-d8 (I)




10.518min (+ 0.023) 0.40 ng/ul m

response 4381

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.60	15.09
54.00	13.90	17.24#
68.00	8.40	10.78#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
Data File : BN036716.D
Acq On : 25 Mar 2025 09:50
Operator : RC/JU
Sample : PB167176BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 24 17:31:03 2025
Response via : Initial Calibration

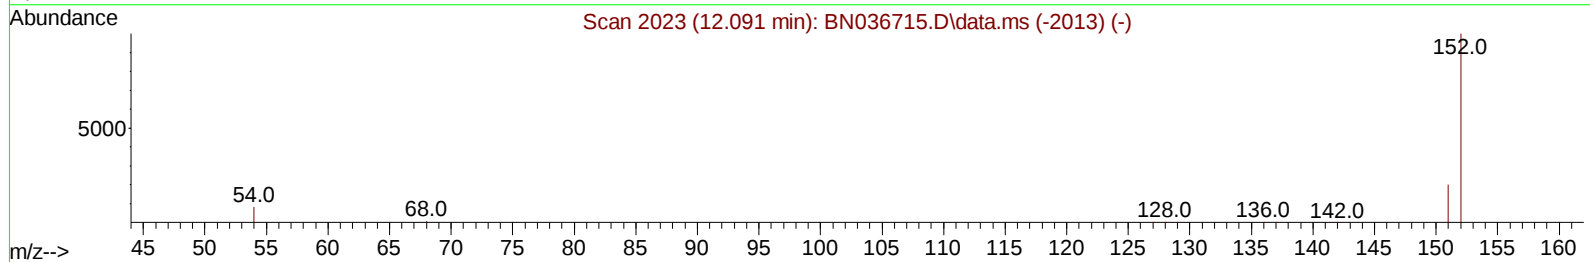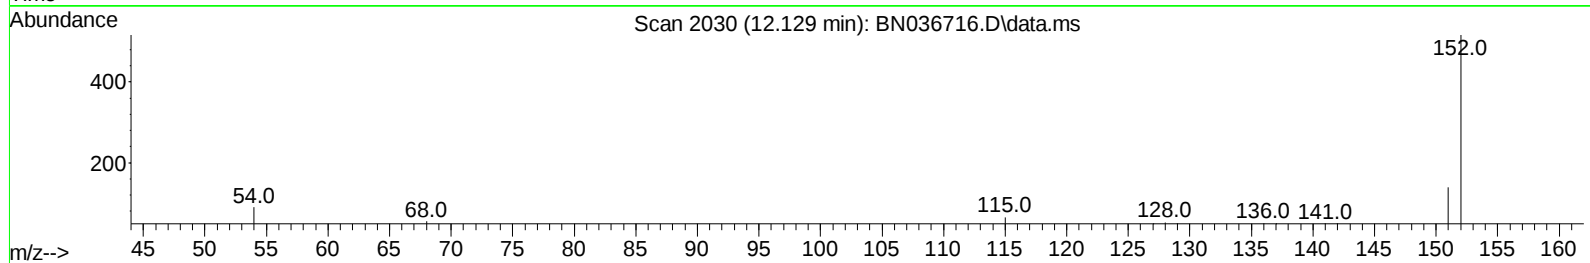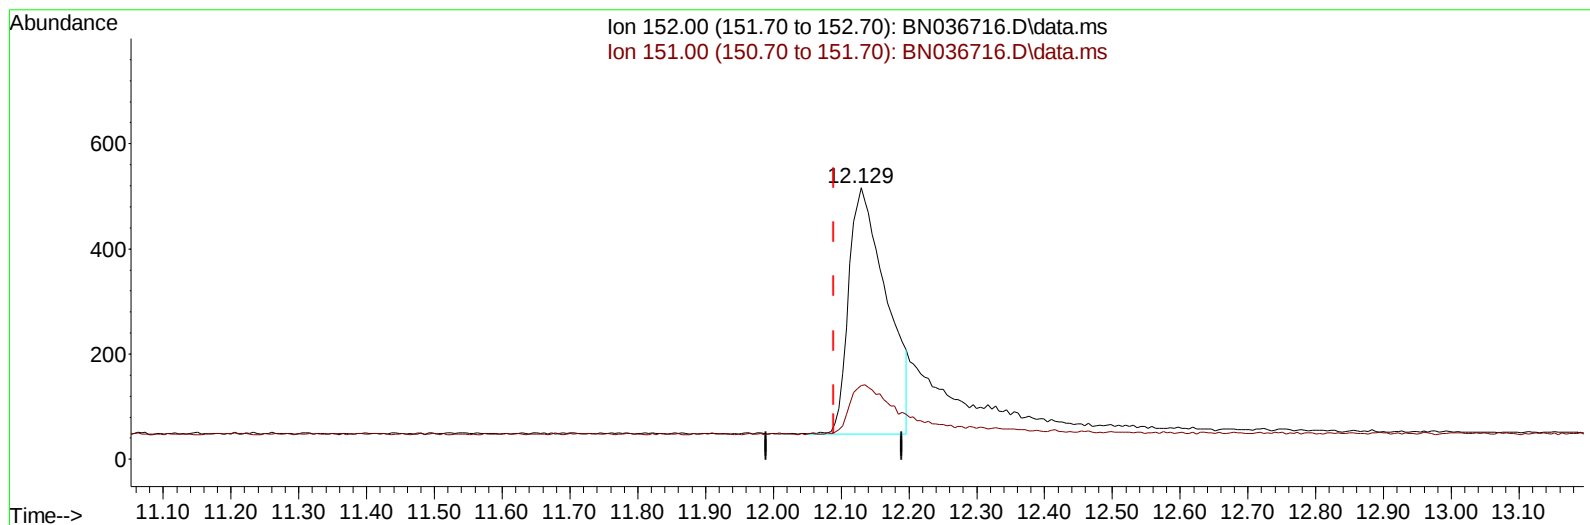

TIC: BN036716.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)




12.129min (+ 0.040) 0.29 ng/u1

response 1799

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	22.00	21.01
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
Data File : BN036716.D
Acq On : 25 Mar 2025 09:50
Operator : RC/JU
Sample : PB167176BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 24 17:31:03 2025
Response via : Initial Calibration

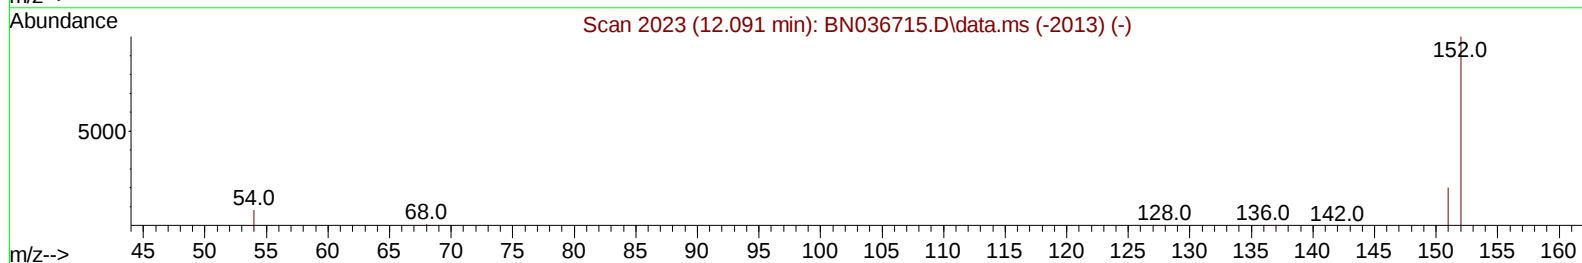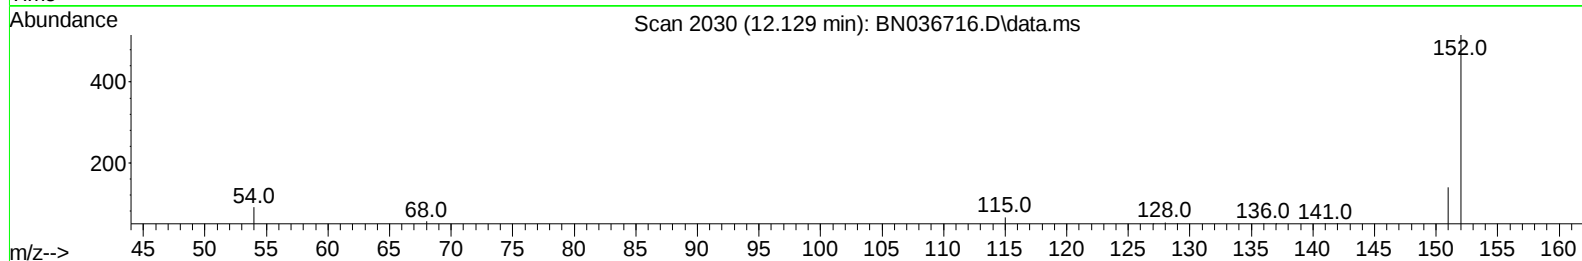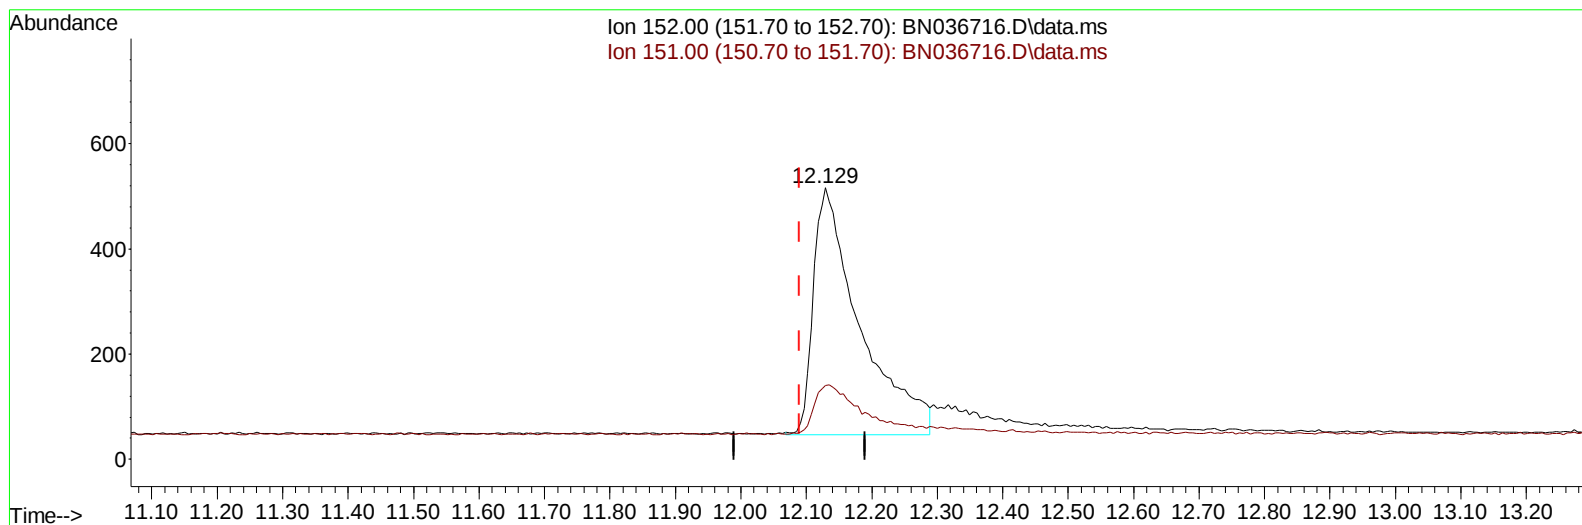

TIC: BN036716.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.129min (+ 0.040) 0.37 ng/ul m

response 2310

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	22.00	16.36#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
 Data File : BN036716.D
 Acq On : 25 Mar 2025 09:50
 Operator : RC/JU
 Sample : PB167176BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 24 17:31:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.707	152	1946	0.400	ng/ul	0.00
4) Naphthalene-d8	10.518	136	4381m	0.400	ng/ul	0.02
9) Acenaphthene-d10	14.364	164	2679	0.400	ng/ul	0.02
13) Phenanthrene-d10	17.117	188	5325	0.400	ng/ul	0.02
17) Chrysene-d12	21.293	240	4645	0.400	ng/ul	0.00
23) Perylene-d12	23.541	264	4338	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.197	96	1801	0.769	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	2310m	0.375	ng/ul	0.04
18) Fluoranthene-d10	19.133	212	6013	0.395	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032525\
Data File : BN036716.D
Acq On : 25 Mar 2025 09:50
Operator : RC/JU
Sample : PB167176BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 25 11:06:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 24 17:31:03 2025
Response via : Initial Calibration

