

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032618\
 Data File : BN000616.D
 Acq On : 26 Mar 2018 13:02
 Operator : JU/SJ
 Sample : J1969-08DL 10X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 27 02:20:15 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 27 02:19:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	140871	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	621473	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.03	164	345675	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.76	188	687591	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	545298	20.00	ng/ul	0.02
83) Perylene-d12	24.39	264	591751	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.55	99	21776	1.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.71	67	10648	1.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.94	132	14965	1.51	ng/ul	0.00
13) 4-Methylphenol-d8	9.12	113	19486	1.90	ng/ul	0.00
19) Nitrobenzene-d5	9.59	128	7844	1.55	ng/ul	0.00
22) 2-Nitrophenol-d4	10.32	143	8548	1.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	18535	1.98	ng/ul	0.00
29) 4-Chloroaniline-d4	11.38	131	4145	0.43	ng/ul	0.00
43) Dimethylphthalate-d6	14.42	166	60526	2.22	ng/ul	0.00
46) Acenaphthylene-d8	14.73	160	84148	2.34	ng/ul	0.00
51) 4-Nitrophenol-d4	15.22	143	8758	1.73	ng/ul	0.00
57) Fluorene-d10	16.01	176	57151	2.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.15	200	1054	0.27	ng/ul	0.02
70) Anthracene-d10	17.85	188	80115	2.42	ng/ul	0.00
76) Pyrene-d10	20.12	212	68806	2.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	64918	2.32	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
77) Pvrene	20.15	202	39993	1.004	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032618\
Data File : BN000616.D
Acq On : 26 Mar 2018 13:02
Operator : JU/SJ
Sample : J1969-08DL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 27 02:20:15 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 27 02:19:46 2018
Response via : Initial Calibration

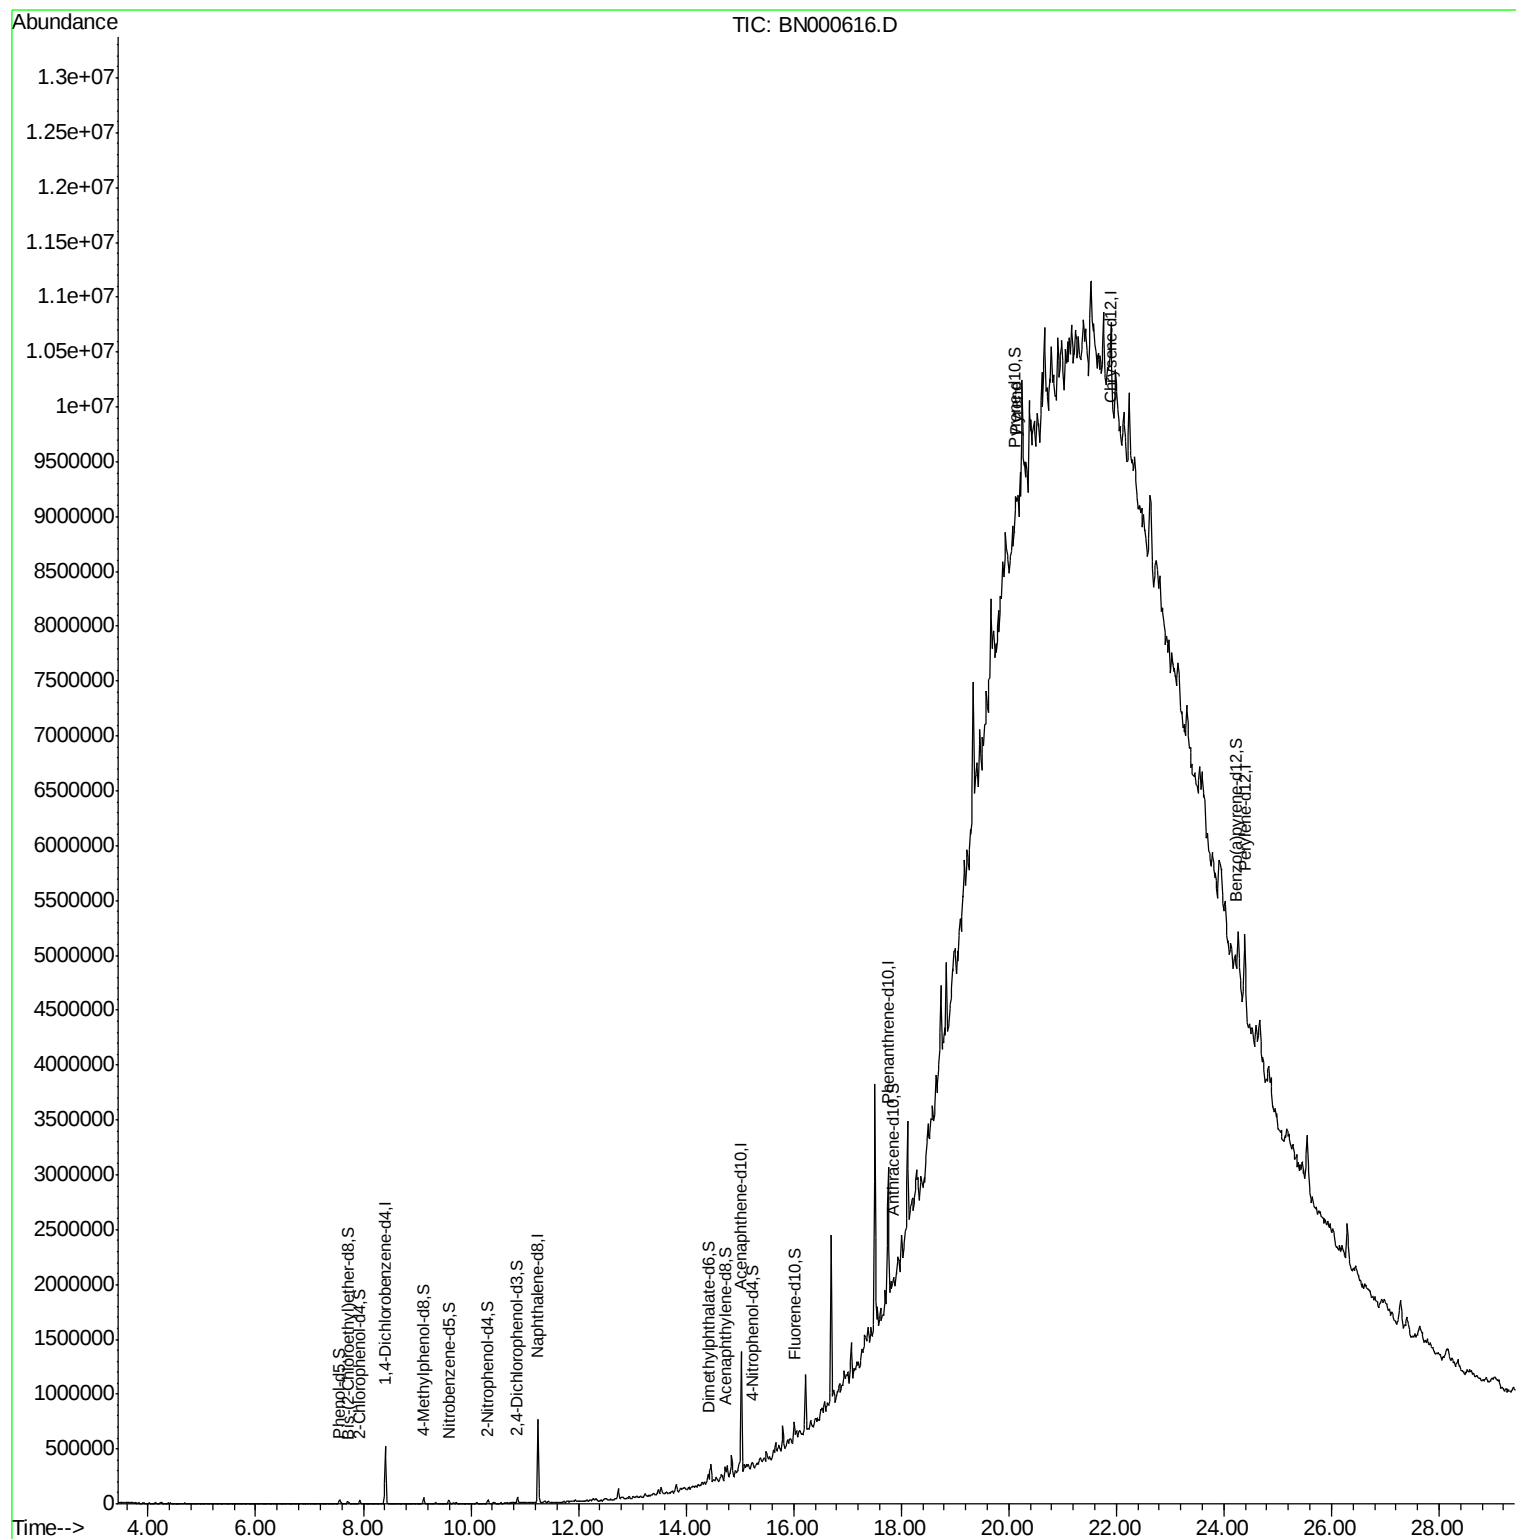

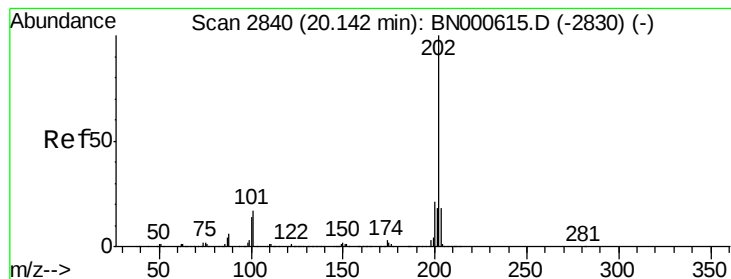

#77

Pvrene

Concen: 1.004 ng/ul

RT: 20.15 min Scan# 2841

Delta R.T. 0.01 min

Lab File: BN000616.D

Acq: 26 Mar 2018 13:02

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 202 Resp: 39993

Ion Ratio Lower Upper

202 100

101 15.8 6.9 10.3#

100 33.1 5.6 8.4#

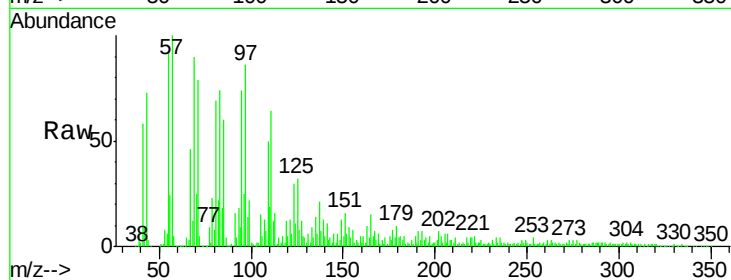

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

