

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032618\
 Data File : BN000635.D
 Acq On : 26 Mar 2018 23:53
 Operator : JU/SJ
 Sample : J1986-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEEJ1

Quant Time: Mar 27 04:08:34 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 27 03:53:32 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	124761	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	556410	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.02	164	307694	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.75	188	660848	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	717057	20.00	ng/ul	0.00
83) Perylene-d12	24.35	264	781564	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.58	96	13763	3.94	ng/uL	0.00
5) Phenol-d5	7.55	99	270788	23.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.71	67	175983	26.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.93	132	210168	23.88	ng/ul	0.00
13) 4-Methylphenol-d8	9.12	113	188498	20.79	ng/ul	0.00
19) Nitrobenzene-d5	9.59	128	110957	24.55	ng/ul	0.00
22) 2-Nitrophenol-d4	10.32	143	119846	25.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	200654	23.91	ng/ul	0.00
29) 4-Chloroaniline-d4	11.38	131	137815	16.00	ng/ul	0.00
43) Dimethylphthalate-d6	14.42	166	707952	29.12	ng/ul	0.00
46) Acenaphthylene-d8	14.72	160	885948	27.63	ng/ul	0.00
51) 4-Nitrophenol-d4	15.22	143	105046	23.27	ng/ul	0.00
57) Fluorene-d10	16.01	176	597408	28.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.13	200	76084	20.10	ng/ul	0.00
70) Anthracene-d10	17.85	188	918704	28.92	ng/ul	0.00
76) Pyrene-d10	20.11	212	1031434	26.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.20	264	1039543	28.18	ng/ul	0.00
Target Compounds						
6) Phenol	7.58	94	19336	1.628	ng/ul	97
44) Dimethylphthalate	14.46	163	109162	4.540	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032618\
Data File : BN000635.D
Acq On : 26 Mar 2018 23:53
Operator : JU/SJ
Sample : J1986-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BEEJ1

Quant Time: Mar 27 04:08:34 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 27 03:53:32 2018
Response via : Initial Calibration

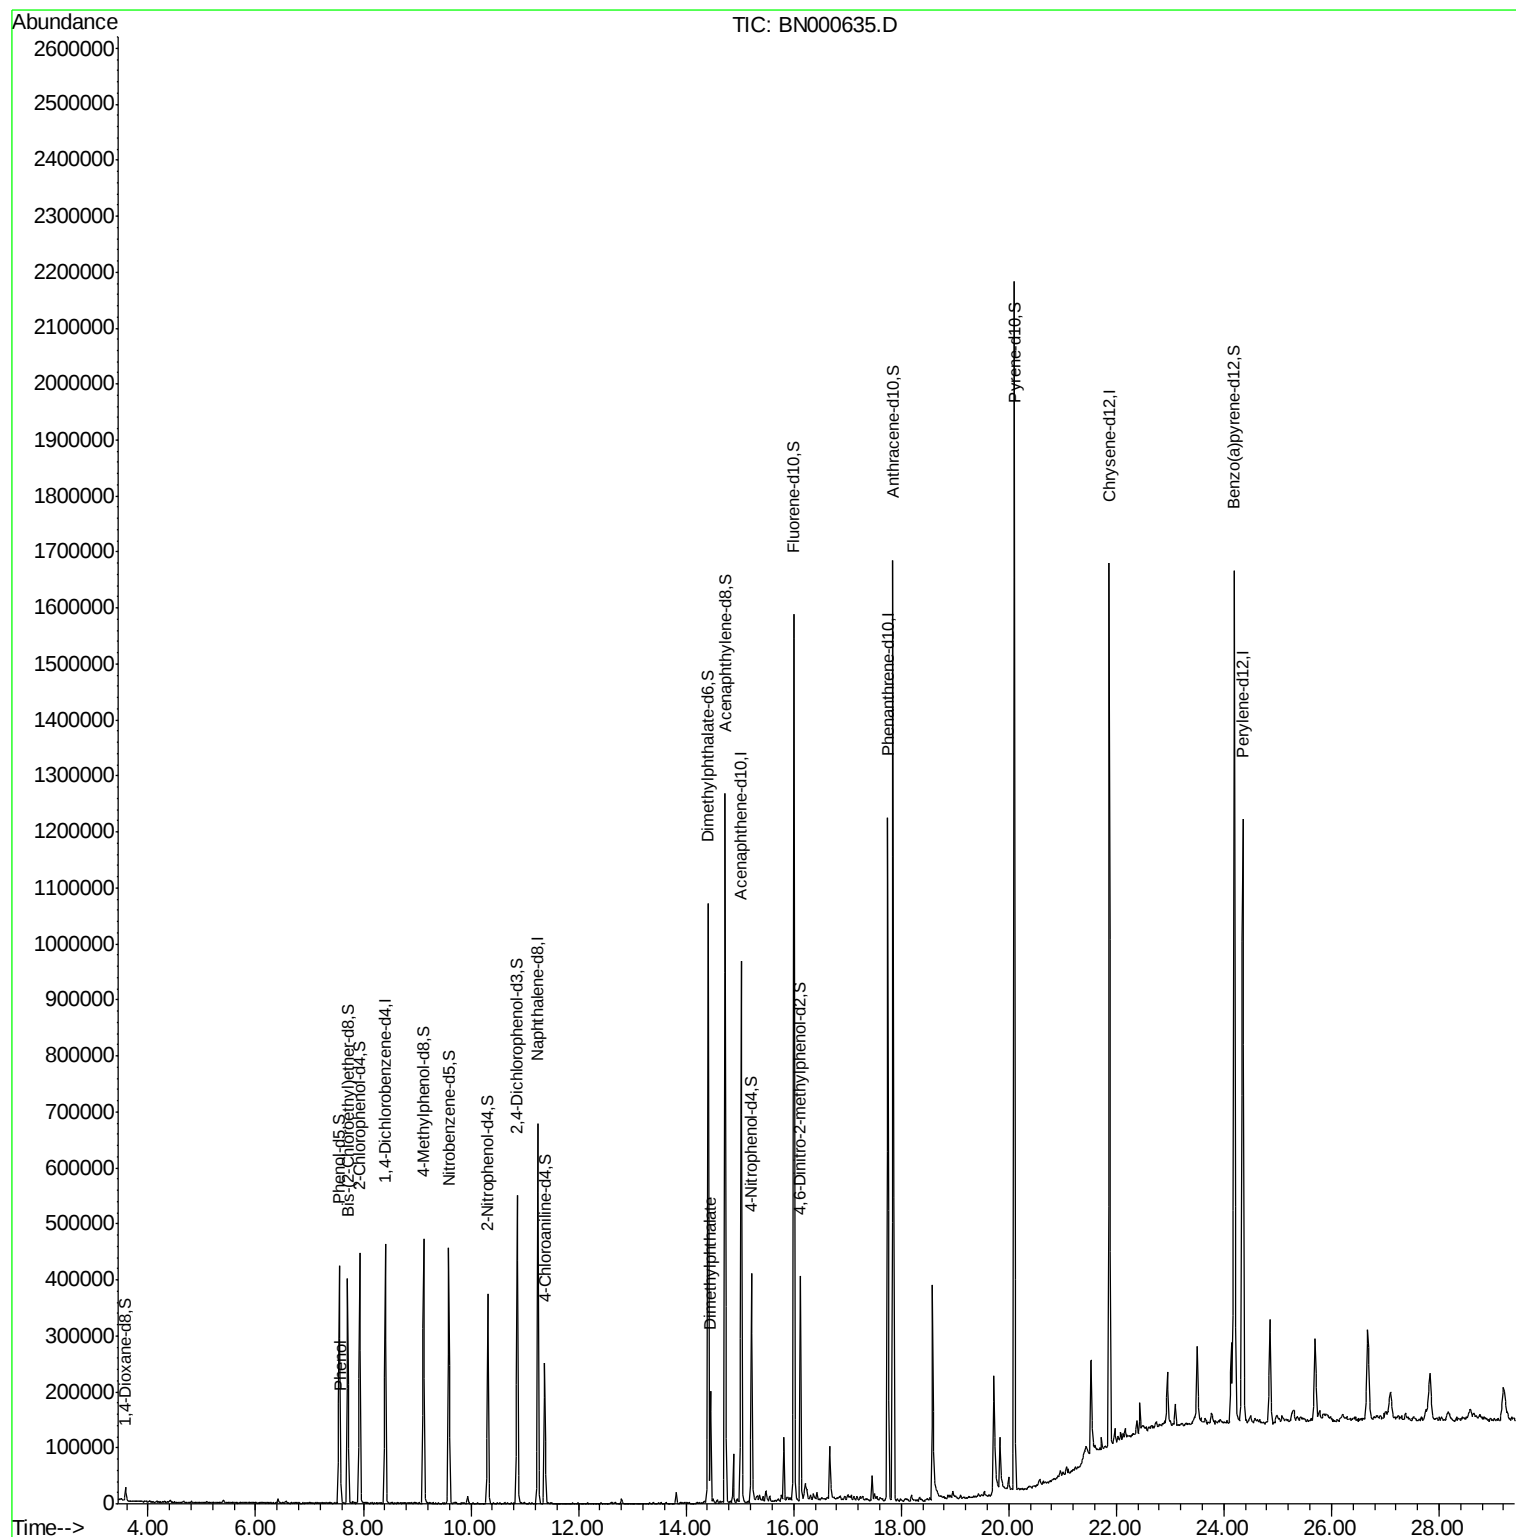

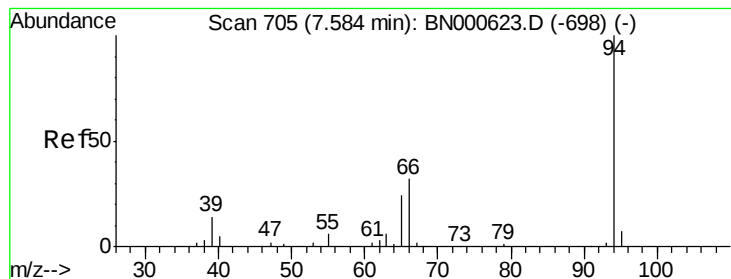





#6

Phenol

Concen: 1.628 ng/ul
 RT: 7.58 min Scan# 704
 Delta R.T. -0.01 min
 Lab File: BN000635.D
 Acq: 26 Mar 2018 23:53

Instrument :
 BNA_N
 ClientSampleId :
 BEEJ1

Tot Ion: 94 Resp: 19336
 Ion Ratio Lower Upper
 94 100
 65 25.7 23.0 34.6
 66 38.7 30.4 45.6

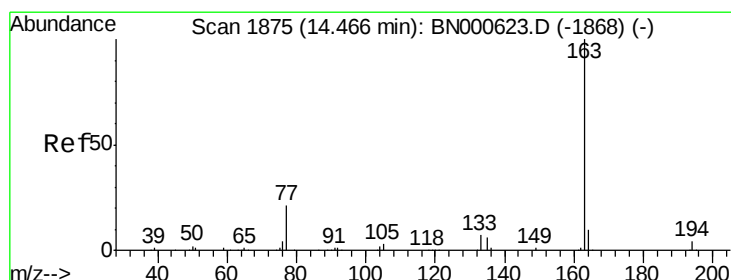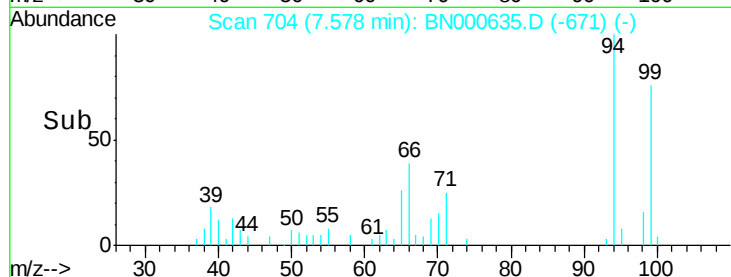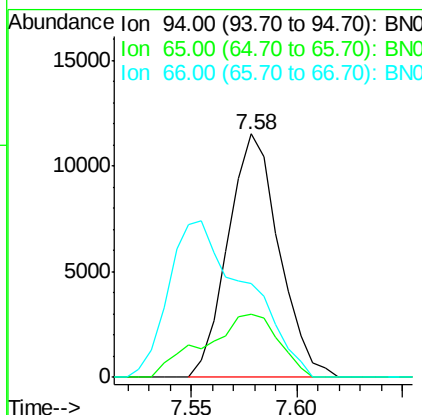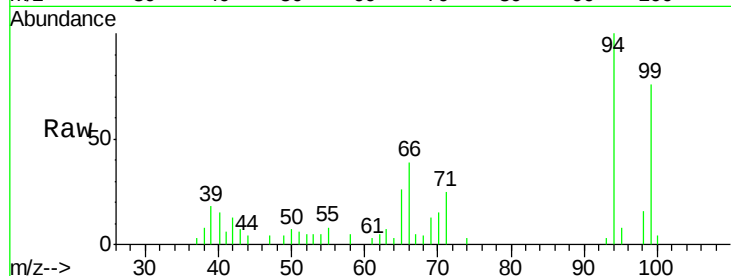

#44

Dimethylphthalate

Concen: 4.540 ng/ul
 RT: 14.46 min Scan# 1874
 Delta R.T. -0.01 min
 Lab File: BN000635.D
 Acq: 26 Mar 2018 23:53

Tgt Ion:163 Resp: 109162
 Ion Ratio Lower Upper
 163 100
 194 3.8 4.0 6.0#
 164 10.1 8.4 12.6

