
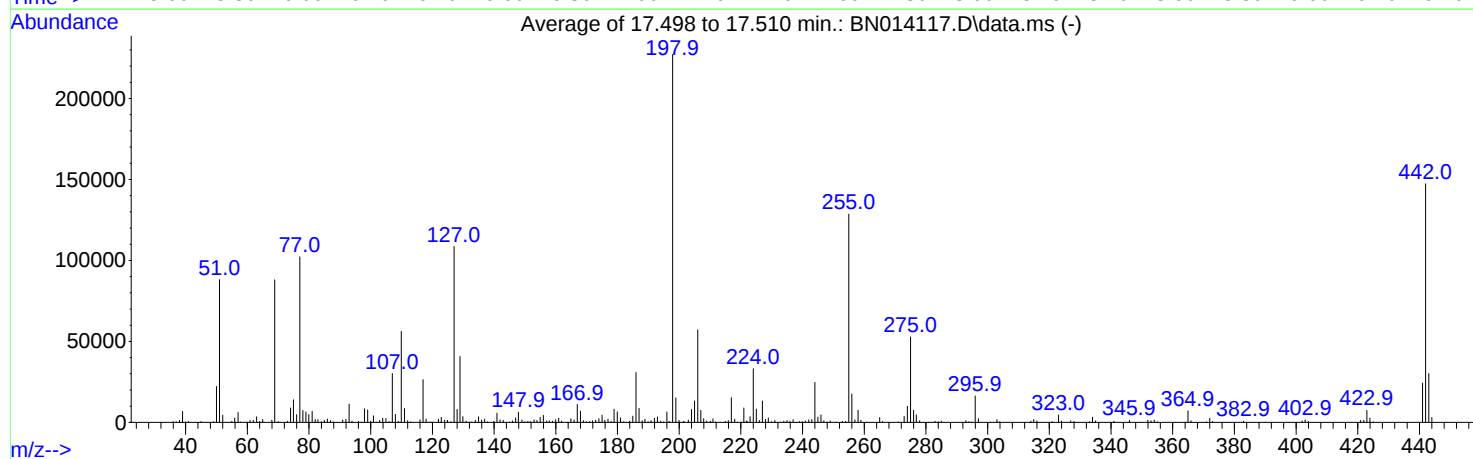


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032621\
 Data File : BN014117.D
 Acq On : 26 Mar 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 26 15:25:59 2021

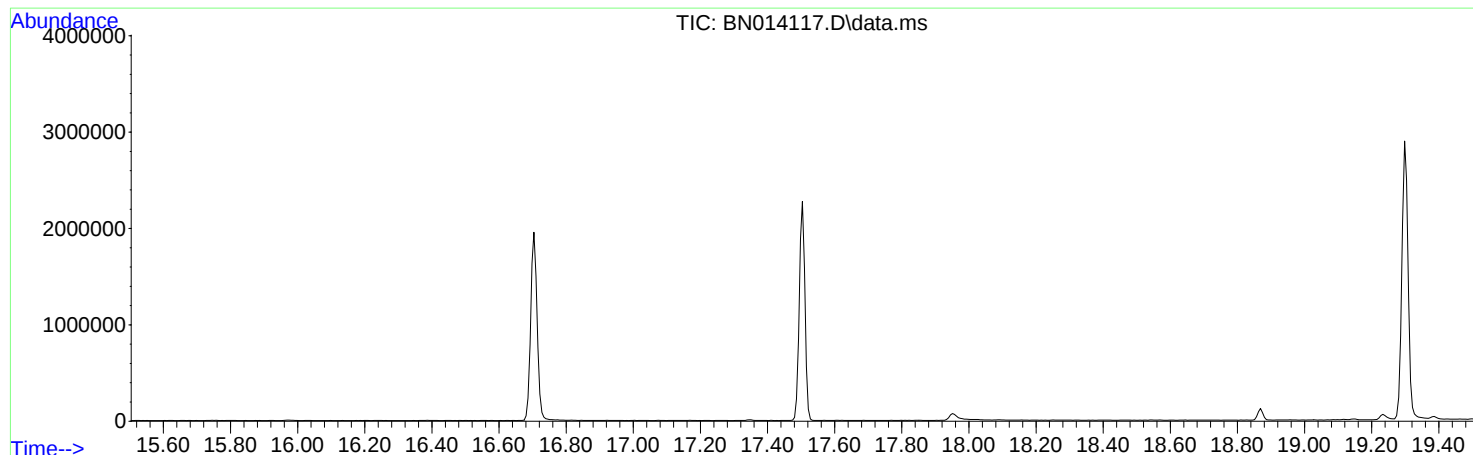




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	88157	PASS
68	69	0.00	2	1.6	1433	PASS
69	198	0.00	100	38.8	88053	PASS
70	69	0.00	2	0.5	480	PASS
127	198	10	80	47.8	108603	PASS
197	198	0.00	2	0.3	724	PASS
198	198	100	100	100.0	227157	PASS
199	198	5	9	6.7	15136	PASS
275	198	10	60	23.2	52744	PASS
365	198	1	100	3.1	7091	PASS
441	198	0.01	100	10.7	24196	PASS
442	442	50	100	100.0	147352	PASS
443	442	15	24	20.5	30163	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032621\
Data File : BN014117.D
Acq On : 26 Mar 2021 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 26 11:51:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

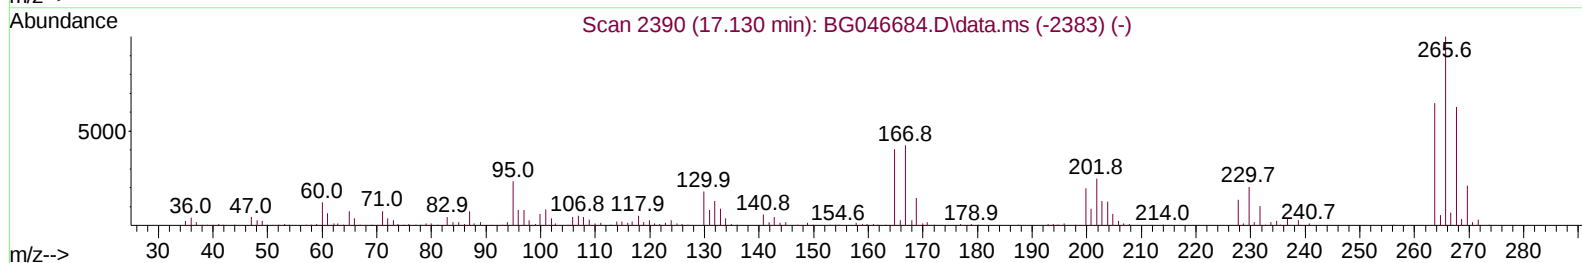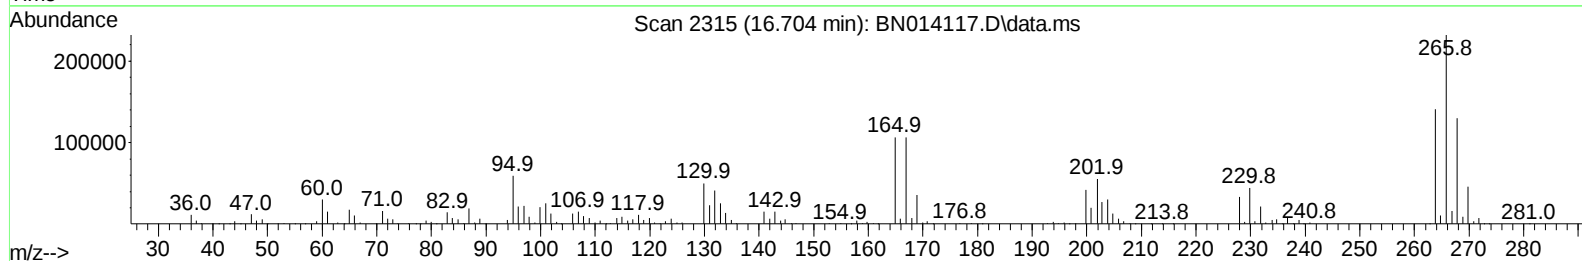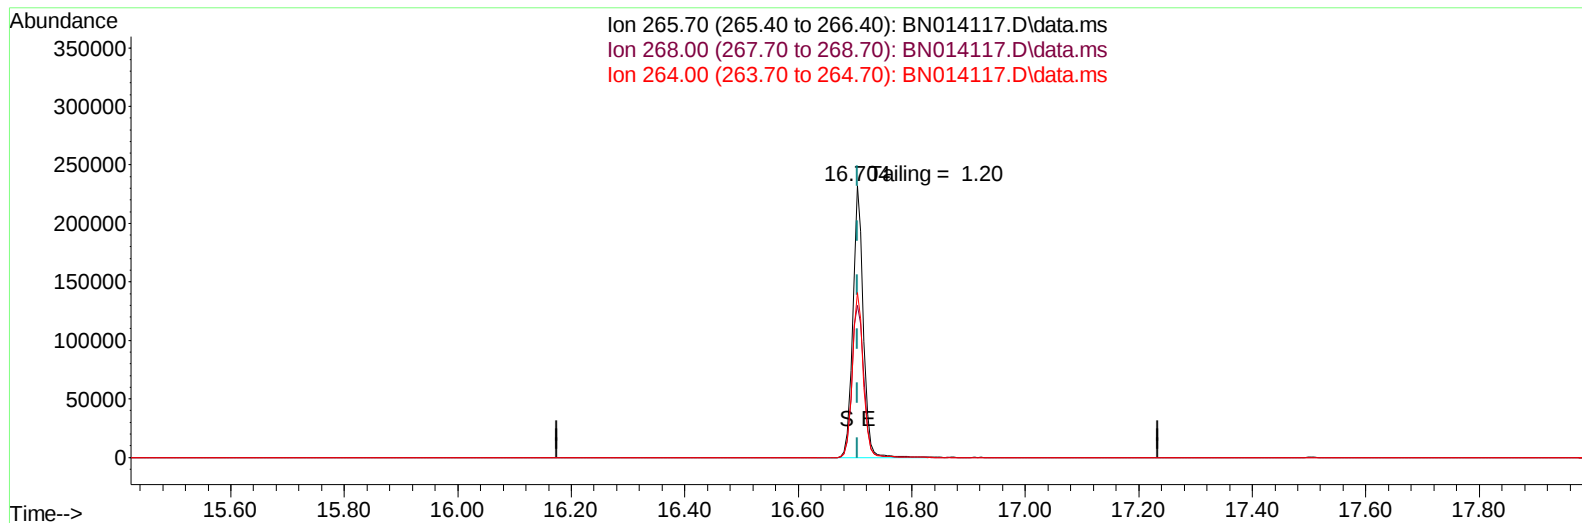

TIC: BN014117.D\data.ms

(70) Pentachlorophenol (C)

16.704min (0.000) 30129.83 ng




response 298638

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.12
264.00	61.60	60.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032621\
Data File : BN014117.D
Acq On : 26 Mar 2021 10:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 26 11:51:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

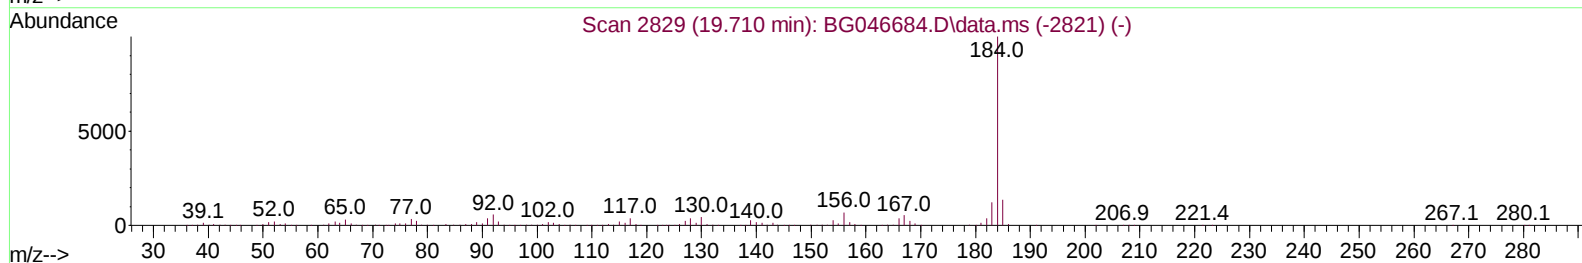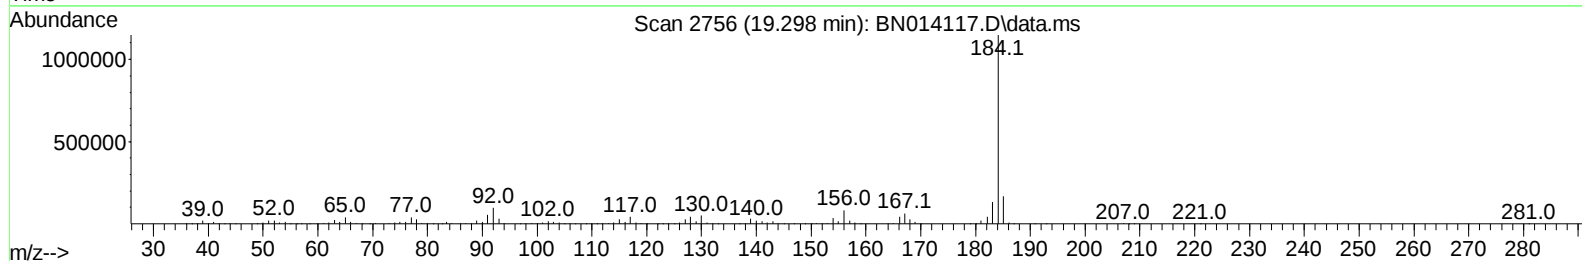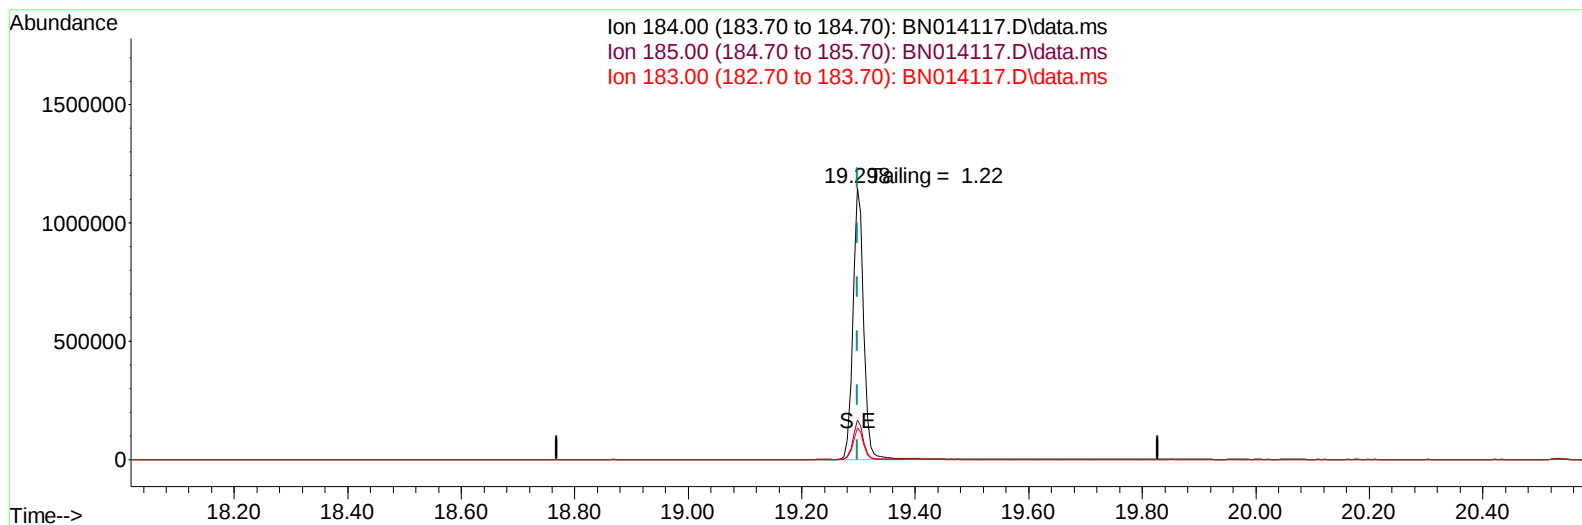

TIC: BN014117.D\data.ms

(77) Benzidine

19.298min (0.000) 0.00 ng

response 1520214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.50
183.00	13.20	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/26/2021	BNA_N	<u>BN014117.D</u>
Compound Name	Response	Retention Time
DDT	819152	20.533
DDD	3298	20.098
DDE	849	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4147	823299	0.50