

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032718\
 Data File : BN000645.D
 Acq On : 27 Mar 2018 14:11
 Operator : JU/SJ
 Sample : J2060-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.584	21	25	35	rVB	48034	73208	1.73%	0.154%
2	3.902	76	79	91	rVB3	3260	8145	0.19%	0.017%
3	5.402	329	334	340	rVB2	7825	12614	0.30%	0.027%
4	6.413	502	506	513	rVB2	6403	11353	0.27%	0.024%
5	6.549	523	529	530	rBV2	3740	5240	0.12%	0.011%
6	6.566	530	532	540	rVB2	5522	7586	0.18%	0.016%
7	7.549	692	699	712	rBV	737426	1284306	30.29%	2.701%
8	7.713	720	727	735	rBV	695307	1071233	25.27%	2.253%
9	7.931	757	764	774	rBV	798331	1291075	30.45%	2.715%
10	8.407	838	845	856	rVB	610541	1004053	23.68%	2.111%
11	9.119	959	966	975	rBV	998171	1642048	38.73%	3.453%
12	9.590	1038	1046	1056	rBV	764205	1261599	29.75%	2.653%
13	9.684	1056	1062	1066	rBV4	3588	6854	0.16%	0.014%
14	9.943	1099	1106	1114	rVB	21323	32268	0.76%	0.068%
15	10.319	1163	1170	1178	rBV	638823	1055551	24.90%	2.220%
16	10.866	1255	1263	1277	rBV	917027	1585588	37.40%	3.334%
17	11.249	1320	1328	1335	rBV	858566	1480311	34.91%	3.113%
18	11.378	1341	1350	1360	rBV	921468	1633589	38.53%	3.435%
19	12.678	1568	1571	1577	rVB2	4116	5819	0.14%	0.012%
20	12.807	1588	1593	1598	rBV	14581	21139	0.50%	0.044%
21	13.395	1686	1693	1699	rVB3	2915	6423	0.15%	0.014%
22	13.537	1712	1717	1722	rVB2	3928	5730	0.14%	0.012%
23	13.625	1727	1732	1734	rBV3	3519	5043	0.12%	0.011%
24	13.819	1759	1765	1773	rVB	33566	47313	1.12%	0.099%
25	13.895	1773	1778	1785	rBV4	3919	9990	0.24%	0.021%
26	14.213	1826	1832	1836	rBV4	2870	5385	0.13%	0.011%
27	14.337	1848	1853	1857	rBV5	4279	7865	0.19%	0.017%
28	14.413	1860	1866	1871	rVV	1668402	2476683	58.41%	5.208%
29	14.460	1871	1874	1879	rVV	329785	436485	10.29%	0.918%
30	14.507	1879	1882	1888	rVB3	11710	18655	0.44%	0.039%
31	14.584	1888	1895	1899	rVB	8850	11731	0.28%	0.025%
32	14.725	1913	1919	1931	rBV	1985170	3043295	71.78%	6.399%
33	14.878	1939	1945	1953	rVB	101034	130270	3.07%	0.274%
34	14.948	1953	1957	1961	rVV5	7122	11410	0.27%	0.024%

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032718\
 Data File : BN000645.D
 Acq On : 27 Mar 2018 14:11
 Operator : JU/SJ
 Sample : J2060-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION

35	15.031	1964	1971	1978	rVV2	1255773	1982189	46.75%	4.168%
36	15.089	1978	1981	1985	rVB2	3816	5482	0.13%	0.012%
37	15.219	1997	2003	2016	rBV	487958	878641	20.72%	1.848%
38	15.313	2016	2019	2025	rVV5	17283	39781	0.94%	0.084%
39	15.372	2025	2029	2034	rVV	15089	25036	0.59%	0.053%
40	15.425	2034	2038	2043	rVV2	12844	20312	0.48%	0.043%
41	15.484	2044	2048	2055	rVV3	20799	39684	0.94%	0.083%
42	15.560	2057	2061	2067	rVB2	10760	14843	0.35%	0.031%
43	15.707	2081	2086	2093	rBV5	4434	10030	0.24%	0.021%
44	15.778	2093	2098	2101	rBV	19857	29490	0.70%	0.062%
45	15.819	2101	2105	2110	rVB	126396	153754	3.63%	0.323%
46	15.878	2110	2115	2119	rBV3	7146	11651	0.27%	0.024%
47	15.925	2121	2123	2131	rVB6	5842	10558	0.25%	0.022%
48	16.007	2131	2137	2145	rBV	2443927	3589321	84.65%	7.548%
49	16.125	2151	2157	2166	rBV	629371	909204	21.44%	1.912%
50	16.219	2166	2173	2175	rVV	31988	66176	1.56%	0.139%
51	16.248	2175	2178	2183	rVB	31204	44646	1.05%	0.094%
52	16.313	2186	2189	2195	rVB4	9946	13187	0.31%	0.028%
53	16.366	2195	2198	2201	rBV2	11914	15222	0.36%	0.032%
54	16.436	2206	2210	2217	rVB2	15252	20556	0.48%	0.043%
55	16.672	2245	2250	2261	rBV	109985	174407	4.11%	0.367%
56	16.860	2279	2282	2288	rVB2	4326	7289	0.17%	0.015%
57	16.948	2292	2297	2300	rVB3	6917	10042	0.24%	0.021%
58	17.007	2304	2307	2311	rBV2	8855	14791	0.35%	0.031%
59	17.072	2315	2318	2322	rVB3	8881	11086	0.26%	0.023%
60	17.131	2324	2328	2331	rBV3	5520	7475	0.18%	0.016%
61	17.178	2332	2336	2339	rBV2	6743	7411	0.17%	0.016%
62	17.242	2344	2347	2350	rVB3	7061	8227	0.19%	0.017%
63	17.283	2350	2354	2359	rBV5	5035	6749	0.16%	0.014%
64	17.454	2378	2383	2387	rBV	59438	73823	1.74%	0.155%
65	17.507	2387	2392	2396	rVV2	16147	27641	0.65%	0.058%
66	17.542	2396	2398	2403	rVV	9121	10123	0.24%	0.021%
67	17.613	2405	2410	2414	rBV6	3661	6578	0.16%	0.014%
68	17.754	2427	2434	2440	rBV	1630322	2319206	54.70%	4.877%
69	17.854	2444	2451	2460	rVV	2636661	3825175	90.22%	8.044%
70	17.925	2460	2463	2469	rVB6	5188	6765	0.16%	0.014%
71	17.989	2471	2474	2479	rVB5	4177	6256	0.15%	0.013%

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032718\
Data File : BN000645.D
Acq On : 27 Mar 2018 14:11
Operator : JU/SJ
Sample : J2060-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Title : SVOA CALIBRATION

72	18.189	2504	2508	2513	rBV	27602	33504	0.79%	0.070%
73	18.360	2536	2537	2544	rVB3	4873	6484	0.15%	0.014%
74	18.601	2572	2578	2587	rBV5	26152	76348	1.80%	0.161%
75	18.872	2620	2624	2627	rBV2	5481	7995	0.19%	0.017%
76	18.913	2627	2631	2636	rVB2	5245	6873	0.16%	0.014%
77	19.348	2700	2705	2709	rBV3	7277	11063	0.26%	0.023%
78	19.483	2725	2728	2732	rBV5	4434	6348	0.15%	0.013%
79	19.742	2768	2772	2776	rBV	31662	39687	0.94%	0.083%
80	19.854	2787	2791	2792	rBV2	5996	6774	0.16%	0.014%
81	19.995	2811	2815	2820	rVB	31211	39898	0.94%	0.084%
82	20.107	2828	2834	2847	rBV2	3058290	4239969	100.00%	8.916%
83	20.966	2974	2980	2985	rBV	150196	196019	4.62%	0.412%
84	21.877	3129	3135	3145	rBV	1734258	2417706	57.02%	5.084%
85	22.442	3228	3231	3235	rBV2	25006	27476	0.65%	0.058%
86	22.948	3313	3317	3322	rVB	59293	86345	2.04%	0.182%
87	23.095	3338	3342	3347	rBV	52307	75923	1.79%	0.160%
88	23.507	3409	3412	3417	rVB2	82053	125246	2.95%	0.263%
89	24.136	3514	3519	3522	rBV	104313	180606	4.26%	0.380%
90	24.195	3522	3529	3541	rVB2	1638098	3425564	80.79%	7.203%
91	24.354	3548	3556	3567	rVB2	1011833	2037037	48.04%	4.283%
92	24.860	3637	3642	3650	rVB	103607	199122	4.70%	0.419%
93	25.695	3780	3784	3792	rVB2	91349	197170	4.65%	0.415%


Sum of corrected areas: 47555821

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN032718\
Data File : BN000645.D
Acq On : 27 Mar 2018 14:11
Operator : JU/SJ
Sample : J2060-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

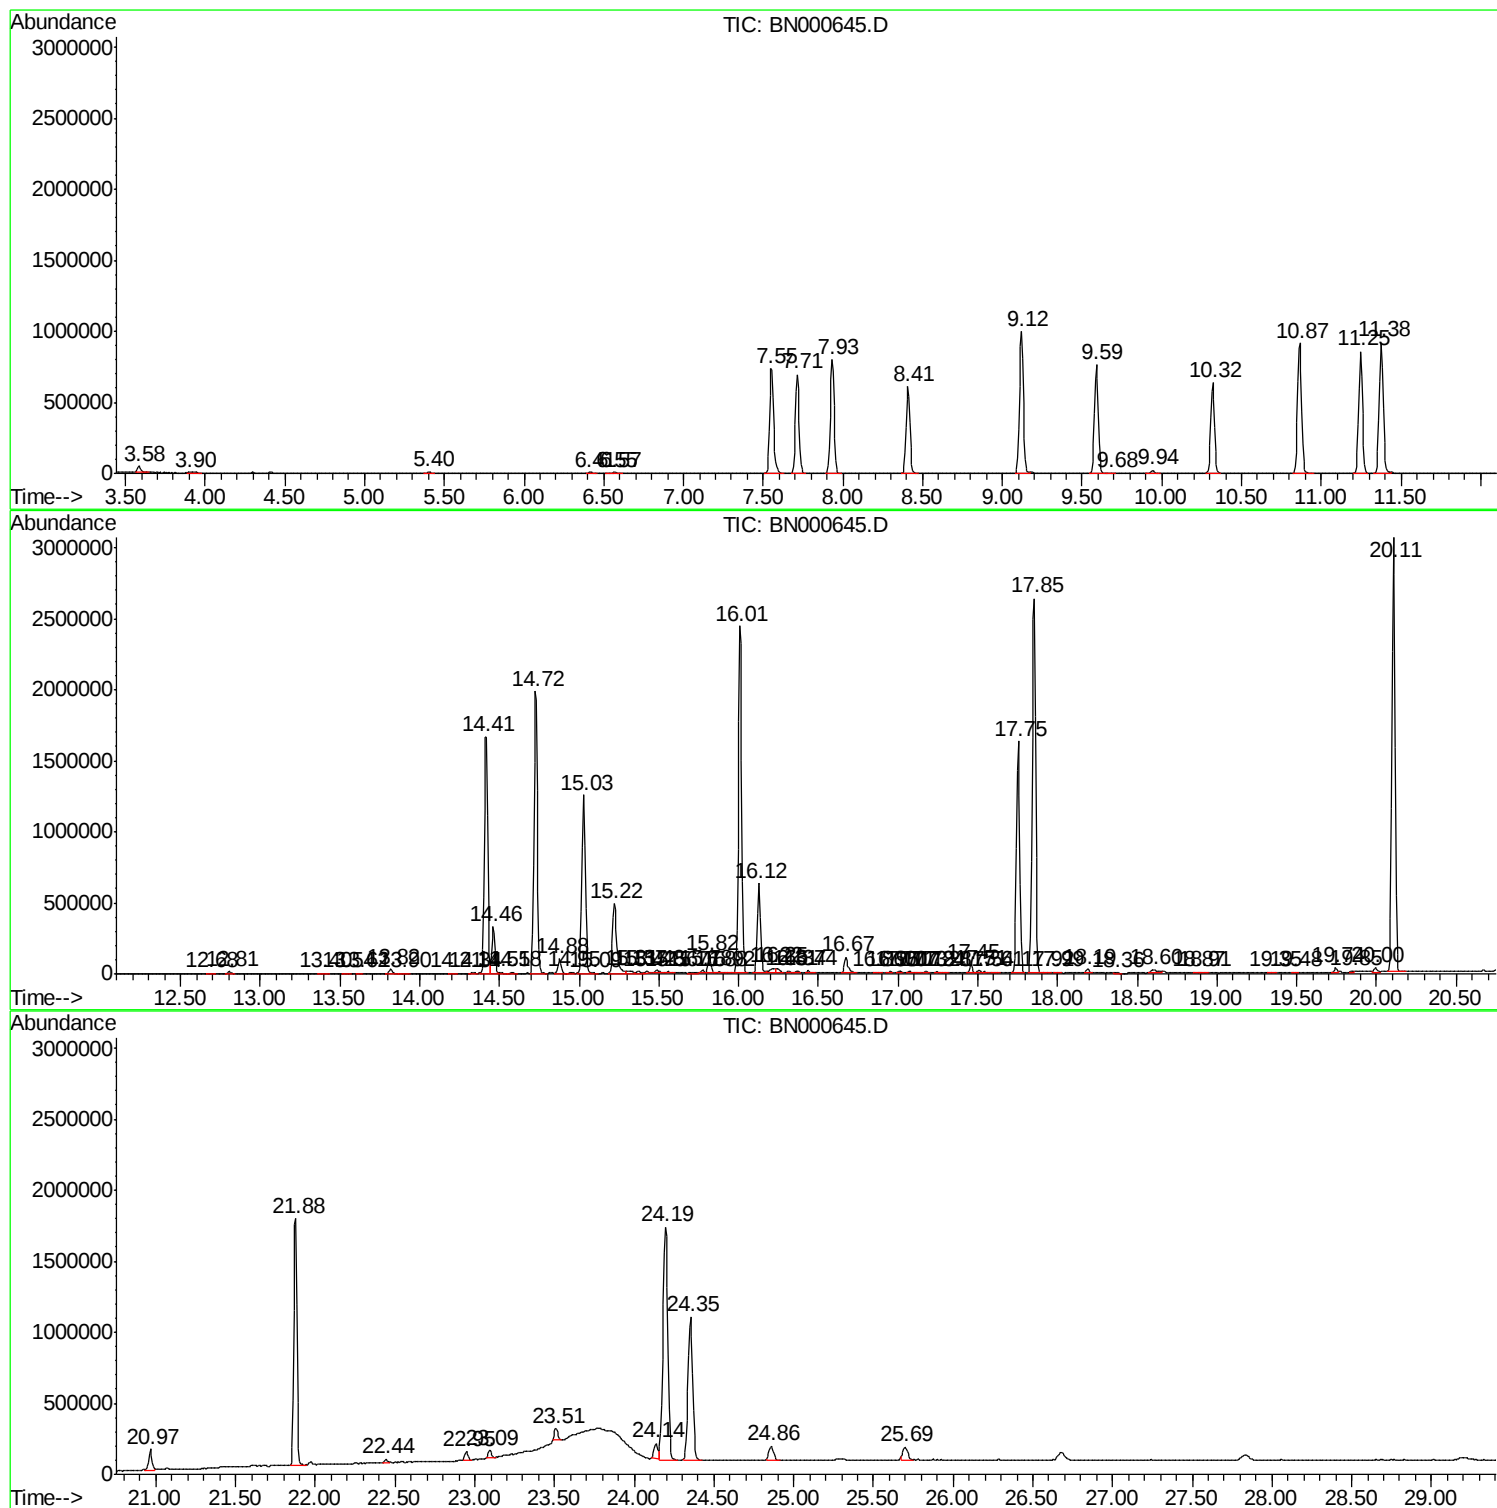

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN032718\
Data File : BN000645.D
Acq On : 27 Mar 2018 14:11
Operator : JU/SJ
Sample : J2060-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN032718\
Data File : BN000645.D
Acq On : 27 Mar 2018 14:11
Operator : JU/SJ
Sample : J2060-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT3

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc