
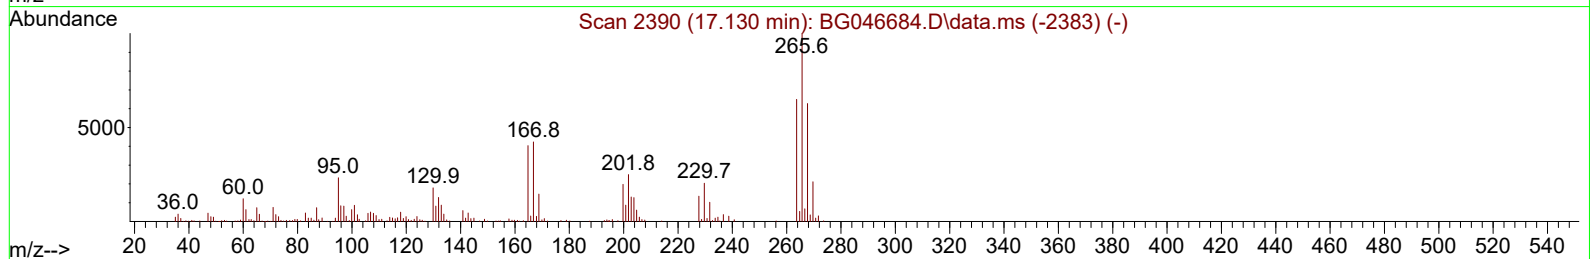
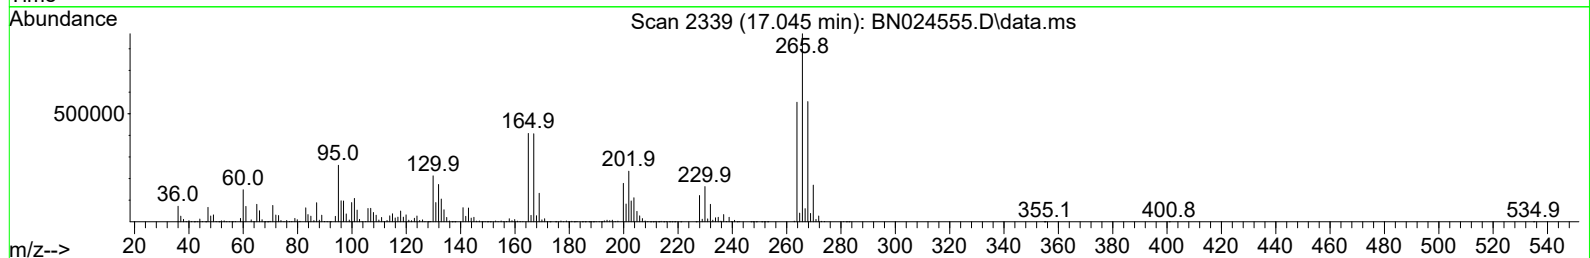


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032723\
Data File : BN024555.D
Acq On : 27 Mar 2023 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 02:59:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 02:59:08 2023
Response via : Initial Calibration

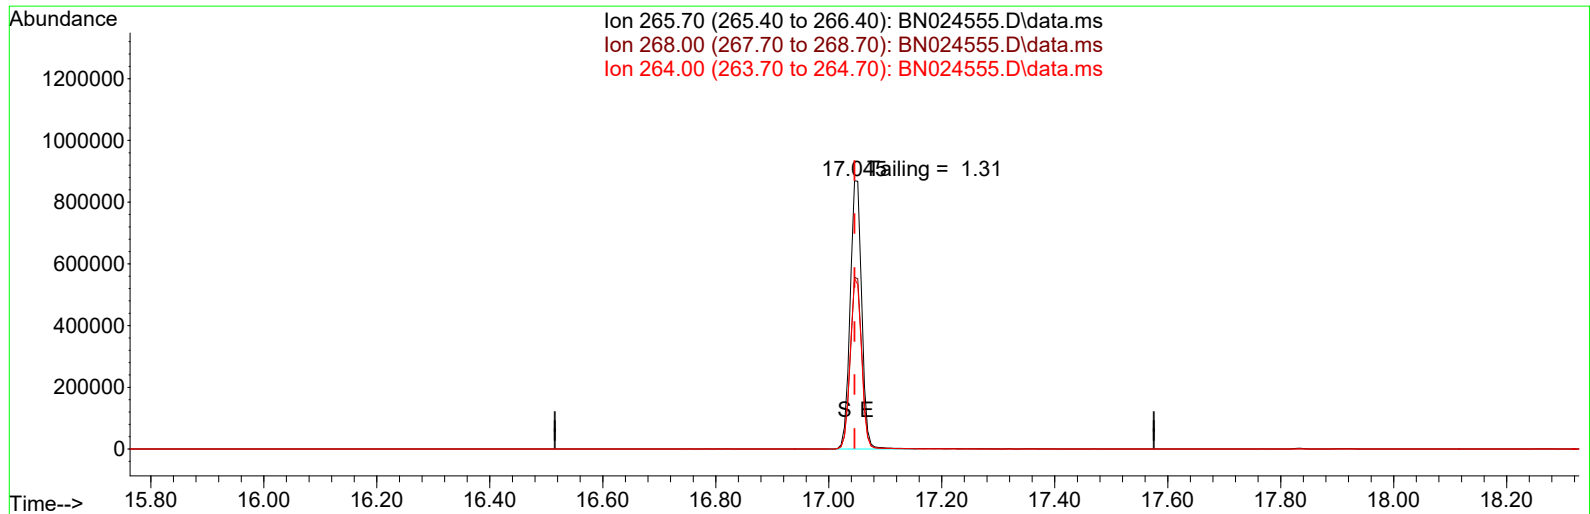

TIC: BN024555.D\data.ms

(70) Pentachlorophenol (C)




17.045min (0.000) 24044.45 ng

response 1244631

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.95
264.00	61.60	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032723\
Data File : BN024555.D
Acq On : 27 Mar 2023 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 02:59:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 02:59:08 2023
Response via : Initial Calibration

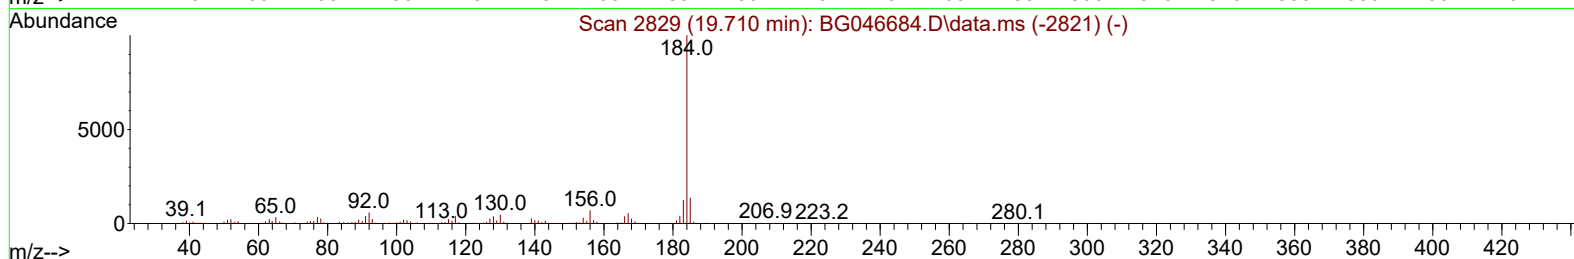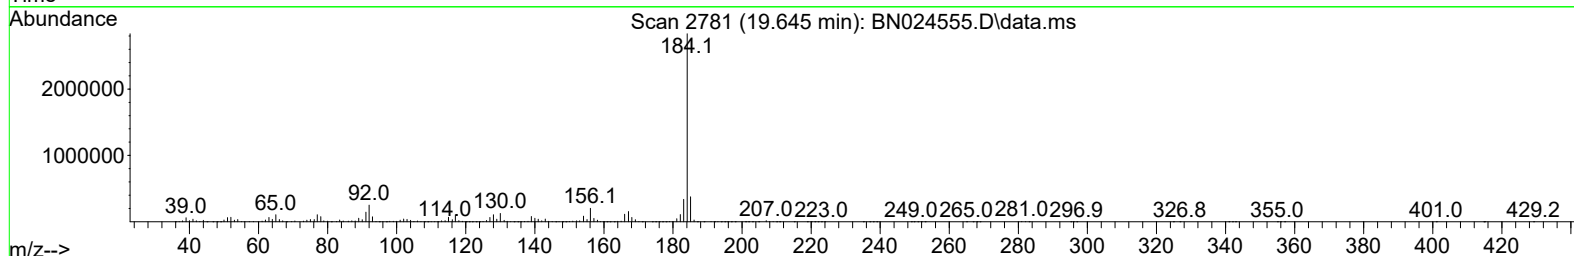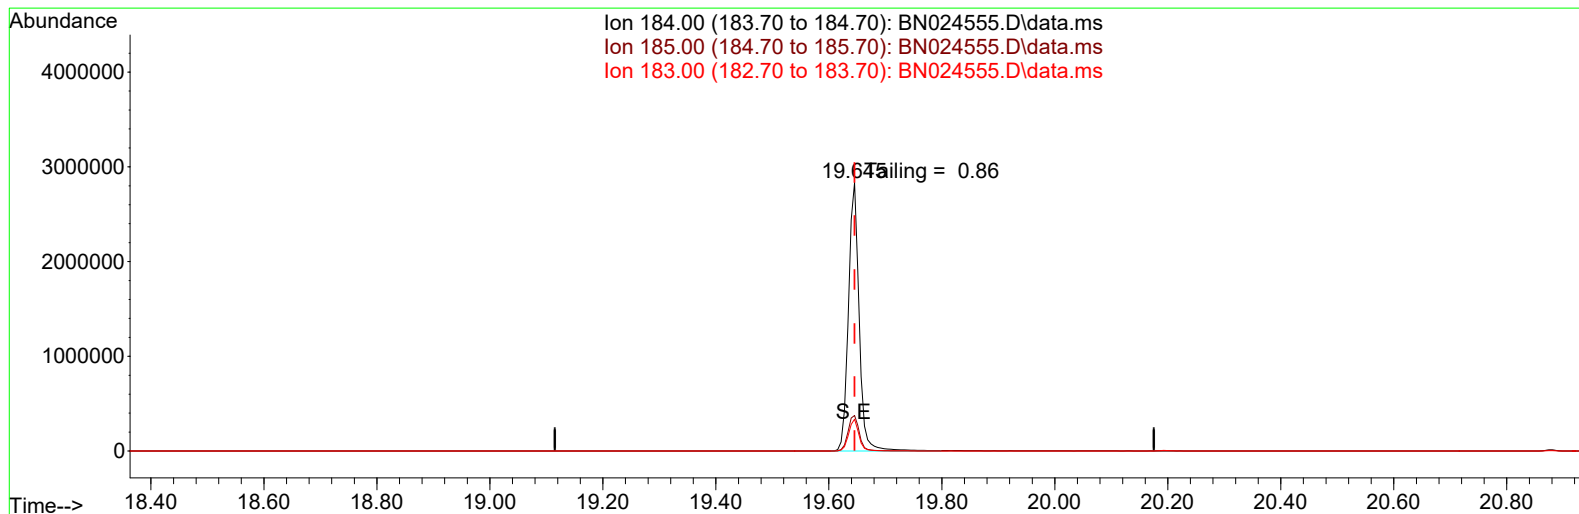

TIC: BN024555.D\data.ms

(77) Benzidine**19.645min (0.000) 1954151.15 ng****response 3734721**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.28
183.00	13.20	11.90
0.00	0.00	0.00