
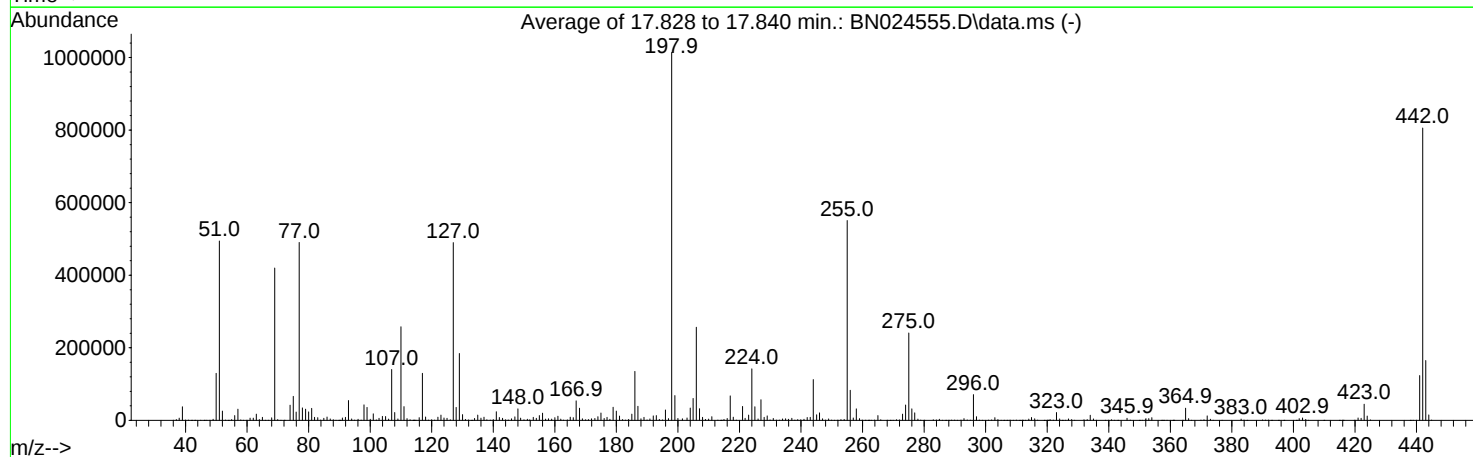


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032723\  
Data File : BN024555.D  
Acq On : 27 Mar 2023 09:39  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN031323.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Mar 25 00:22:43 2023

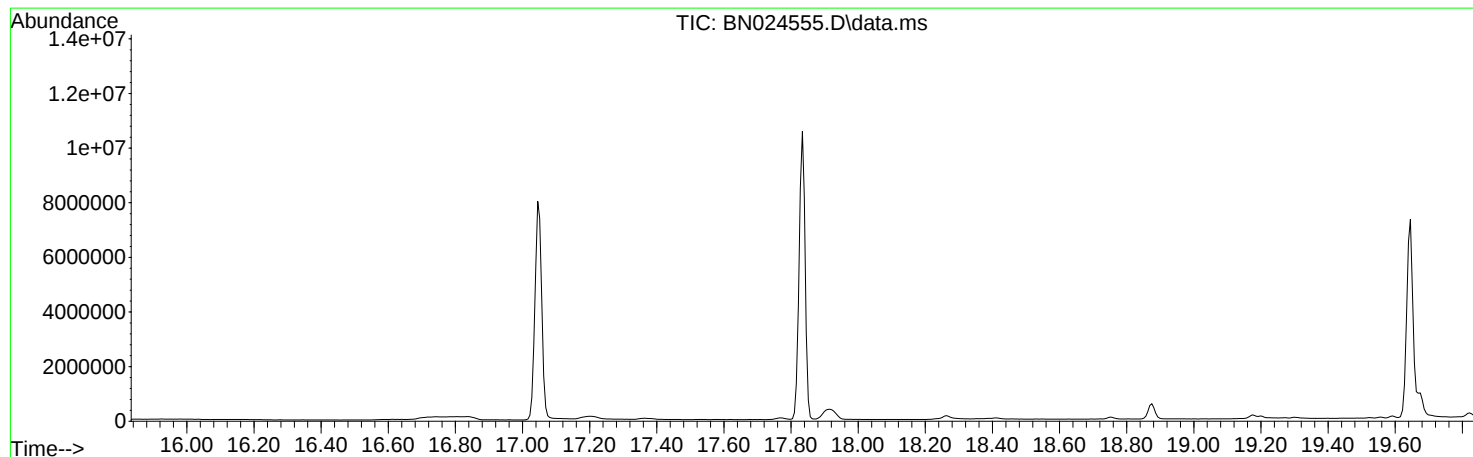




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw     | Result    |
|--------|---------|--------|--------|-------|---------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn     | Pass/Fail |
| 51     | 198     | 10     | 80     | 48.8  | 494565  | PASS      |
| 68     | 69      | 0.00   | 2      | 1.6   | 6915    | PASS      |
| 69     | 198     | 0.00   | 100    | 41.4  | 419833  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 2185    | PASS      |
| 127    | 198     | 10     | 80     | 48.3  | 489800  | PASS      |
| 197    | 198     | 0.00   | 2      | 0.5   | 5101    | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 1013824 | PASS      |
| 199    | 198     | 5      | 9      | 6.8   | 68472   | PASS      |
| 275    | 198     | 10     | 60     | 23.8  | 240896  | PASS      |
| 365    | 198     | 1      | 100    | 3.3   | 33744   | PASS      |
| 441    | 198     | 0.01   | 100    | 12.2  | 123432  | PASS      |
| 442    | 442     | 50     | 100    | 100.0 | 805824  | PASS      |
| 443    | 442     | 15     | 24     | 20.5  | 164869  | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032723\  
 Data File : BN024555.D  
 Acq On : 27 Mar 2023 09:39  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 28 02:59:12 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Mar 28 02:59:08 2023  
 Response via : Initial Calibration

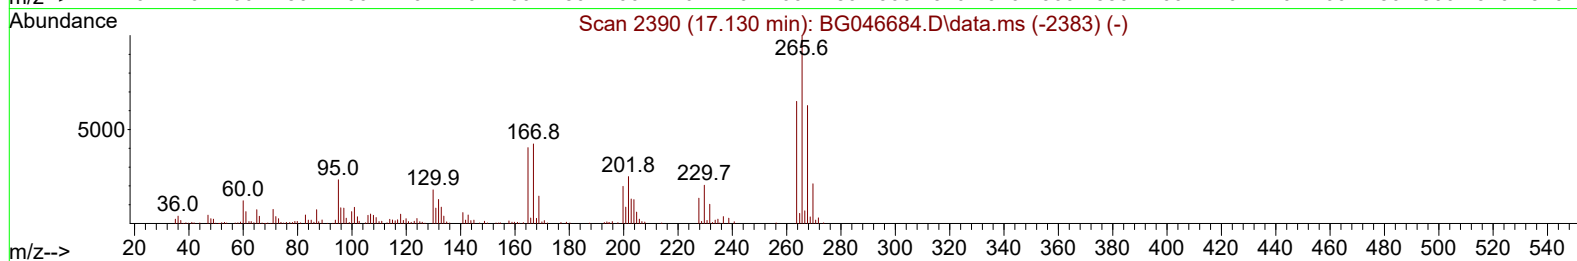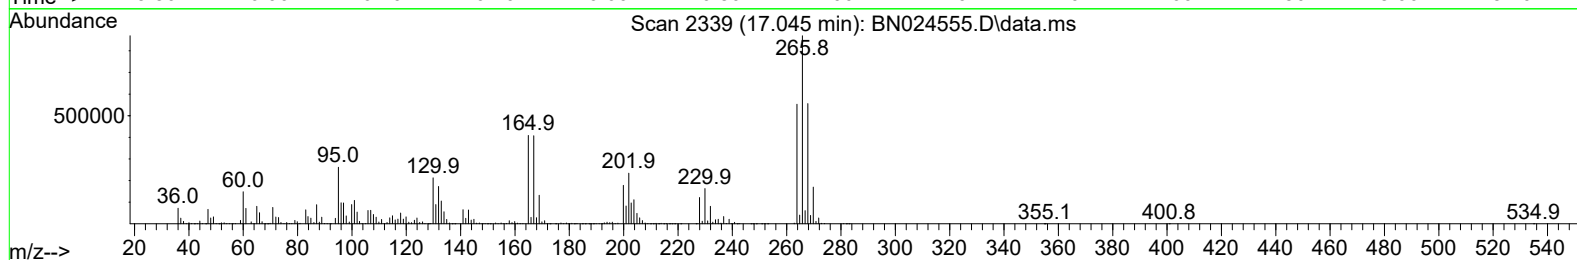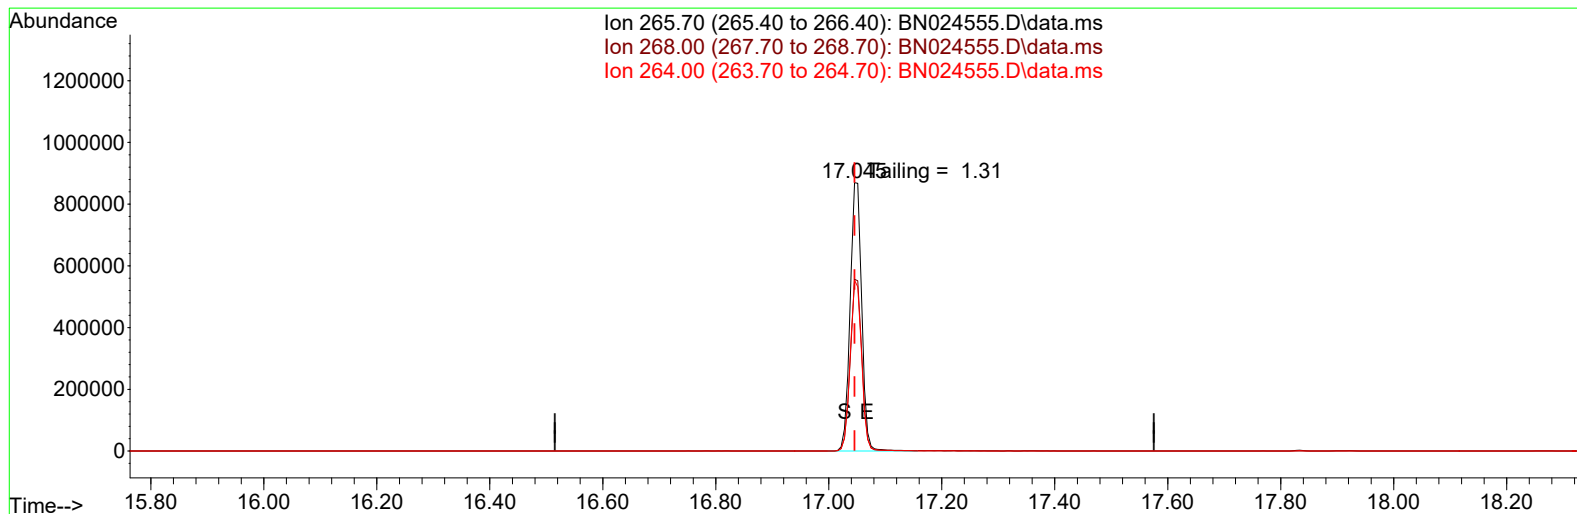

TIC: BN024555.D\data.ms

**(70) Pentachlorophenol (C)**

17.045min ( 0.000) 24044.45 ng




response 1244631

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.95  |
| 264.00 | 61.60  | 63.60  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN032723\  
Data File : BN024555.D  
Acq On : 27 Mar 2023 09:39  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Mar 28 02:59:12 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 28 02:59:08 2023  
Response via : Initial Calibration

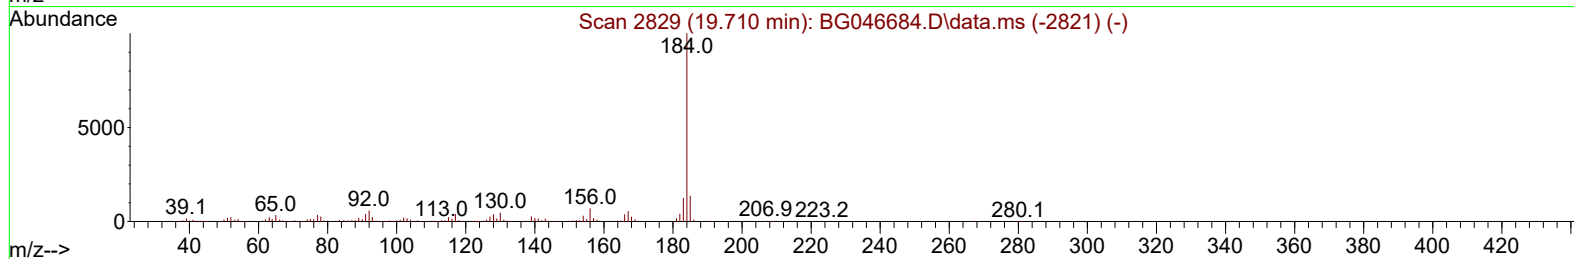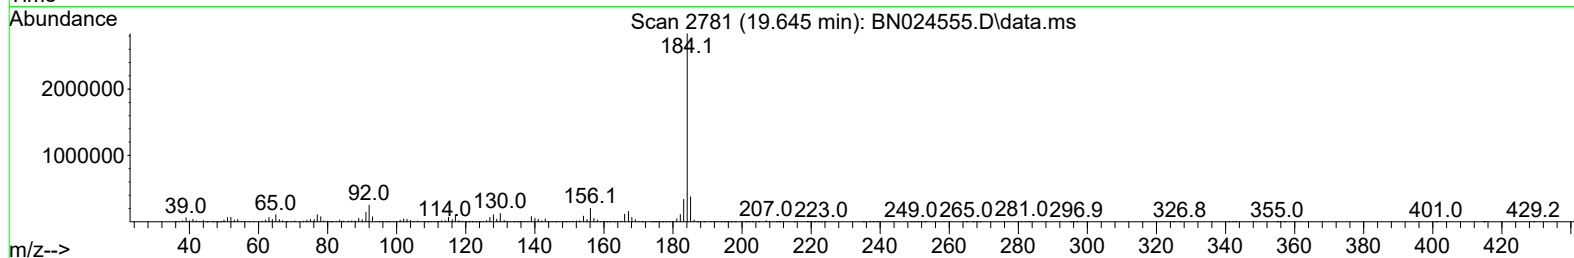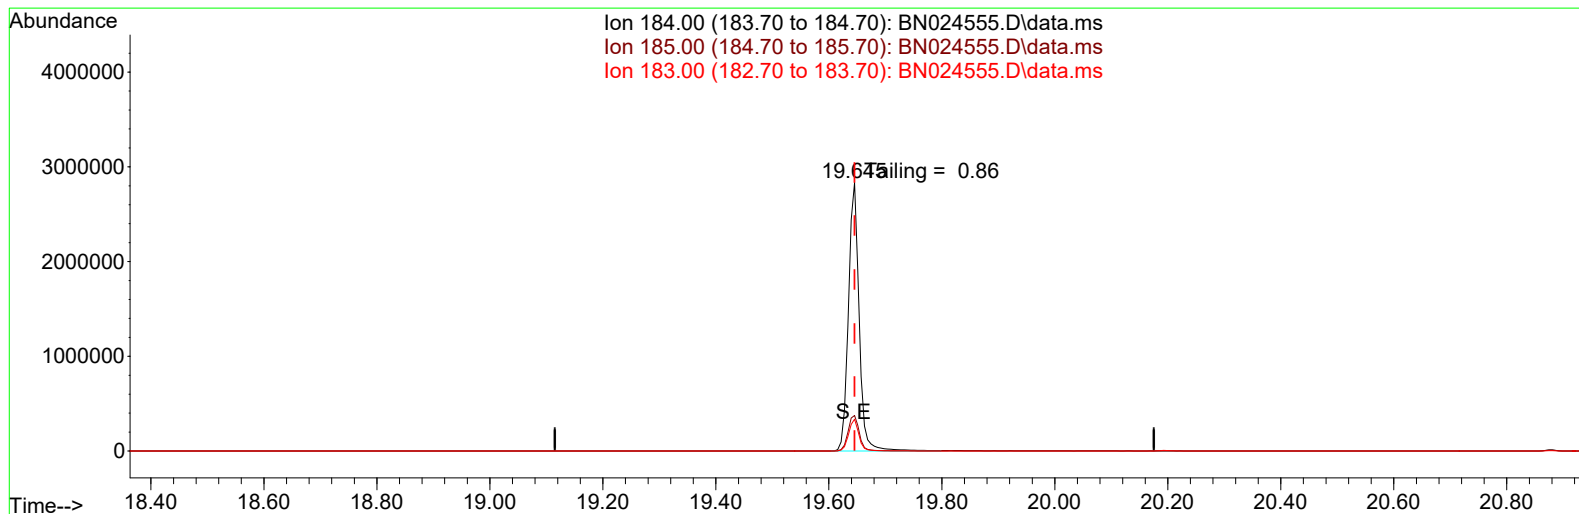

TIC: BN024555.D\data.ms

**(77) Benzidine****19.645min ( 0.000) 1954151.15 ng****response 3734721**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.28  |
| 183.00 | 13.20  | 11.90  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/27/2023     | BNA_N            | <u>BN024555.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 3142083          | 20.881             |
| DDD           | 146242           | 20.433             |
| DDE           | 22529            | 19.928             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 168771        | 3310854          | 5.10               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP