
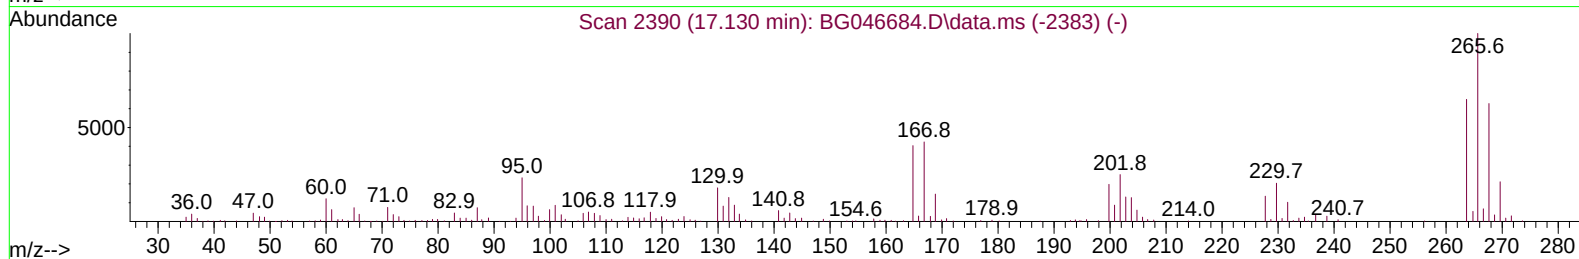
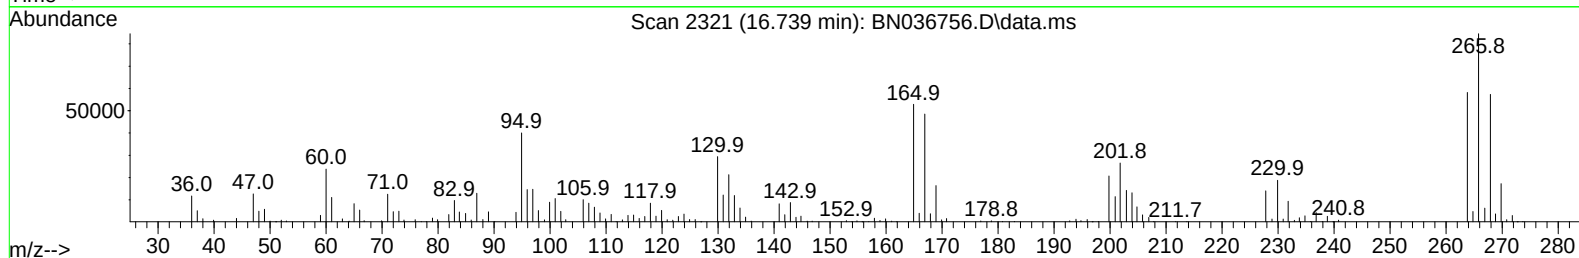


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036756.D
Acq On : 28 Mar 2025 03:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 28 05:40:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 28 05:40:24 2025
Response via : Initial Calibration

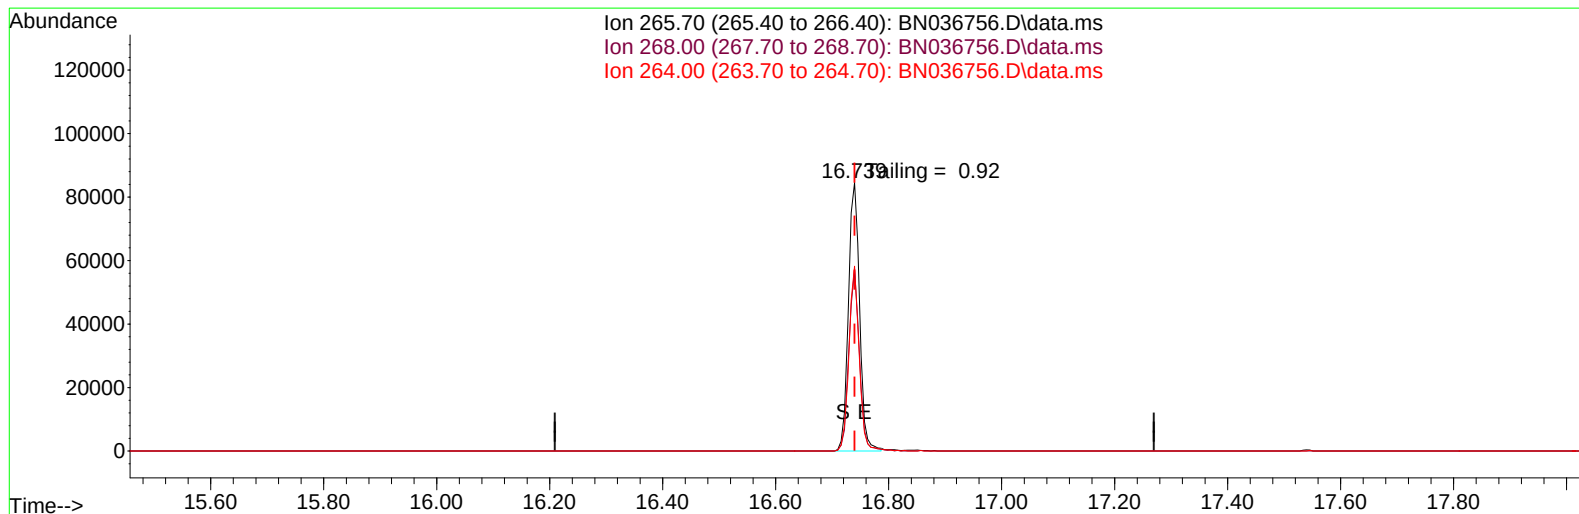

TIC: BN036756.D\data.ms

(70) Pentachlorophenol (C)




16.739min (0.000) 15913.57 ng

response 116893

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.77
264.00	61.60	68.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036756.D
Acq On : 28 Mar 2025 03:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 28 05:40:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 28 05:40:24 2025
Response via : Initial Calibration

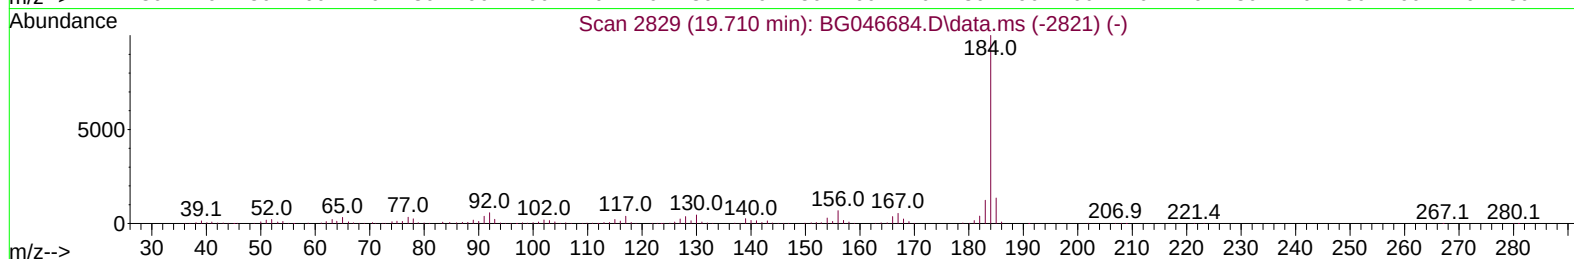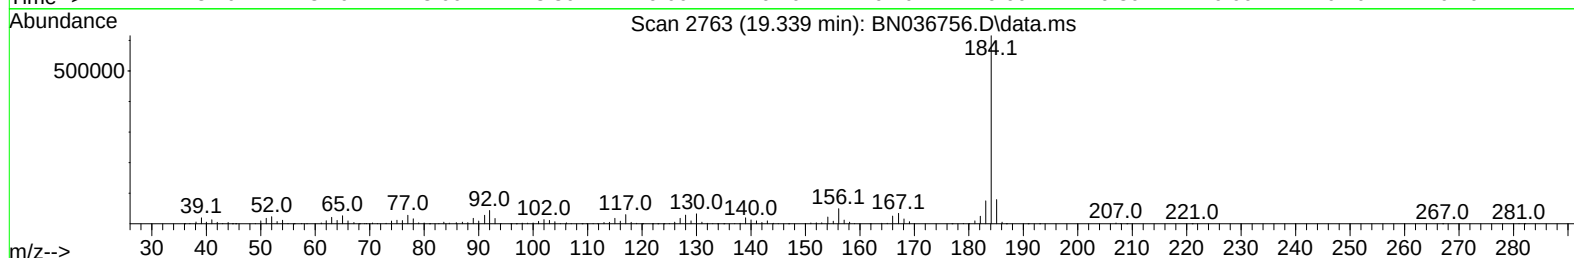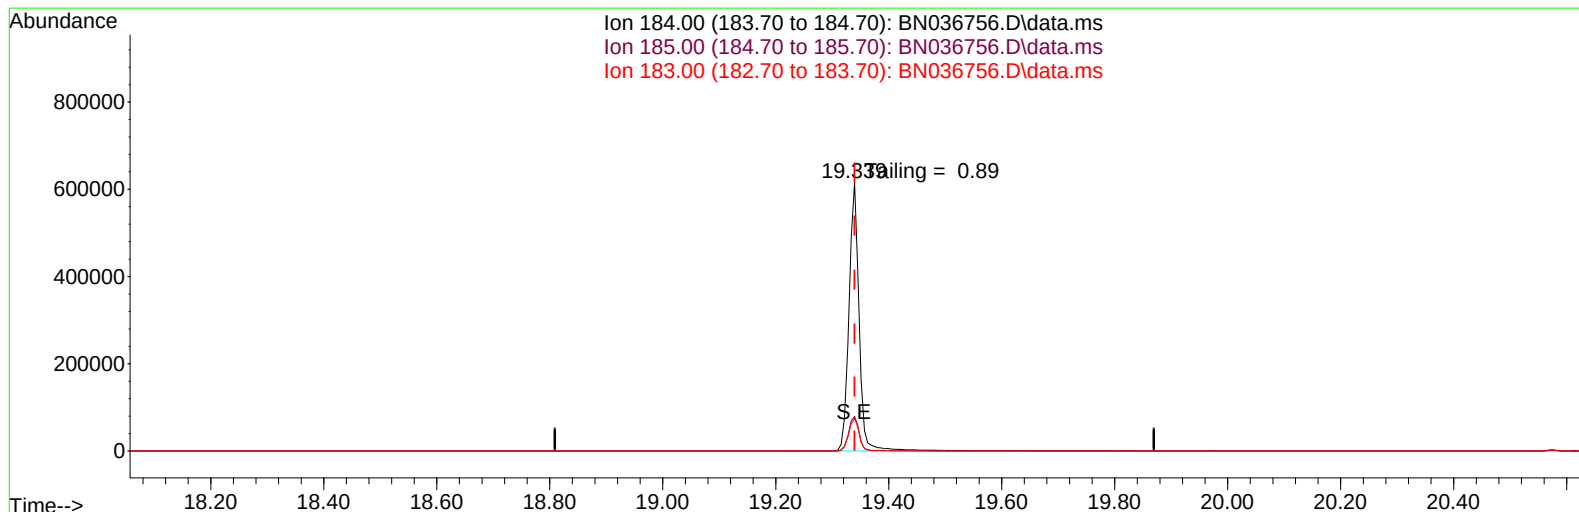

TIC: BN036756.D\data.ms

(77) Benzidine

19.339min (0.000) 0.00 ng

response 762967

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.92
183.00	13.20	12.18
0.00	0.00	0.00