


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036728.D
Acq On : 27 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

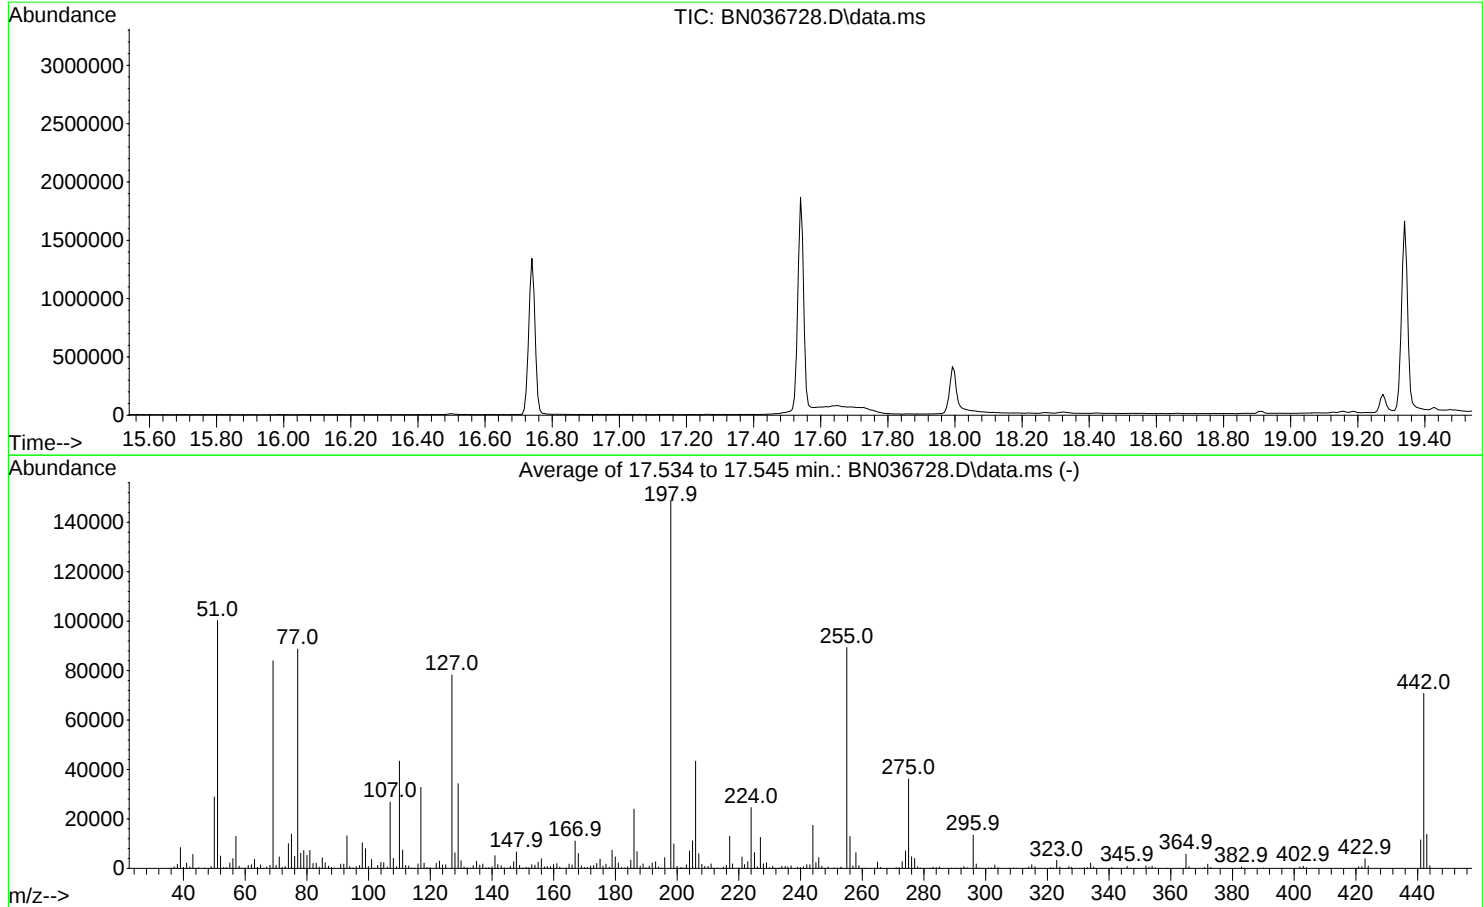




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.4	100301	PASS
68	69	0.00	2	1.4	1200	PASS
69	198	0.00	100	56.4	83945	PASS
70	69	0.00	2	1.4	1186	PASS
127	198	10	80	52.6	78248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148824	PASS
199	198	5	9	6.6	9881	PASS
275	198	10	60	24.3	36125	PASS
365	198	1	100	3.8	5714	PASS
441	198	0.01	100	7.8	11555	PASS
442	442	50	100	100.0	70779	PASS
443	442	15	24	19.5	13814	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036728.D
Acq On : 27 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 27 16:00:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

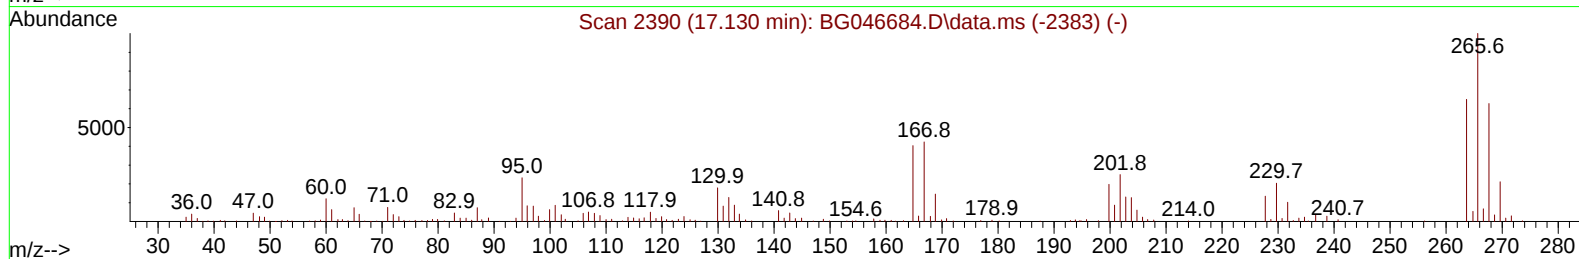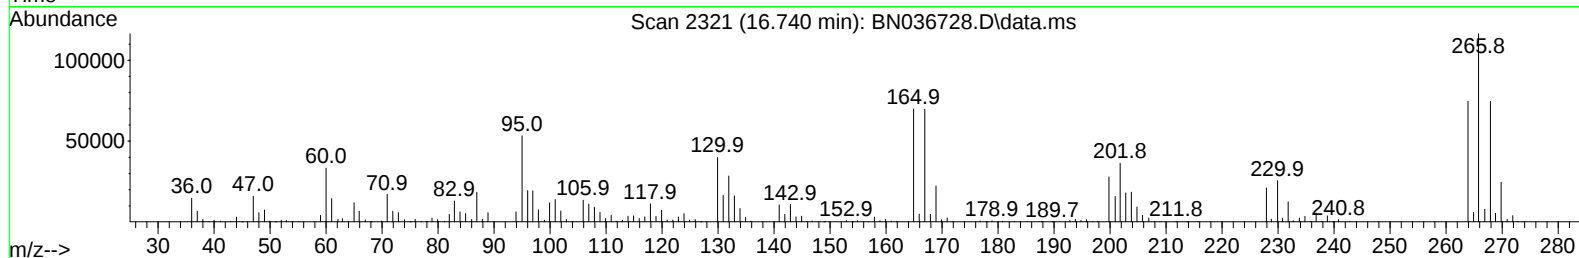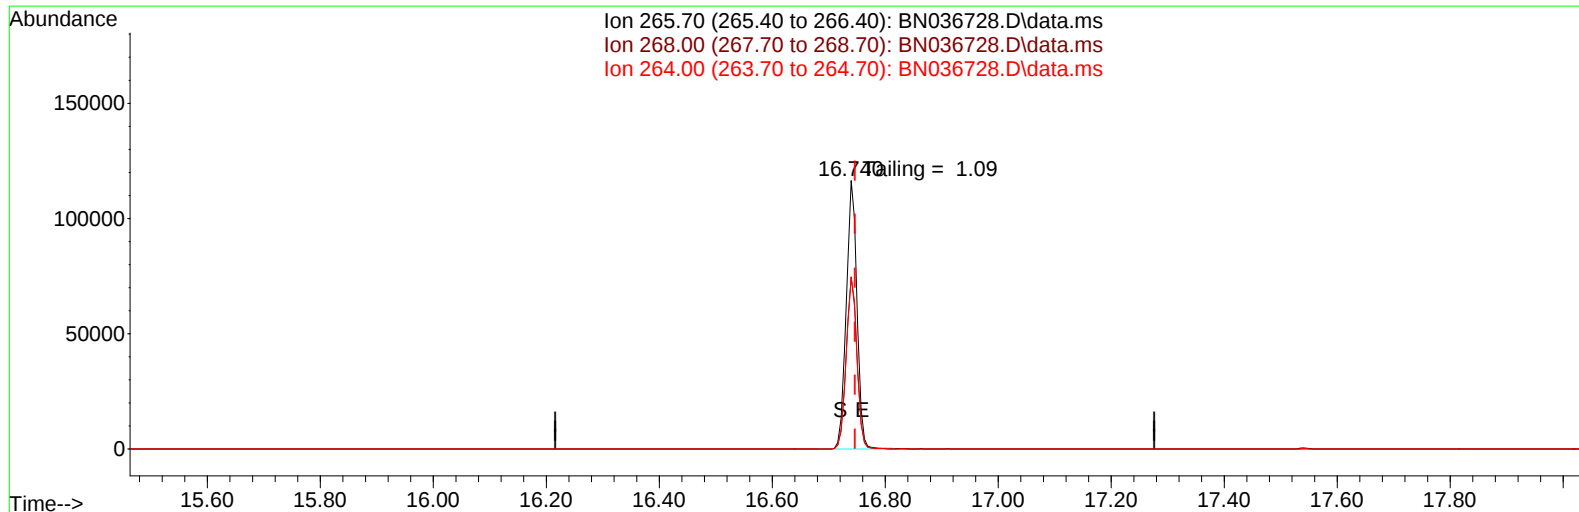

TIC: BN036728.D\data.ms

(70) Pentachlorophenol (C)

16.740min (-0.006) 17975.64 ng




response 152777

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.09
264.00	61.60	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036728.D
Acq On : 27 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 27 16:00:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

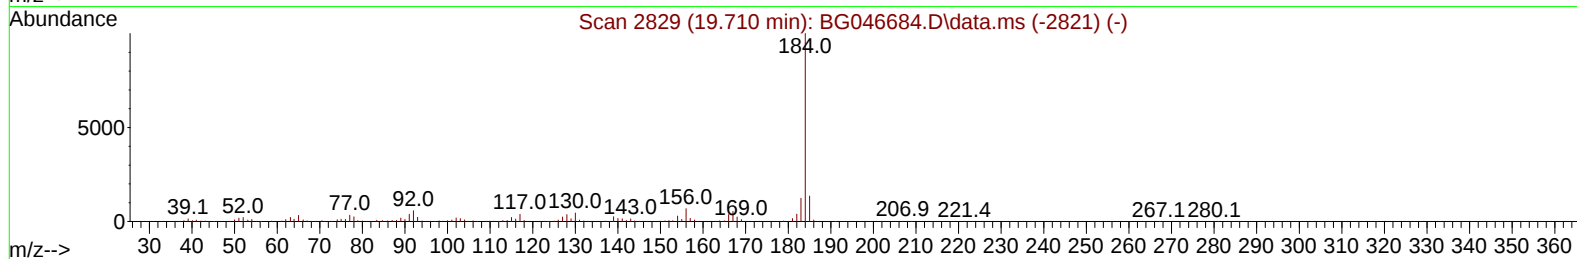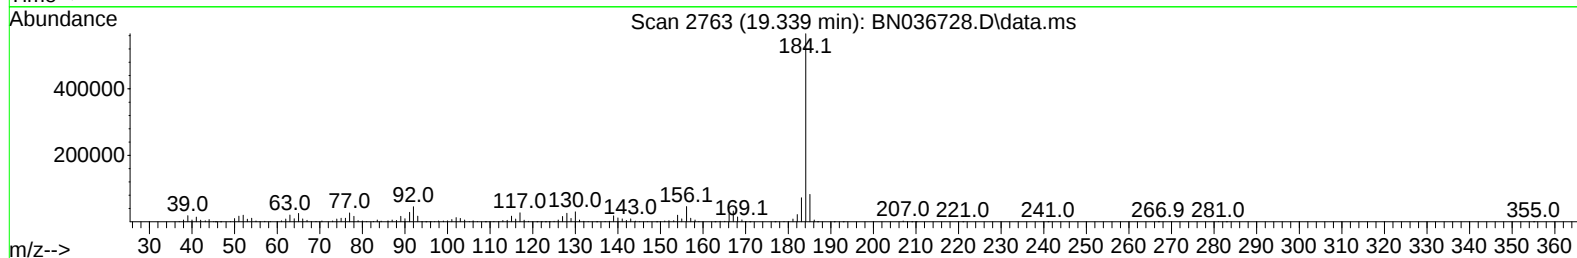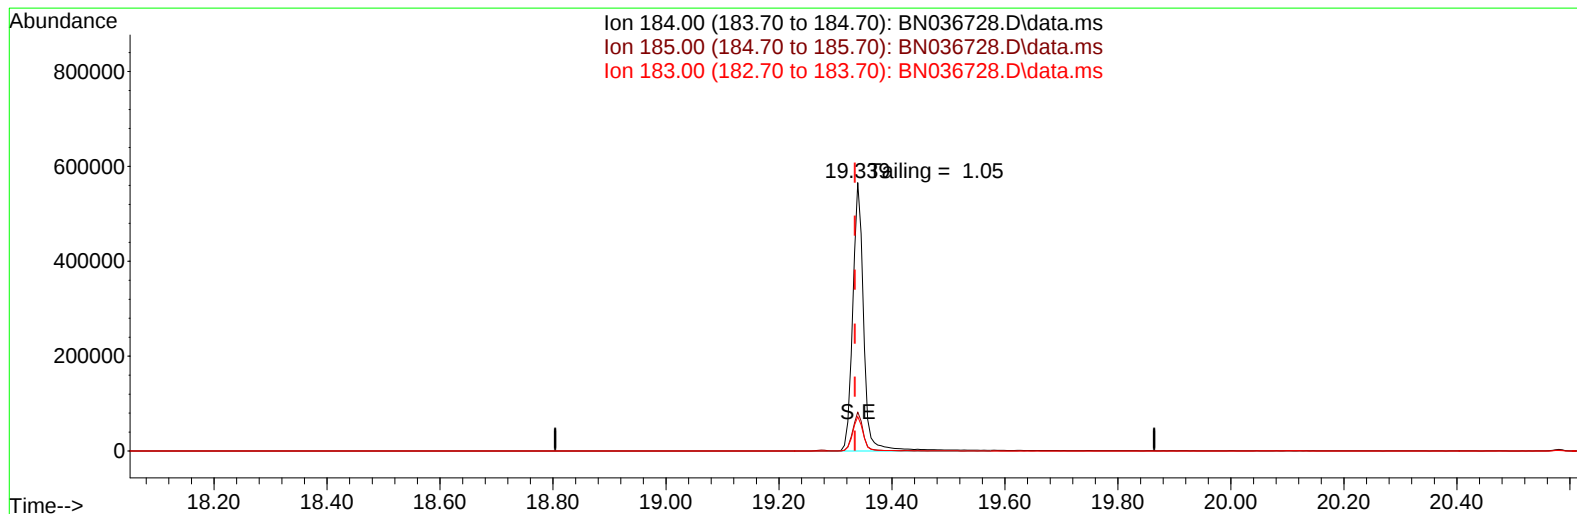

TIC: BN036728.D\data.ms

(77) Benzidine

19.339min (+ 0.005) 0.00 ng

response 768035

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.55
183.00	13.20	12.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/27/2025	BNA_N	<u>BN036728.D</u>
Compound Name	Response	Retention Time
DDT	567441	20.581
DDD	8560	20.192
DDE	316	19.634
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8876	576317	1.54

Instrument :
BNA_N
ClientSampleId :
DFTPP