
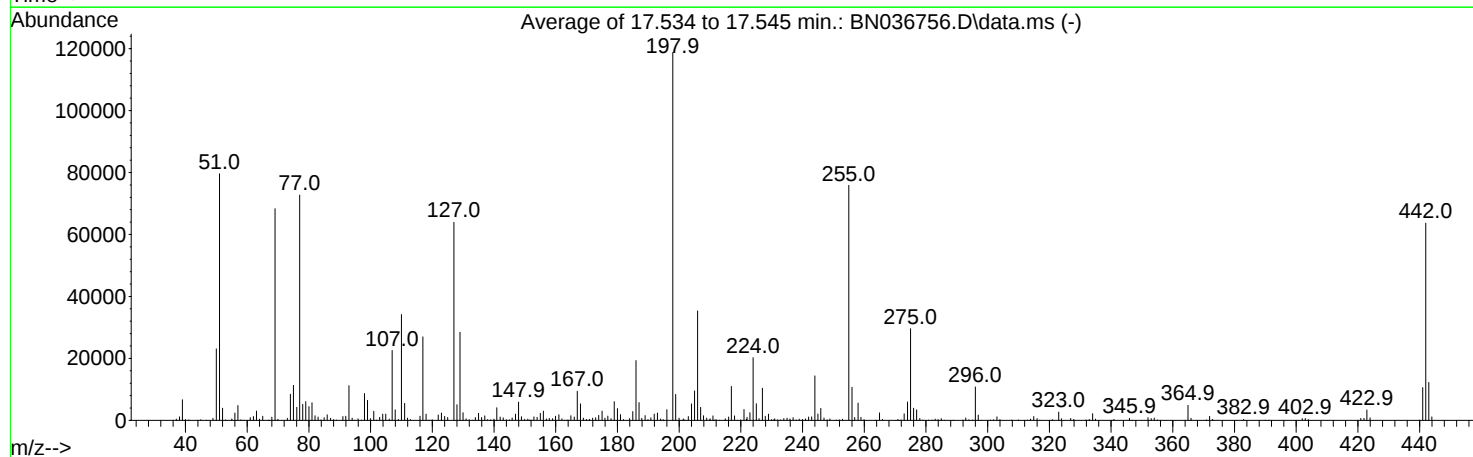


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036756.D
Acq On : 28 Mar 2025 03:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

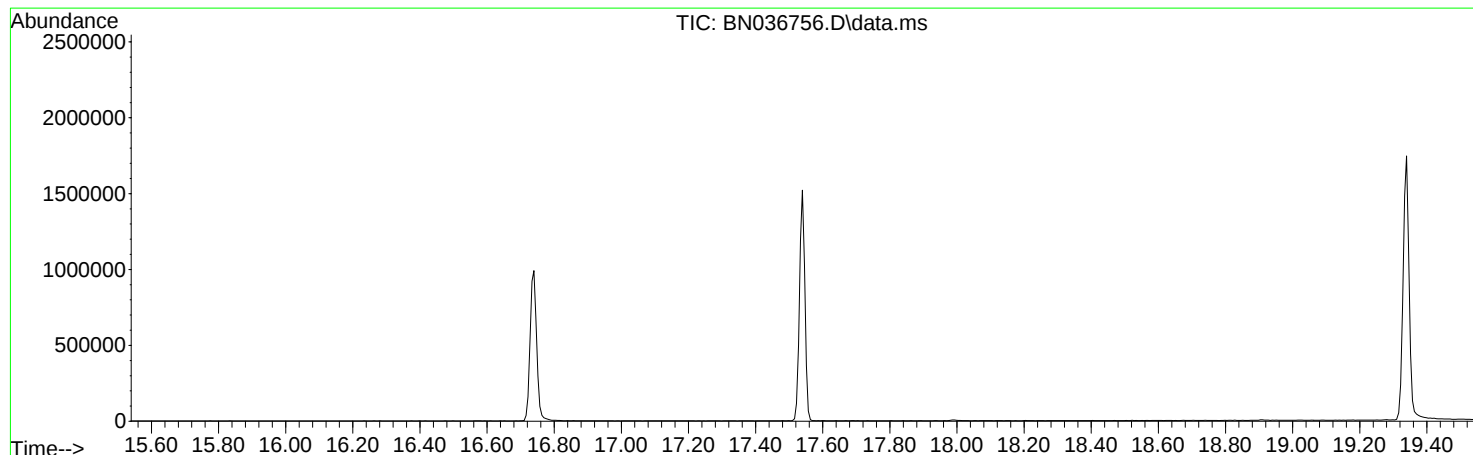




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	67.0	79608	PASS
68	69	0.00	2	1.5	1020	PASS
69	198	0.00	100	57.5	68325	PASS
70	69	0.00	2	0.5	357	PASS
127	198	10	80	53.9	63944	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118744	PASS
199	198	5	9	7.1	8386	PASS
275	198	10	60	24.9	29595	PASS
365	198	1	100	4.1	4858	PASS
441	198	0.01	100	8.9	10582	PASS
442	442	50	100	100.0	63691	PASS
443	442	15	24	19.2	12256	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036756.D
Acq On : 28 Mar 2025 03:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 28 05:40:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 28 05:40:24 2025
Response via : Initial Calibration

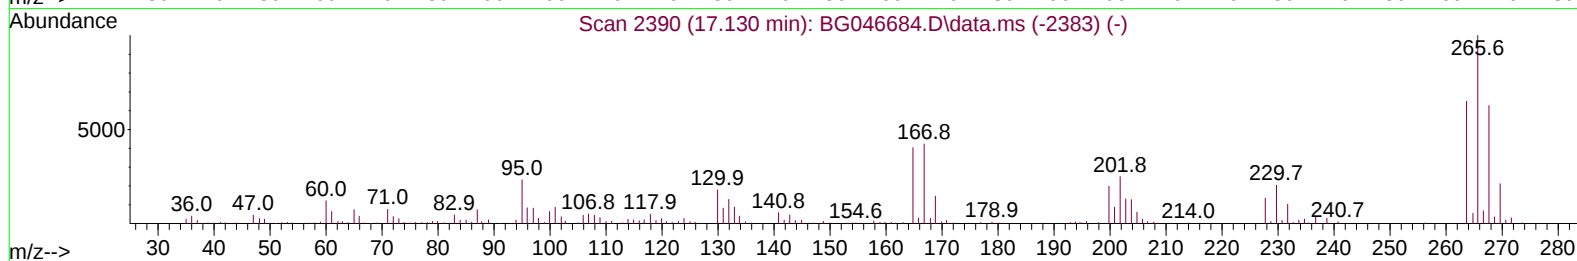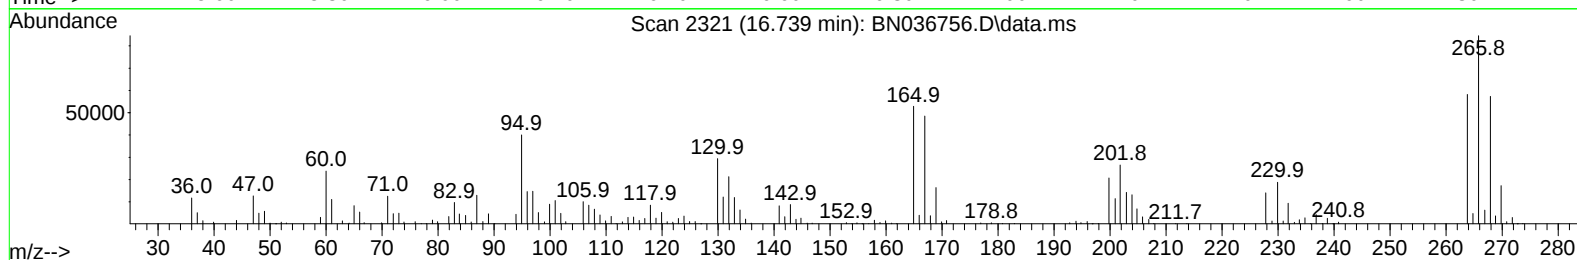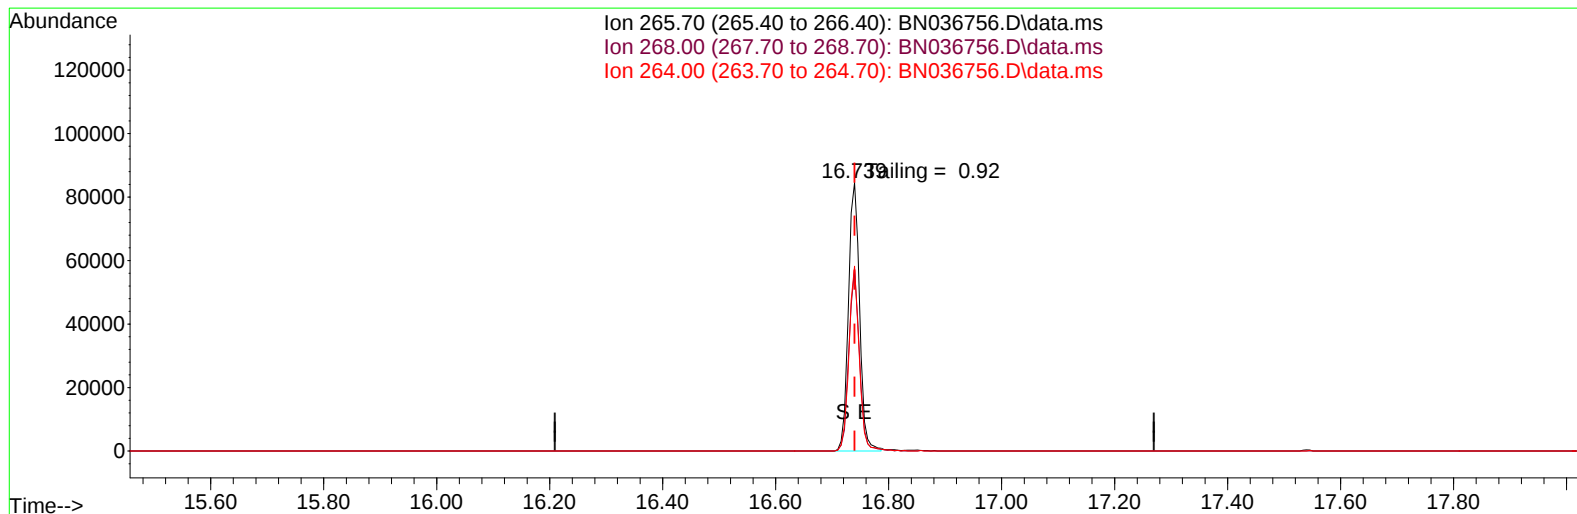

TIC: BN036756.D\data.ms

(70) Pentachlorophenol (C)

16.739min (0.000) 15913.57 ng




response 116893

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.77
264.00	61.60	68.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032725\
Data File : BN036756.D
Acq On : 28 Mar 2025 03:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 28 05:40:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 28 05:40:24 2025
Response via : Initial Calibration

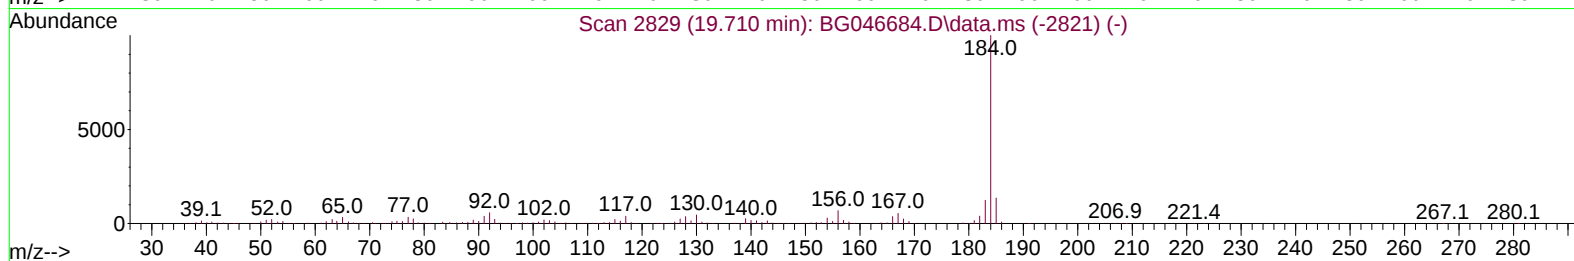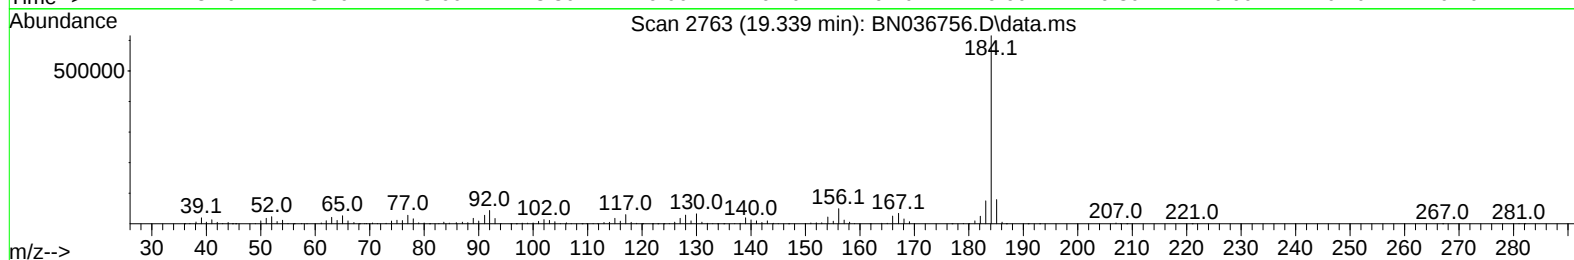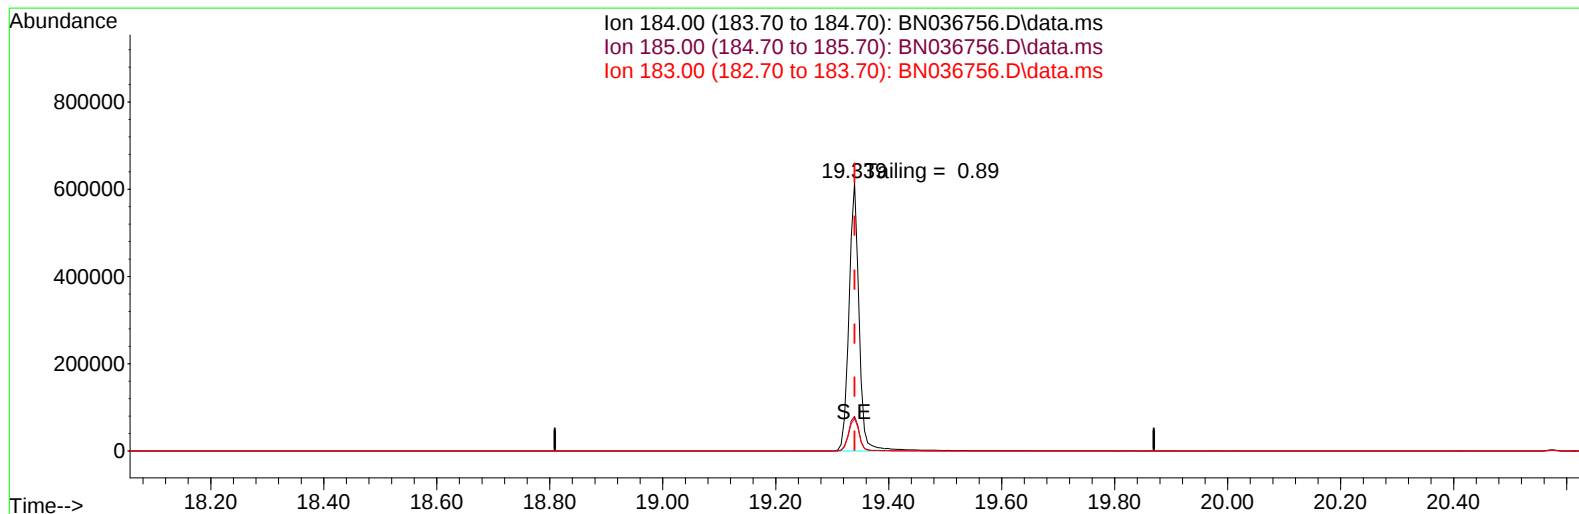

TIC: BN036756.D\data.ms

(77) Benzidine

19.339min (0.000) 0.00 ng

response 762967

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.92
183.00	13.20	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/27/2025	BNA_N	<u>BN036756.D</u>
Compound Name	Response	Retention Time
DDT	412653	20.575
DDD	5613	20.186
DDE	207	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5820	418473	1.39

Instrument :
BNA_N
ClientSampleId :
DFTPP