

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032818\
 Data File : BN000660.D
 Acq On : 28 Mar 2018 15:45
 Operator : JU/SJ
 Sample : PB107731BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 29 07:09:36 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 29 07:07:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	177904	20.00	ng/ul	0.00
18) Naphthalene-d8	11.25	136	811340	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.03	164	456695	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.75	188	969867	20.00	ng/ul	0.00
75) Chrysene-d12	21.88	240	858644	20.00	ng/ul	0.00
83) Perylene-d12	24.36	264	683572	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.58	96	29360	5.89	ng/uL	0.00
5) Phenol-d5	7.55	99	541824	32.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.71	67	334111	34.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.93	132	400993	31.95	ng/ul	0.00
13) 4-Methylphenol-d8	9.12	113	440029	34.04	ng/ul	0.00
19) Nitrobenzene-d5	9.59	128	207225	31.45	ng/ul	0.00
22) 2-Nitrophenol-d4	10.32	143	225557	33.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	368799	30.14	ng/ul	0.00
29) 4-Chloroaniline-d4	11.38	131	561958	44.74	ng/ul	0.00
43) Dimethylphthalate-d6	14.42	166	1329440	36.85	ng/ul	0.00
46) Acenaphthylene-d8	14.72	160	1596658	33.54	ng/ul	0.00
51) 4-Nitrophenol-d4	15.22	143	184754	27.58	ng/ul	0.00
57) Fluorene-d10	16.01	176	1061565	34.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.13	200	147630	26.58	ng/ul	0.00
70) Anthracene-d10	17.85	188	1670744	35.84	ng/ul	0.00
76) Pyrene-d10	20.11	212	1737964	36.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.20	264	1242829	38.52	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.12	70	10694	1.064	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN032818\
Data File : BN000660.D
Acq On : 28 Mar 2018 15:45
Operator : JU/SJ
Sample : PB107731BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 29 07:09:36 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 29 07:07:58 2018
Response via : Initial Calibration

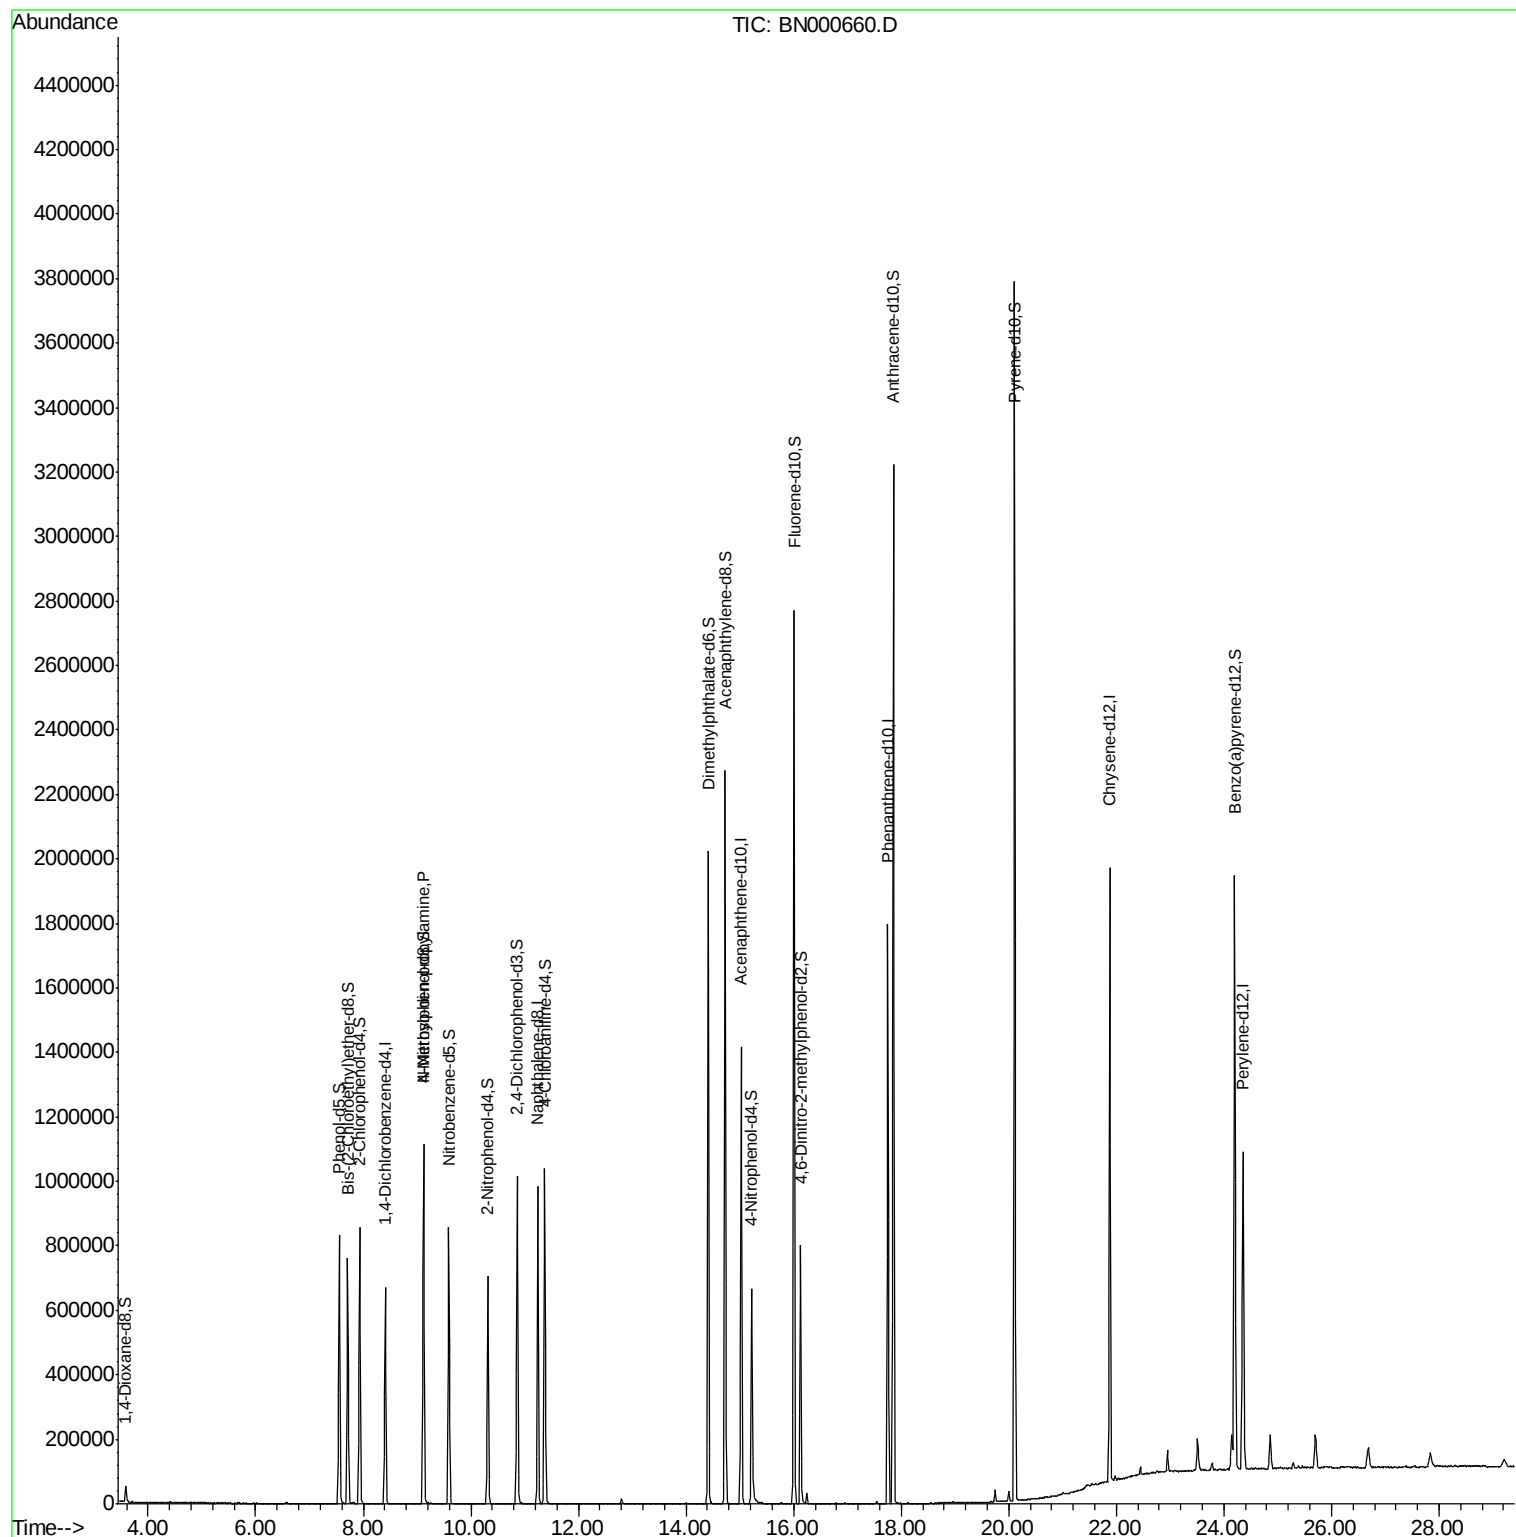

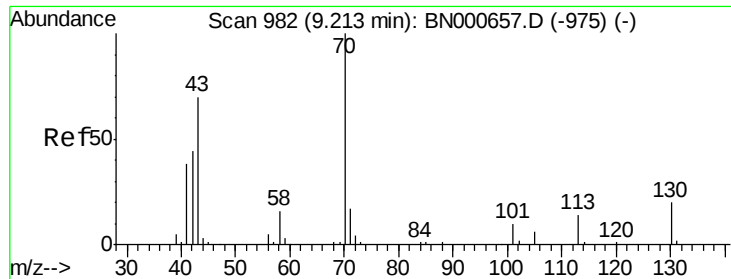

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.064 ng/ul
 RT: 9.12 min Scan# 966
 Delta R.T. -0.09 min
 Lab File: BN000660.D
 Acq: 28 Mar 2018 15:45

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 10694
 Ion Ratio Lower Upper
 70 100
 42 318.6 40.2 60.4#
 101 0.0 7.7 11.5#
 130 0.0 17.8 26.6#

