
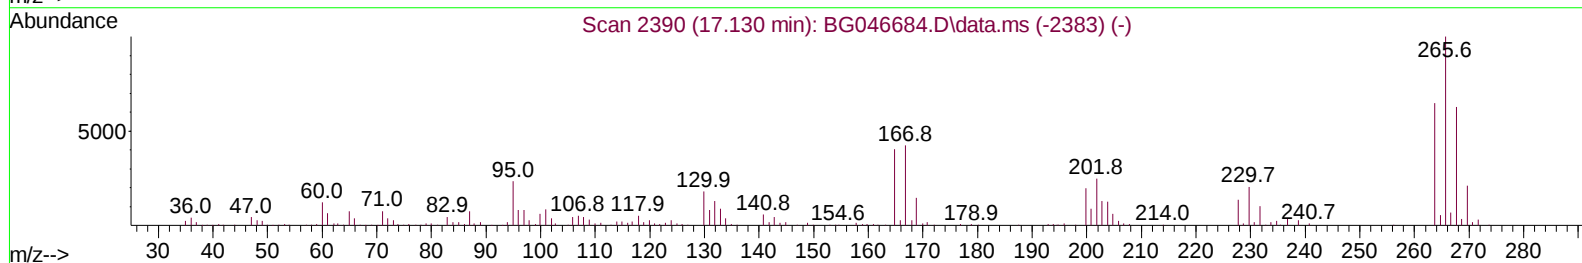
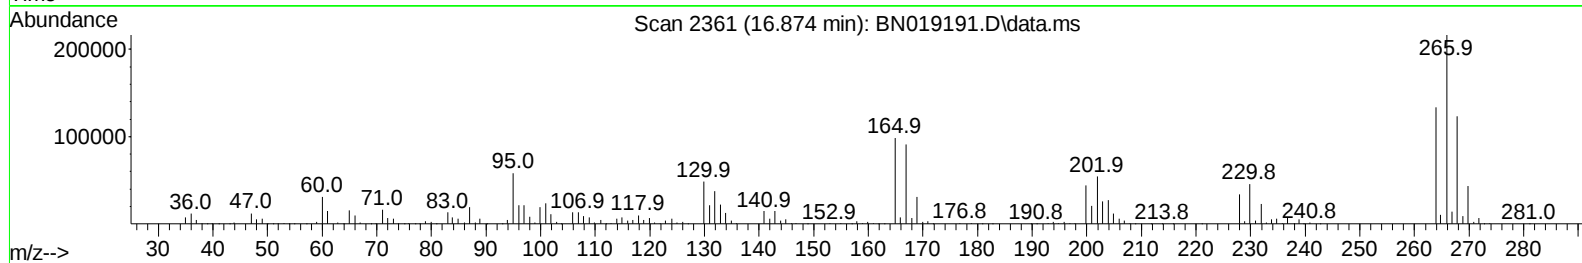


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
Data File : BN019191.D
Acq On : 28 Mar 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 18:41:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:41:21 2022
Response via : Initial Calibration

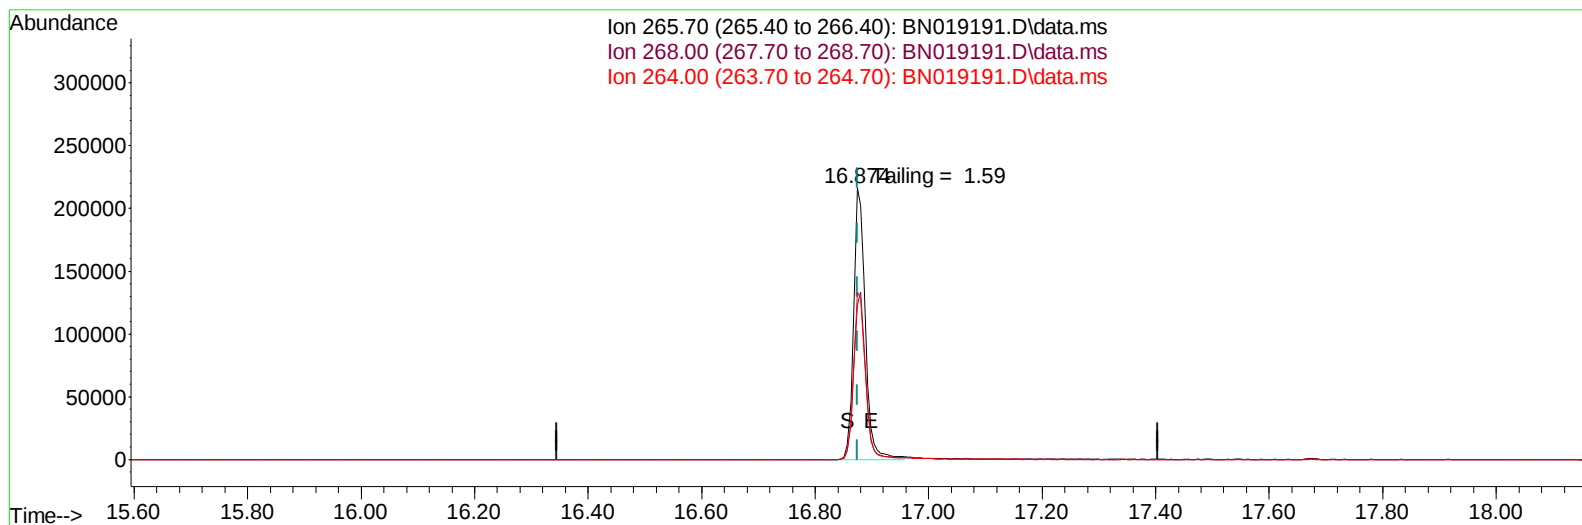




TIC: BN019191.D\data.ms

(70) Pentachlorophenol (C)**16.874min (0.000) 23034.62 ng****response 317432**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.95
264.00	61.60	61.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
Data File : BN019191.D
Acq On : 28 Mar 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 18:41:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 18:41:21 2022
Response via : Initial Calibration

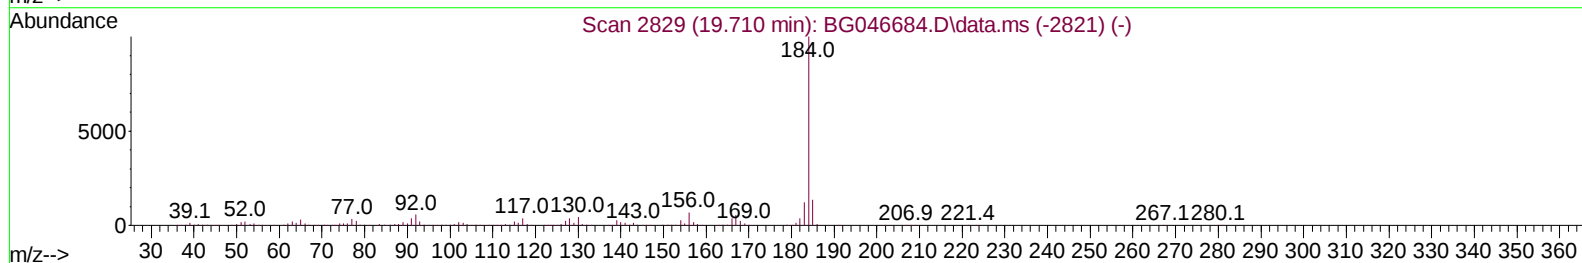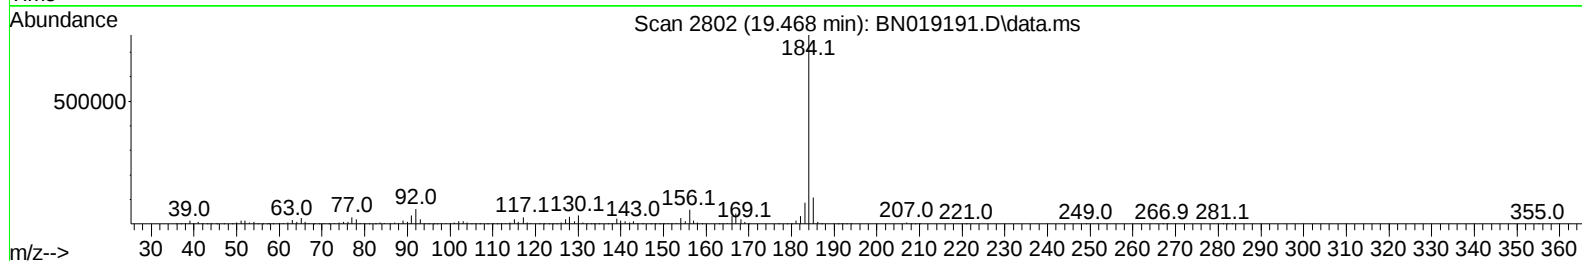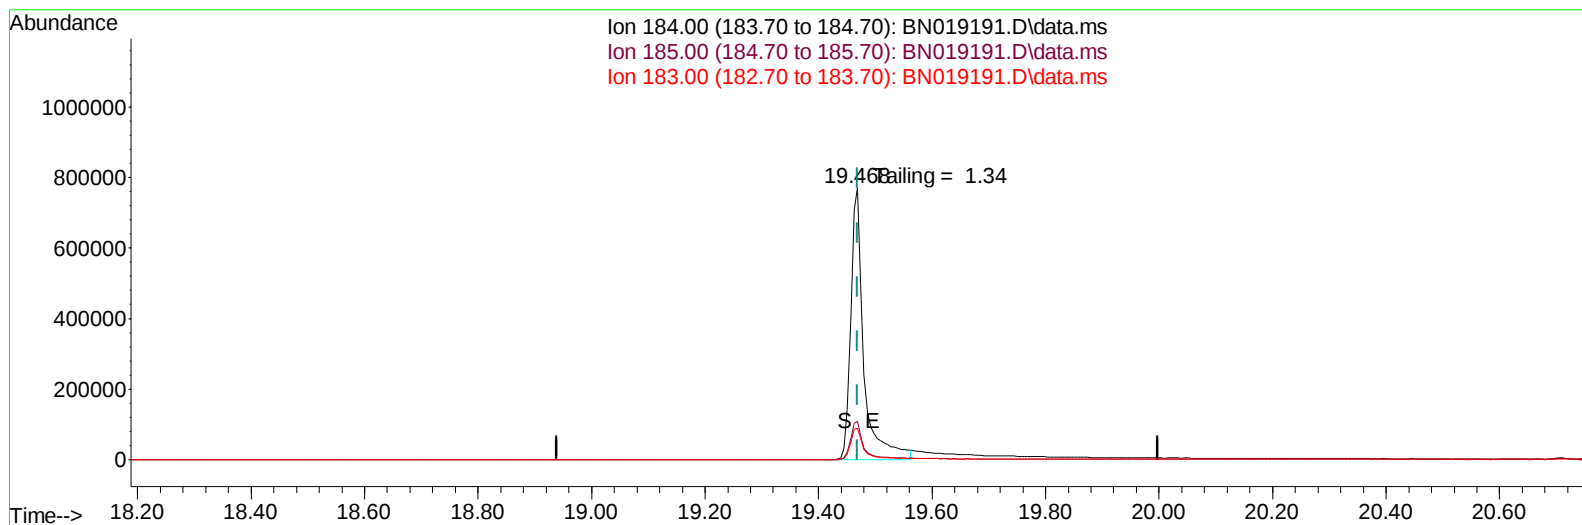

TIC: BN019191.D\data.ms

(77) Benzidine**19.468min (0.000) 0.00 ng****response 1383582**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.38
0.00	0.00	0.00