
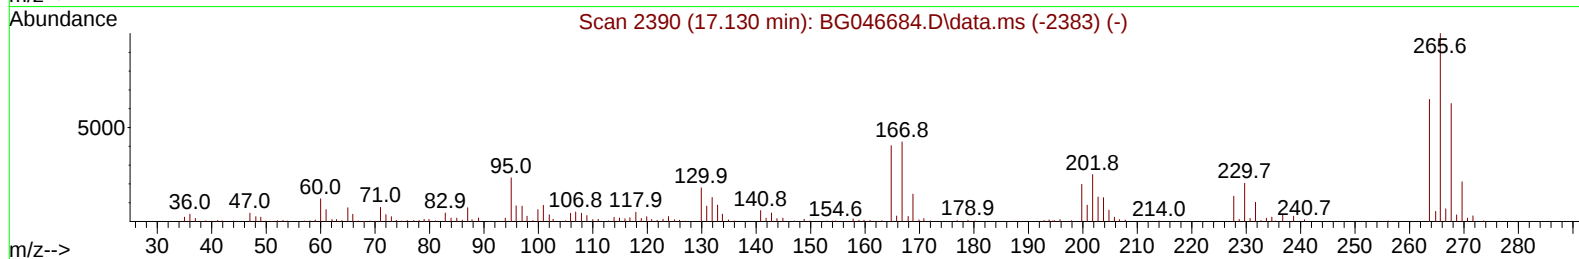
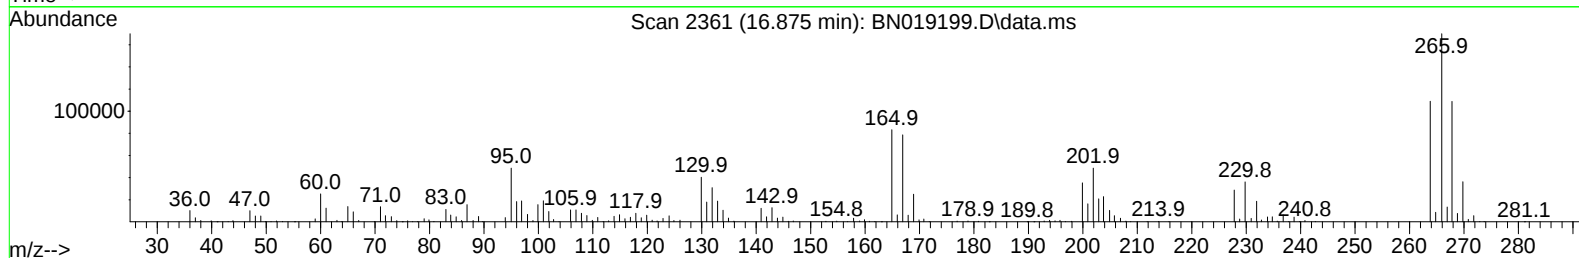


Quant Time: Mar 29 08:49:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 08:49:42 2022
Response via : Initial Calibration

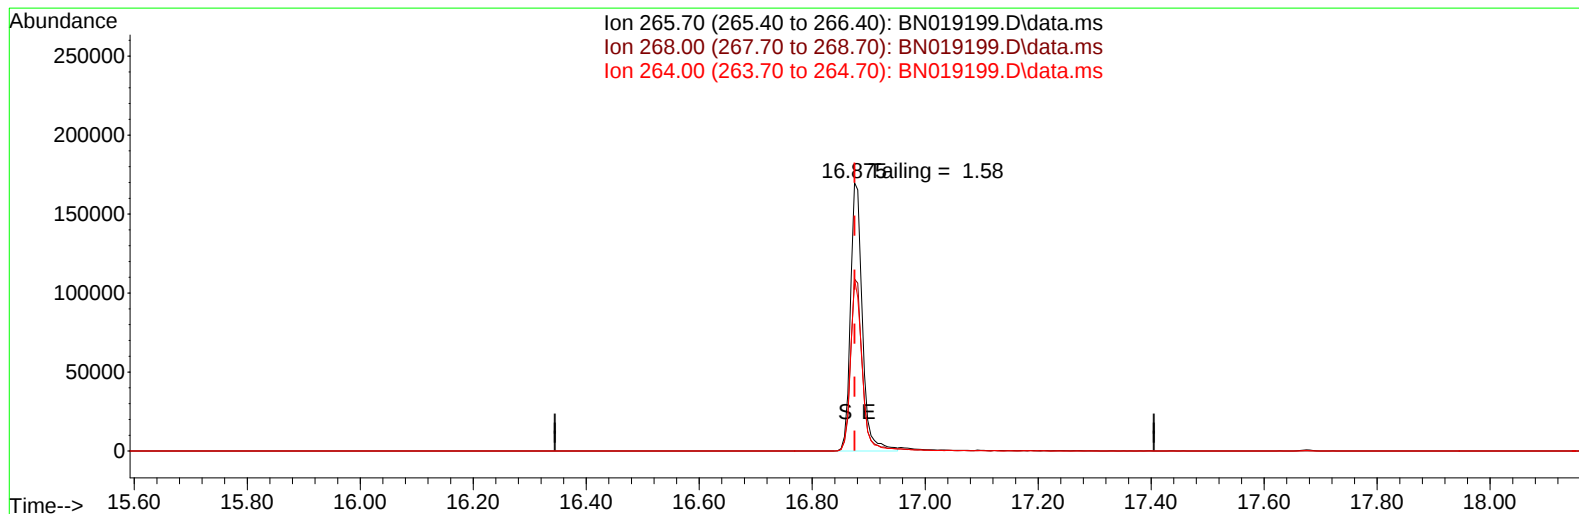

TIC: BN019199.D\data.ms

(70) Pentachlorophenol (C)




16.875min (0.000) 18330.03 ng

response **254182**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.06
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
Data File : BN019199.D
Acq On : 28 Mar 2022 17:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 08:49:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 08:49:42 2022
Response via : Initial Calibration

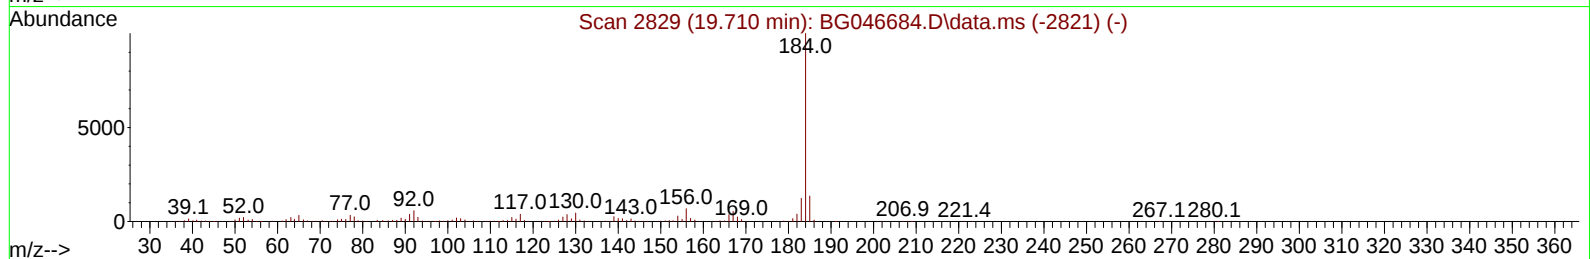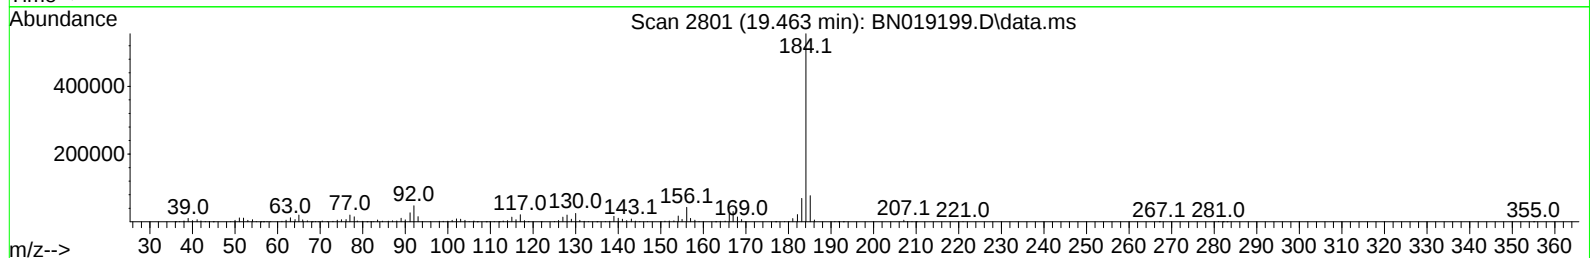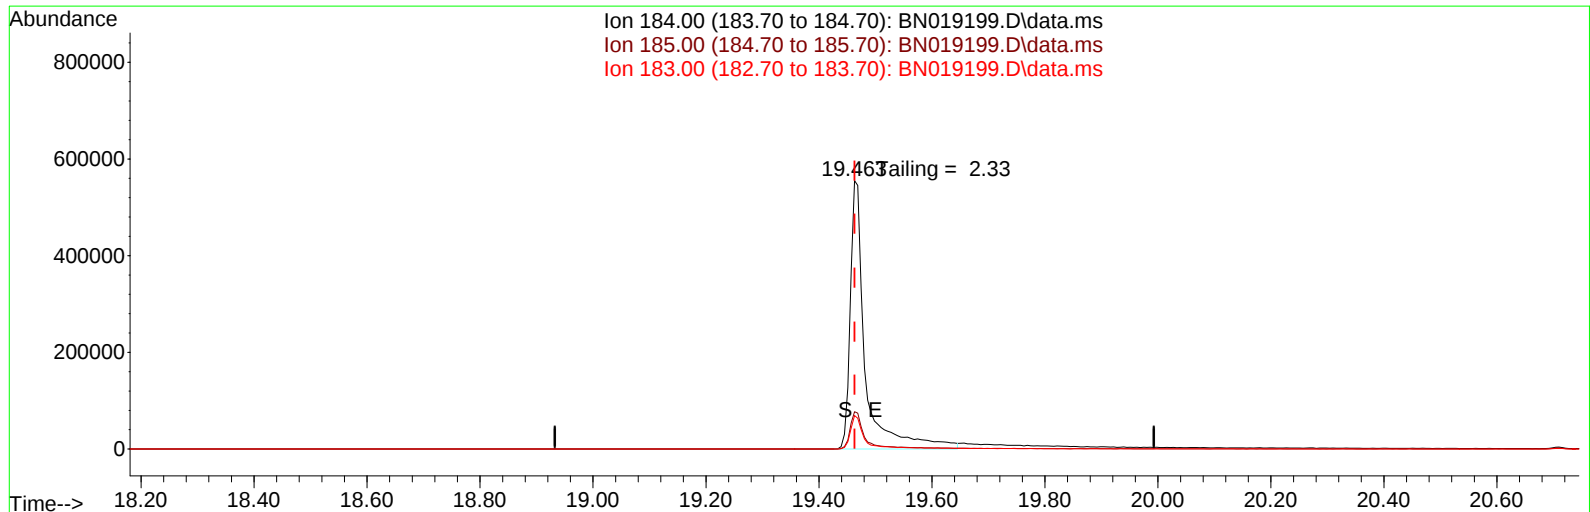

TIC: BN019199.D\data.ms

(77) Benzidine

19.463min (0.000) 0.00 ng

response 1068544

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	12.45
0.00	0.00	0.00