

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
 Data File : BN019213.D
 Acq On : 29 Mar 2022 01:55
 Operator : CG/JU
 Sample : N2095-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GW-01-(SB-01)

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 03/29/2022
 Supervised By : Jagrut Upadhyay 03/29/2022

Quant Time: Mar 29 06:25:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 19:03:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.847	152	3421	0.400	ng	0.00
7) Naphthalene-d8	10.648	136	9251	0.400	ng	# 0.00
13) Acenaphthene-d10	14.485	164	5514	0.400	ng	0.00
19) Phenanthrene-d10	17.226	188	11085	0.400	ng	0.00
29) Chrysene-d12	21.413	240	7714	0.400	ng	# 0.00
35) Perylene-d12	23.776	264	6125	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.406	112	1342	0.166	ng	0.00
5) Phenol-d6	7.017	99	828	0.089	ng	0.01
8) Nitrobenzene-d5	9.014	82	1466m	0.204	ng	0.02
11) 2-Methylnaphthalene-d10	12.242	152	4456	0.301	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	688	0.257	ng	0.00
15) 2-Fluorobiphenyl	13.105	172	6616	0.286	ng	0.00
27) Fluoranthene-d10	19.257	212	13516	0.417	ng	0.00
31) Terphenyl-d14	19.851	244	7483	0.435	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.324	149	1498	0.099	ng	# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
Data File : BN019213.D
Acq On : 29 Mar 2022 01:55
Operator : CG/JU
Sample : N2095-16
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

Quant Time: Mar 29 06:25:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 19:03:12 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

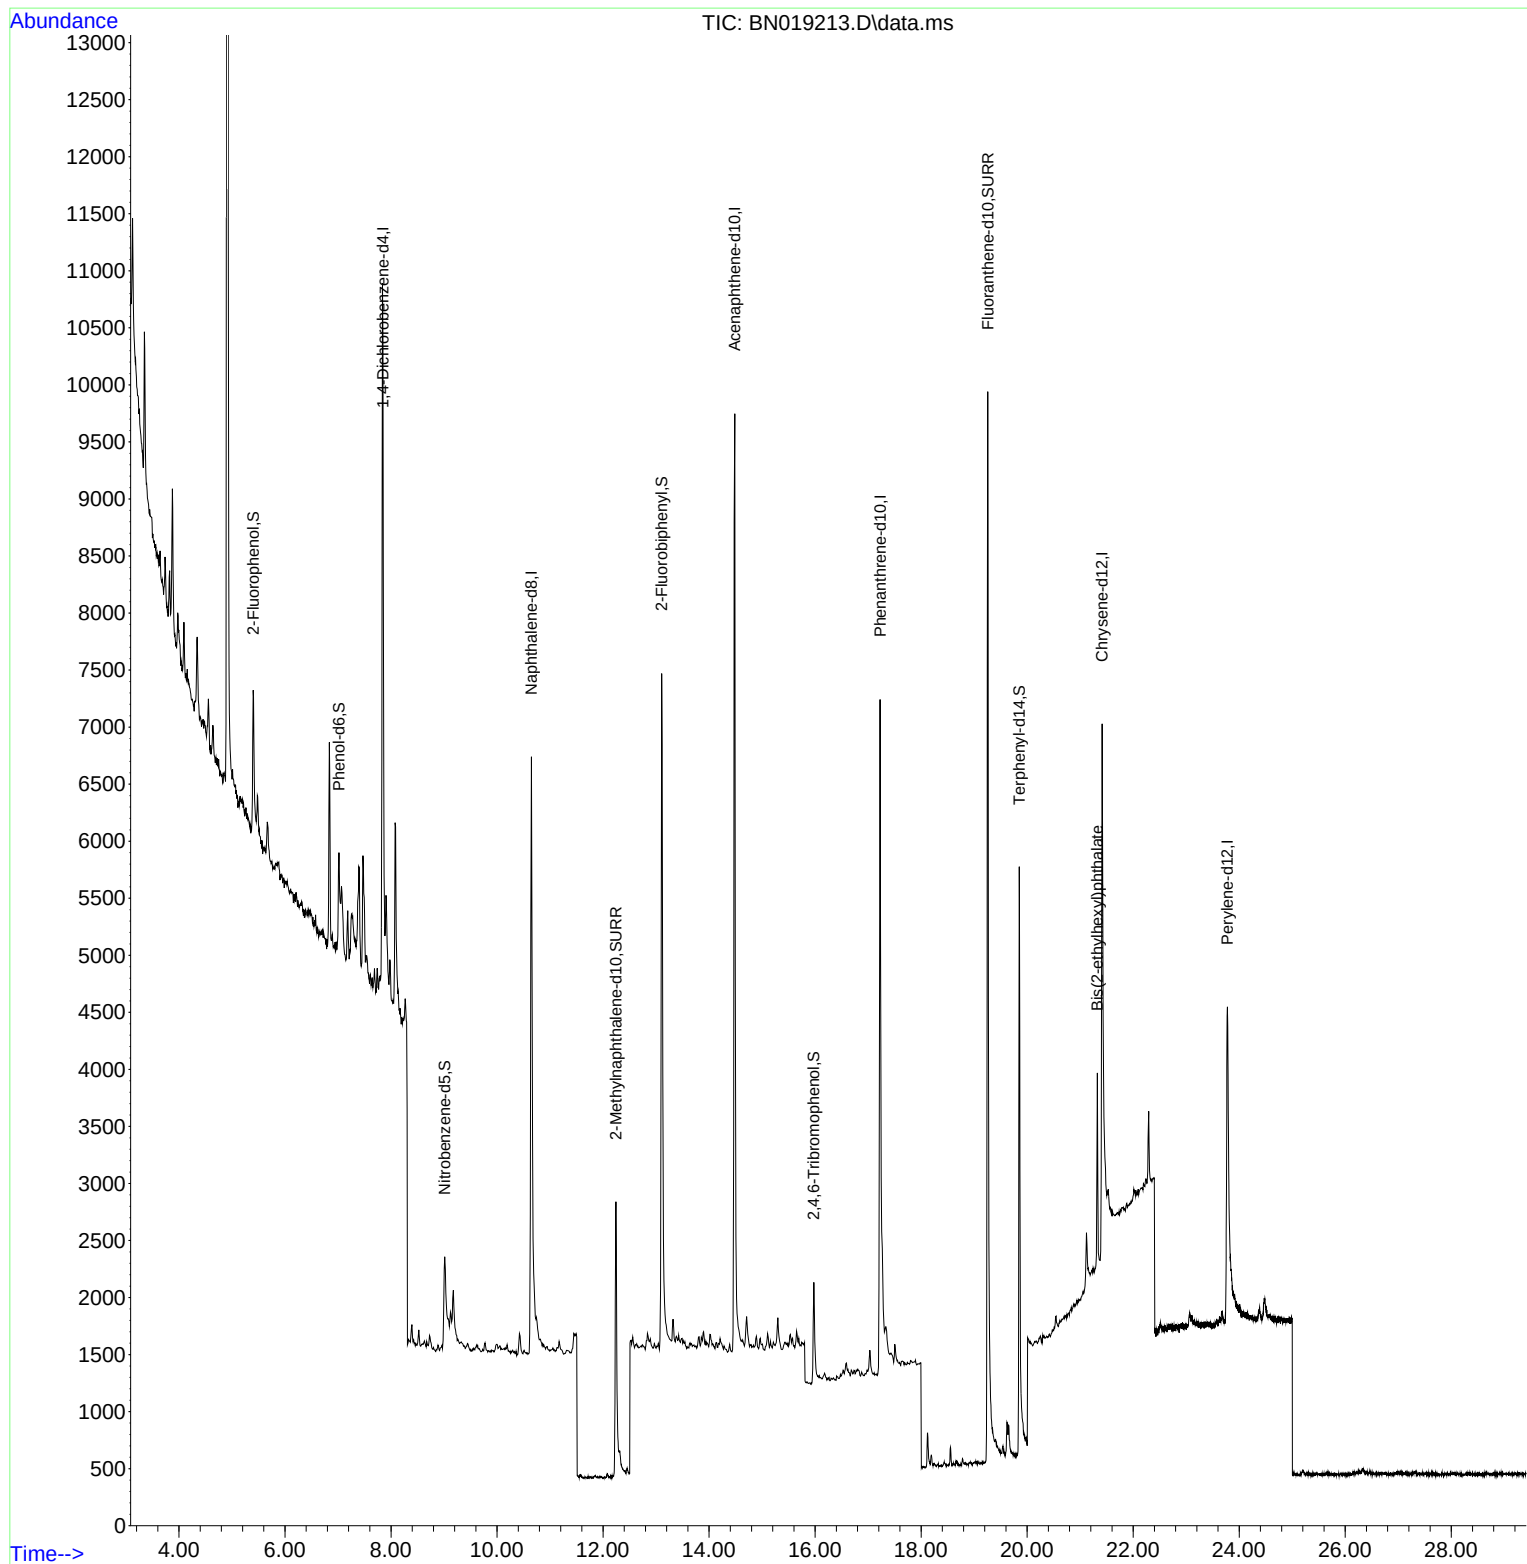



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.847 min Scan# 660
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

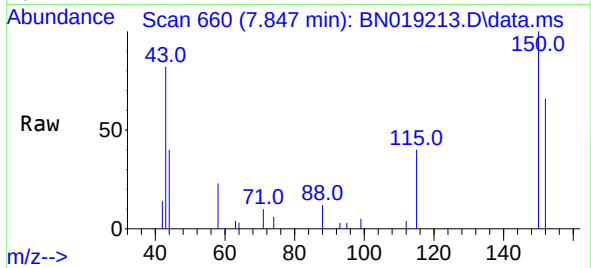


Tgt Ion:152 Resp: 342
Ion Ratio Lower Upper
152 100
150 151.1 123.9 185.9
115 60.1 48.2 72.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

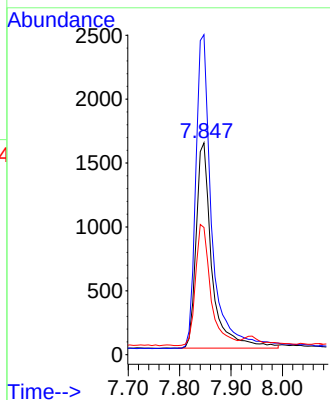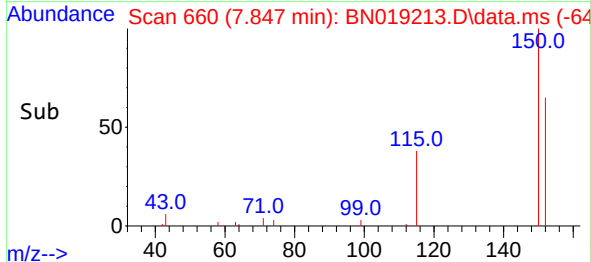


#4
2-Fluorophenol
Concen: 0.166 ng
RT: 5.406 min Scan# 322
Delta R.T. 0.007 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

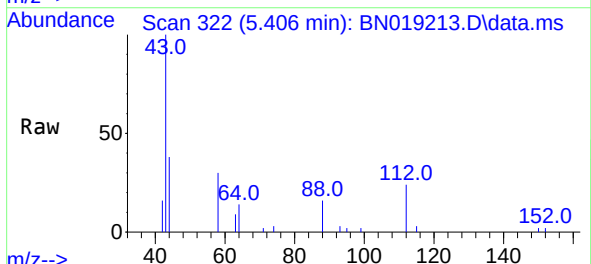


Tgt Ion:112 Resp: 1342
Ion Ratio Lower Upper
112 100
64 65.1 47.8 71.8
63 30.9 25.7 38.5

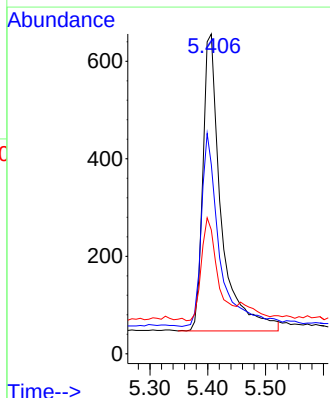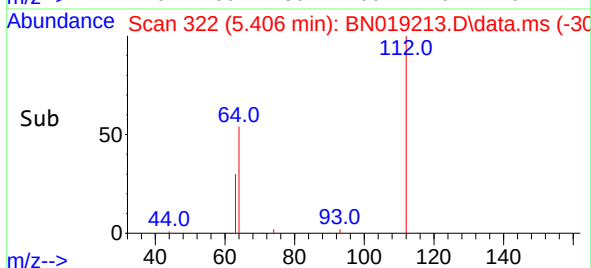



#5
Phenol-d6
Concen: 0.089 ng
RT: 7.017 min Scan# 543
Delta R.T. 0.014 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

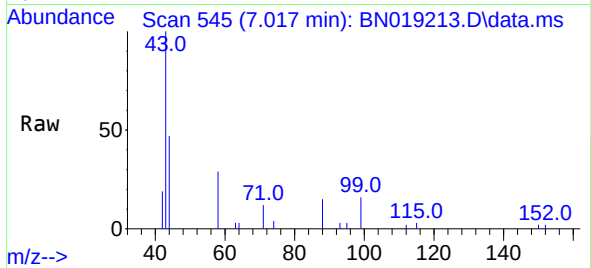


Tgt Ion: 99 Resp: 828
Ion Ratio Lower Upper
99 100
42 18.4 16.2 24.4
71 47.3 27.7 41.5

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

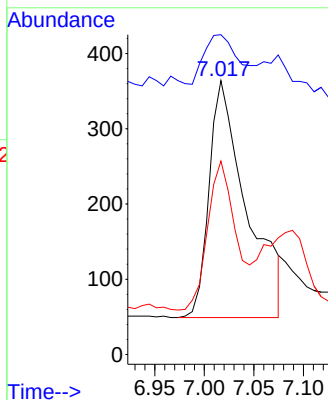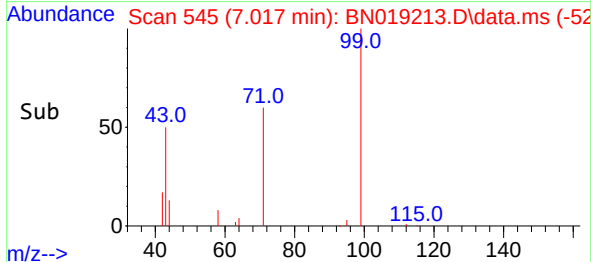


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.648 min Scan# 943
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

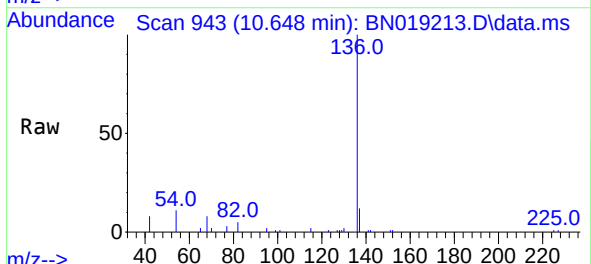


Tgt Ion:136 Resp: 9251
Ion Ratio Lower Upper
136 100
137 12.2 9.0 13.4
54 11.4 5.8 8.6#
68 8.1 4.6 7.0#

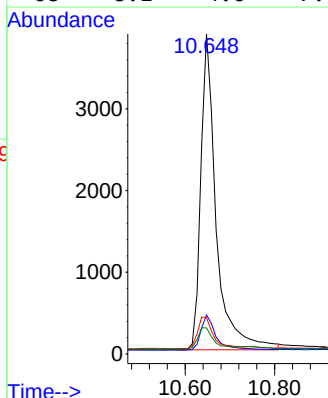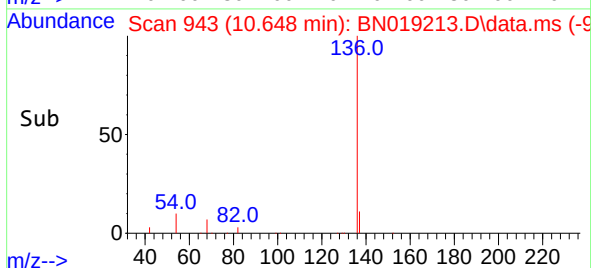

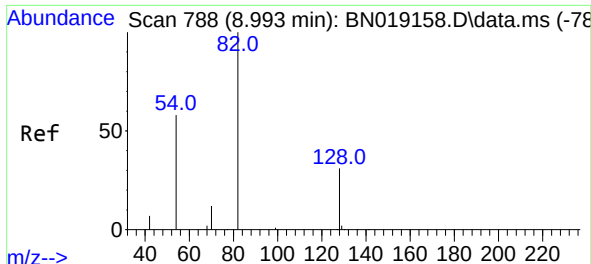

#8
Nitrobenzene-d5
Concen: 0.204 ng m
RT: 9.014 min Scan# 790
Delta R.T. 0.021 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)



Tgt Ion: 82 Resp: 1460
Ion Ratio Lower Upper
82 100
128 43.8 33.0 49.6
54 61.5 42.5 63.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

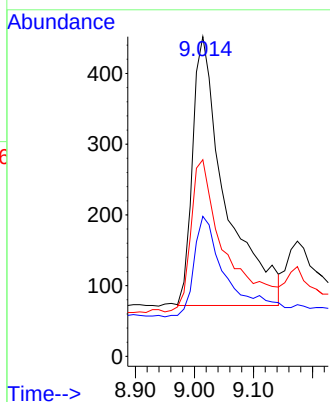

#11
2-Methylnaphthalene-d10
Concen: 0.301 ng
RT: 12.242 min Scan# 1217
Delta R.T. 0.004 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55


Tgt Ion:152 Resp: 4456
Ion Ratio Lower Upper
152 100
151 21.3 16.5 24.7

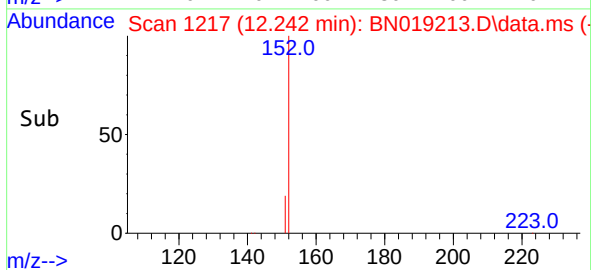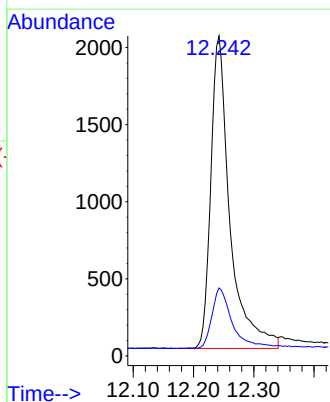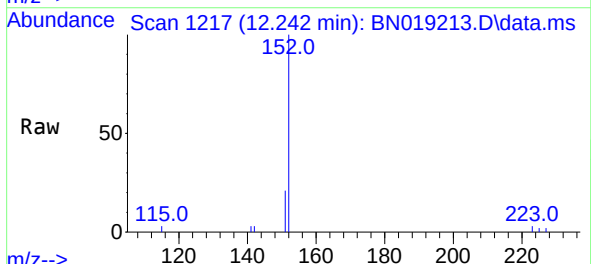



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.485 min Scan# 1472
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

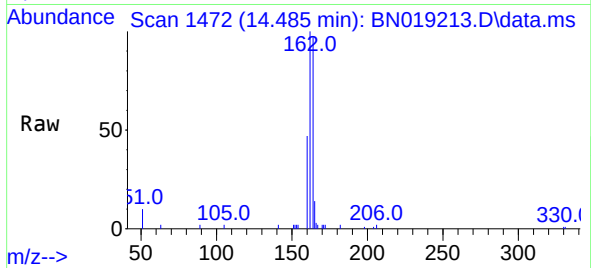


Tgt Ion:164 Resp: 5514
Ion Ratio Lower Upper
164 100
162 103.4 85.2 127.8
160 49.1 41.5 62.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

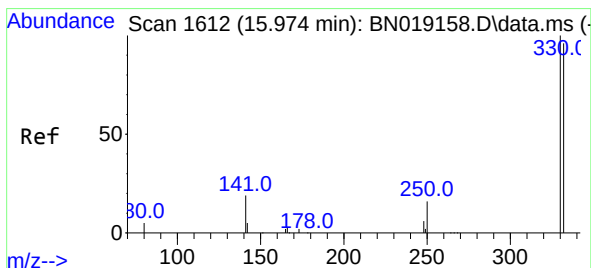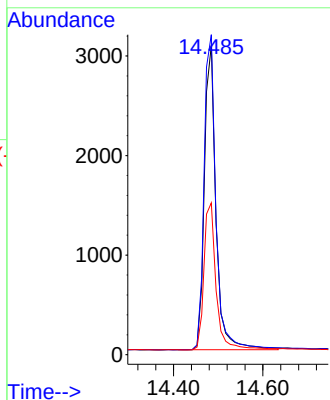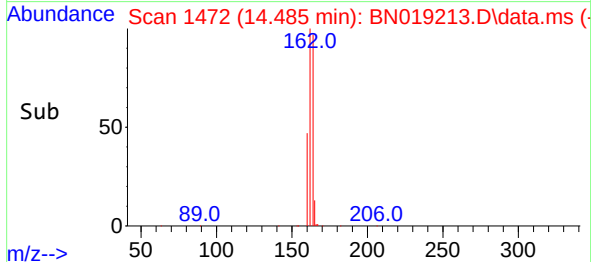


#14
2,4,6-Tribromophenol
Concen: 0.257 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

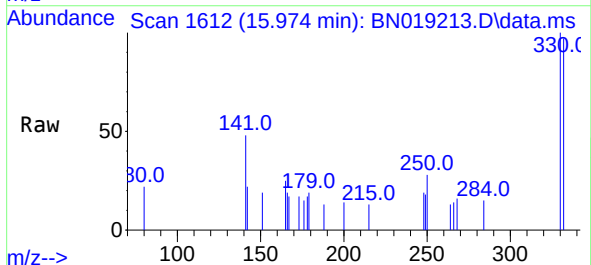


Tgt Ion:330 Resp: 688
Ion Ratio Lower Upper
330 100
332 95.1 76.8 115.2
141 42.4 32.2 48.2

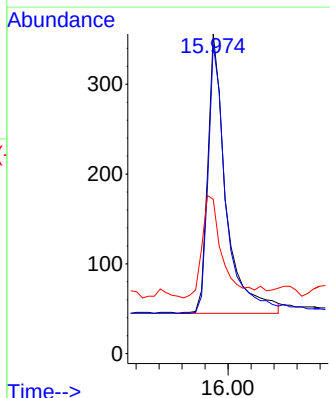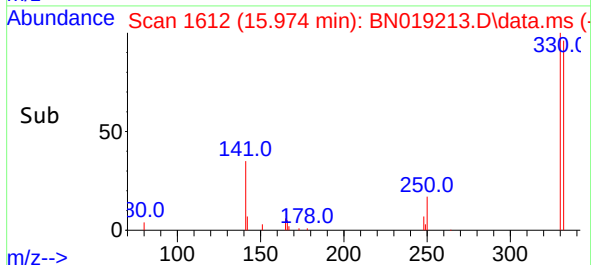



#15
2-Fluorobiphenyl
Concen: 0.286 ng
RT: 13.105 min Scan# 1343
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)




Tgt Ion:172 Resp: 6610
Ion Ratio Lower Upper
172 100
171 36.8 28.2 42.2
170 24.9 18.7 28.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

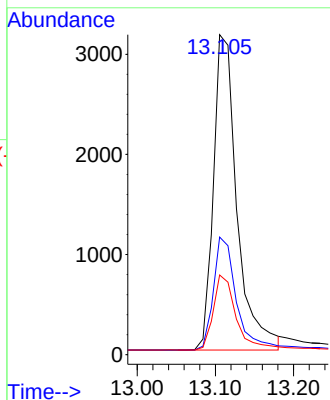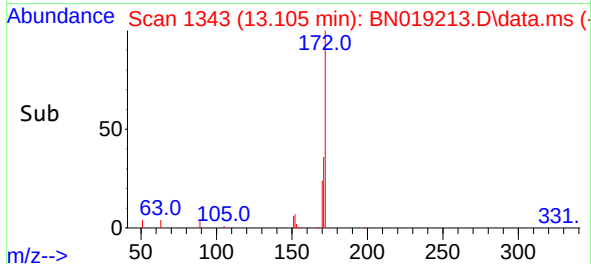


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.226 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

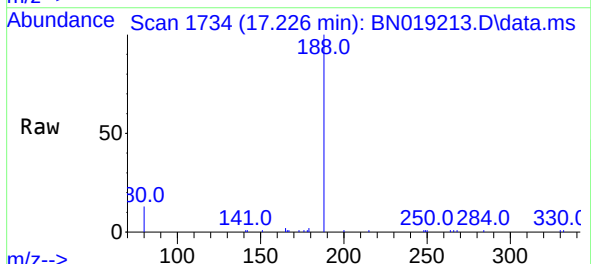


Tgt Ion:188 Resp: 11085
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.8 11.8 17.8

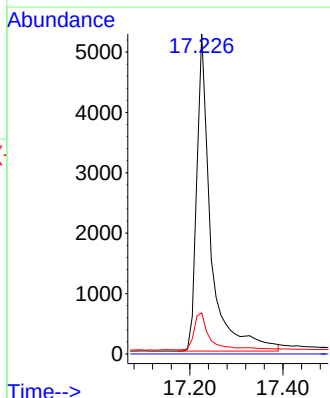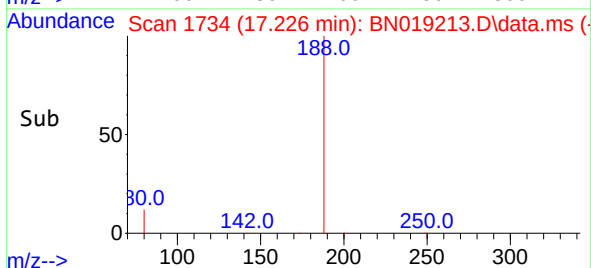

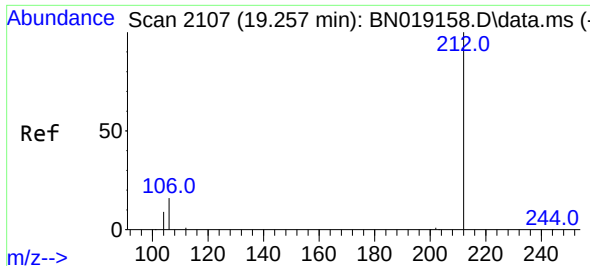

#27
Fluoranthene-d10
Concen: 0.417 ng
RT: 19.257 min Scan# 2107
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55




Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

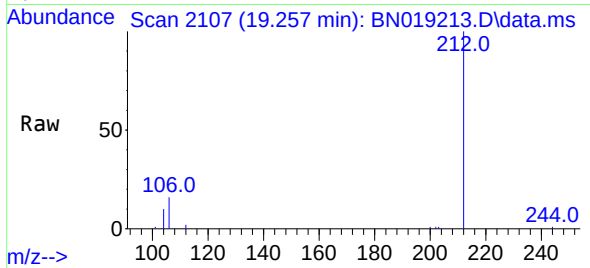


Tgt Ion:212 Resp: 13510
Ion Ratio Lower Upper
212 100
106 15.3 12.7 19.1
104 8.8 7.1 10.7

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

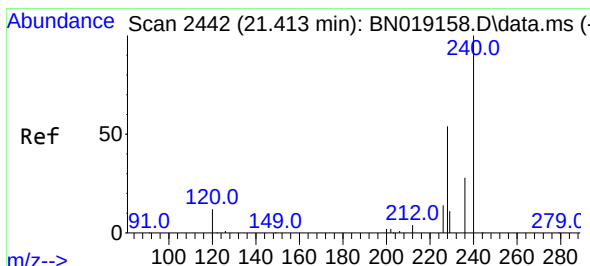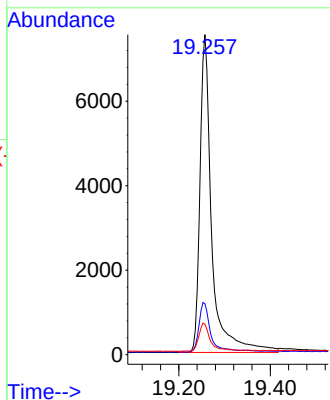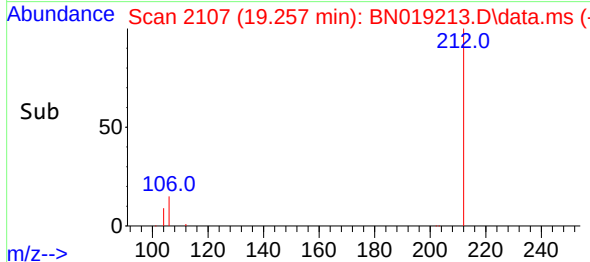


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.413 min Scan# 2442
Delta R.T. 0.000 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

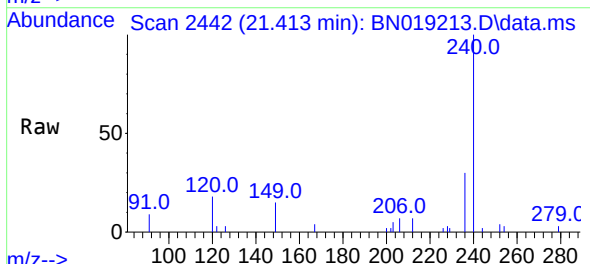

Tgt Ion:240 Resp: 7714
Ion Ratio Lower Upper
240 100
120 18.5 8.5 12.7#
236 29.6 22.4 33.6

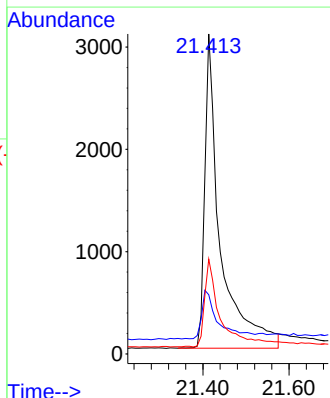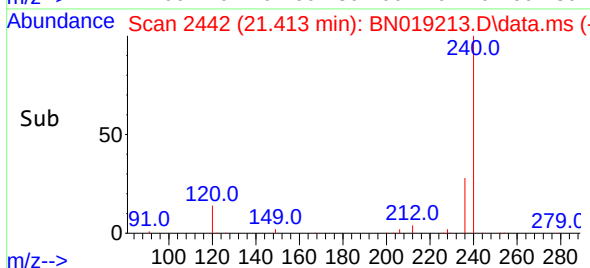




#31
 Terphenyl-d14
 Concen: 0.435 ng
 RT: 19.851 min Scan# 211
 Delta R.T. 0.000 min
 Lab File: BN019213.D
 Acq: 29 Mar 2022 01:55

Instrument :

BNA_N

ClientSampleId :

GW-01-(SB-01)



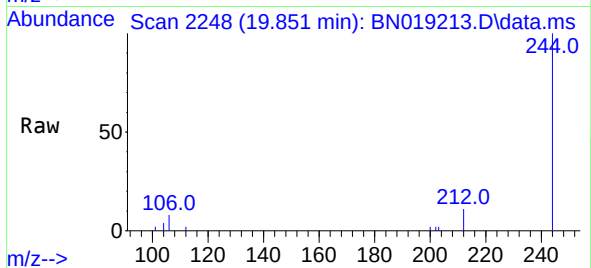


Tgt Ion:244 Resp: 748
 Ion Ratio Lower Upper
 244 100
 212 11.3 8.2 12.4
 122 0.0 0.0 0.0


Manual Integrations

APPROVED



Reviewed By :Christian Giraldo 03/29/2022
 Supervised By :Jagrut Upadhyay 03/29/2022

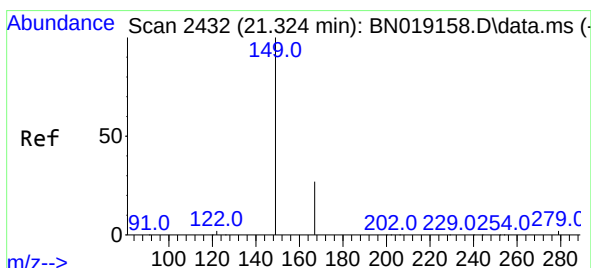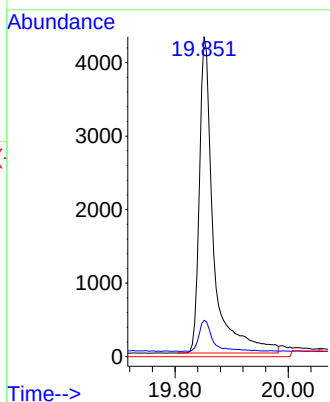


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.099 ng
 RT: 21.324 min Scan# 2432
 Delta R.T. 0.000 min
 Lab File: BN019213.D
 Acq: 29 Mar 2022 01:55



Tgt Ion:149 Resp: 1498
 Ion Ratio Lower Upper
 149 100
 167 25.4 21.8 32.8
 279 3.3 2.0 3.0#

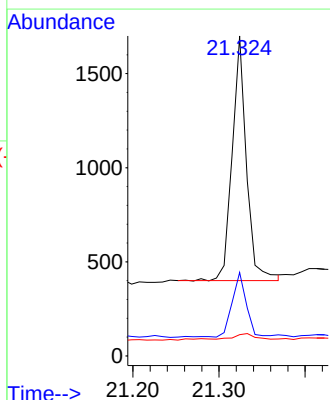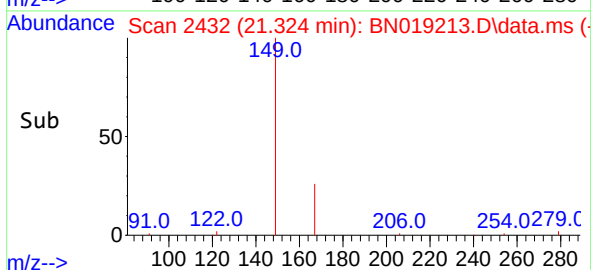

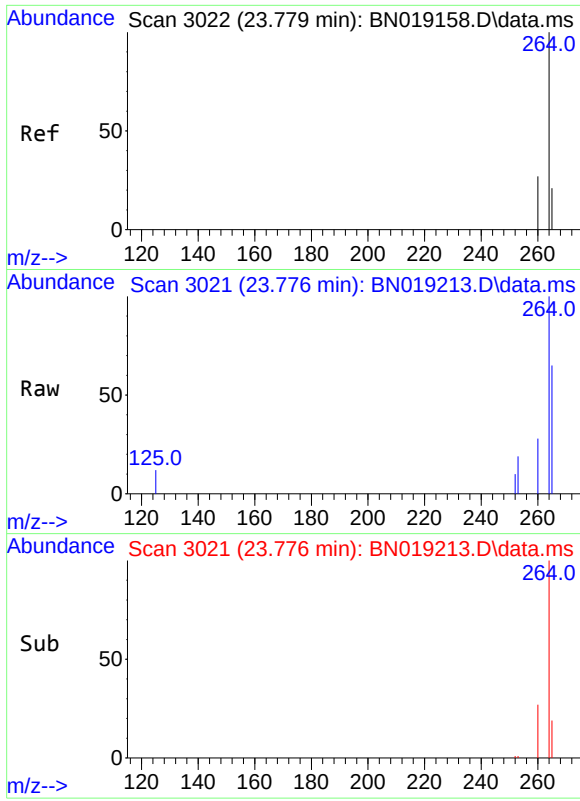

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.776 min Scan# 30
Delta R.T. -0.003 min
Lab File: BN019213.D
Acq: 29 Mar 2022 01:55

Instrument :
BNA_N
ClientSampleId :
GW-01-(SB-01)

Tgt Ion:264 Resp: 612
Ion Ratio Lower Upper
264 100
260 28.5 22.4 33.6
265 65.1 25.3 37.9

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/29/2022
Supervised By :Jagrut Upadhyay 03/29/2022

