
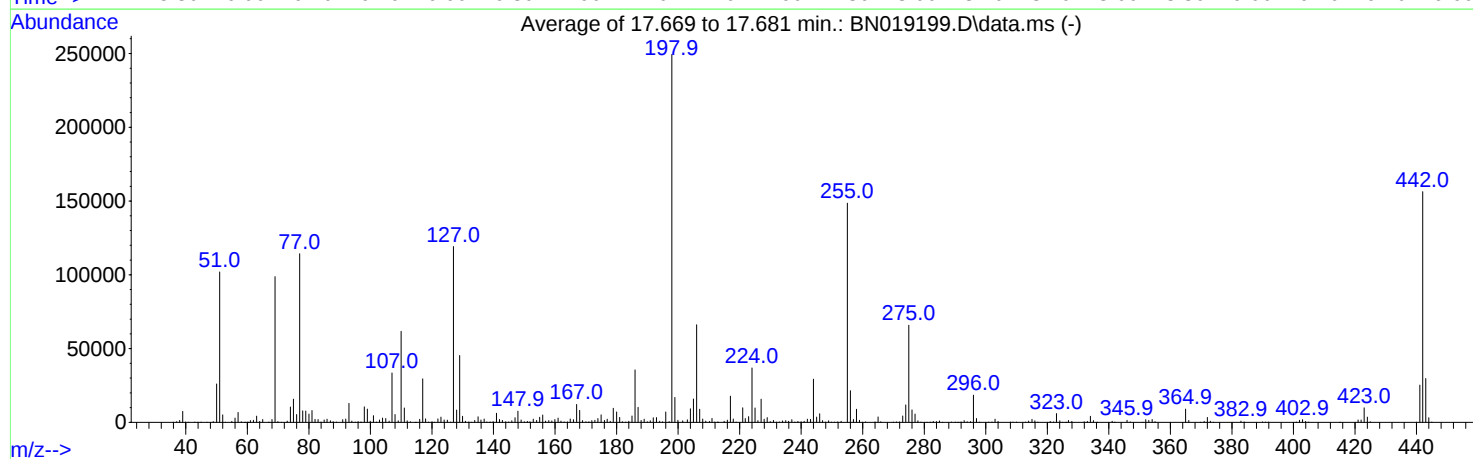


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
 Data File : BN019199.D
 Acq On : 28 Mar 2022 17:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 19:03:12 2022

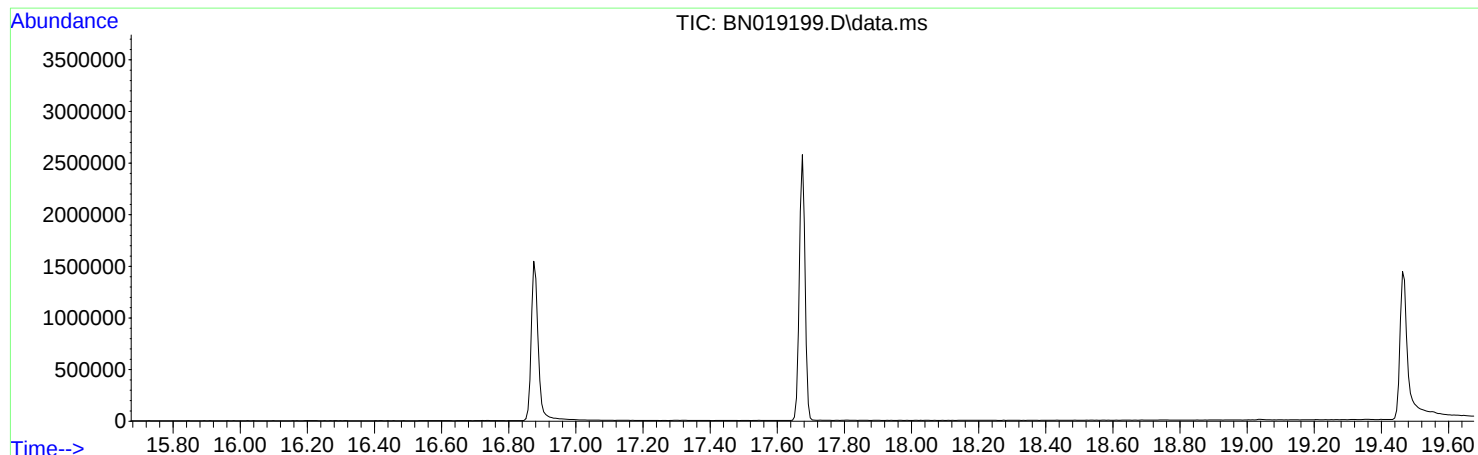




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	101990	PASS
68	69	0.00	2	1.9	1914	PASS
69	198	0.00	100	39.6	98835	PASS
70	69	0.00	2	0.5	532	PASS
127	198	10	80	47.8	119184	PASS
197	198	0.00	2	0.2	496	PASS
198	198	100	100	100.0	249323	PASS
199	198	5	9	6.8	16968	PASS
275	198	10	60	26.4	65848	PASS
365	198	1	100	3.6	8961	PASS
441	198	0.01	100	10.1	25280	PASS
442	442	50	100	100.0	156419	PASS
443	442	15	24	19.0	29760	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
 Data File : BN019199.D
 Acq On : 28 Mar 2022 17:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 08:49:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 08:49:42 2022
 Response via : Initial Calibration

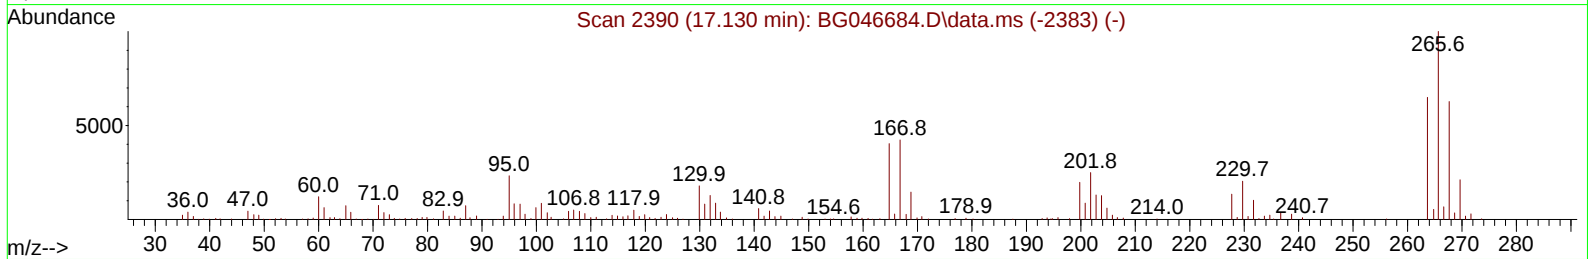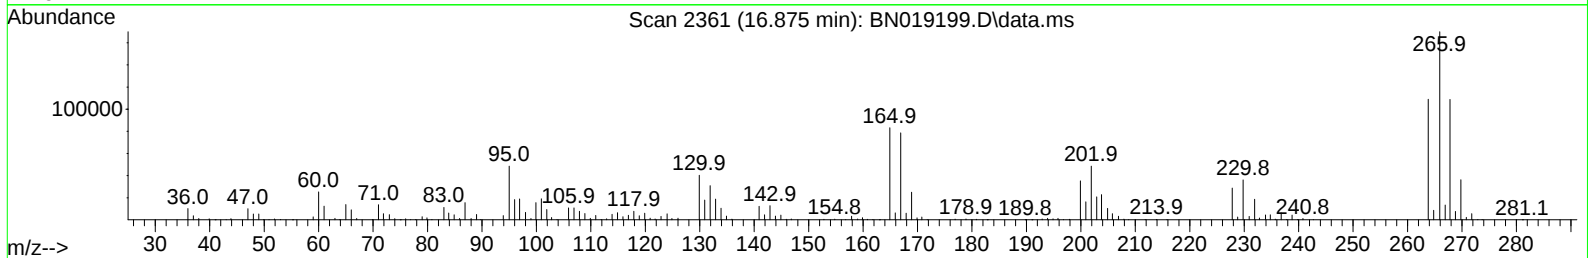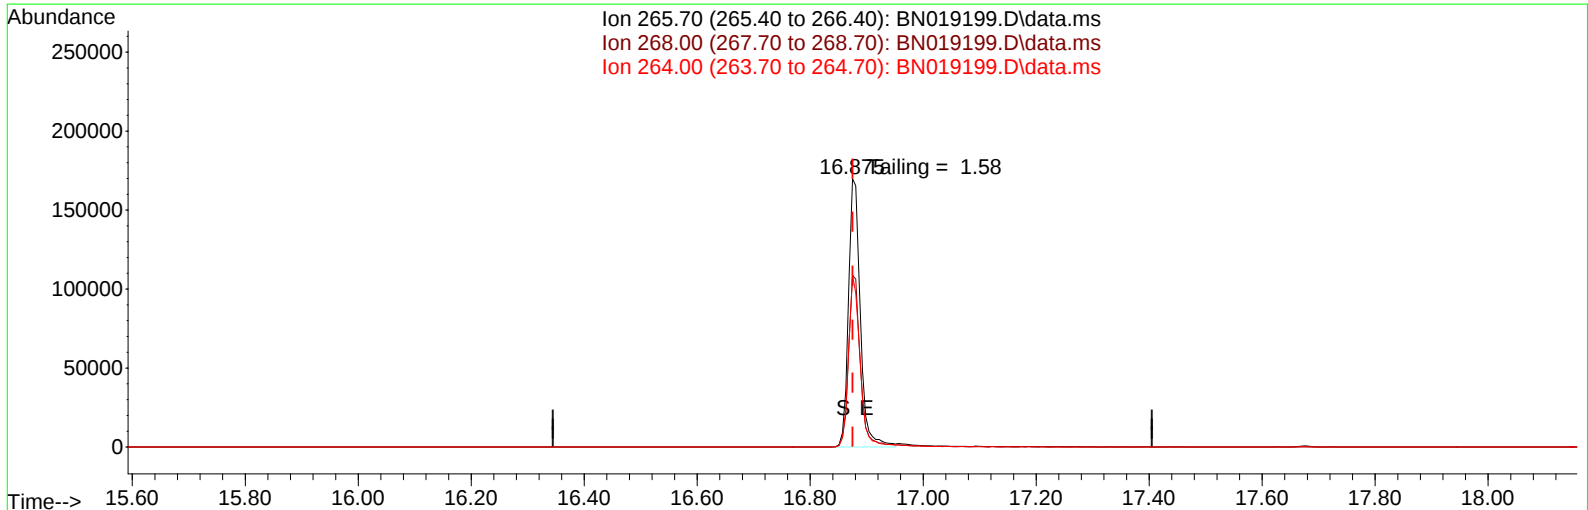

TIC: BN019199.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 18330.03 ng




response 254182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.06
264.00	61.60	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032822\
Data File : BN019199.D
Acq On : 28 Mar 2022 17:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 08:49:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 08:49:42 2022
Response via : Initial Calibration

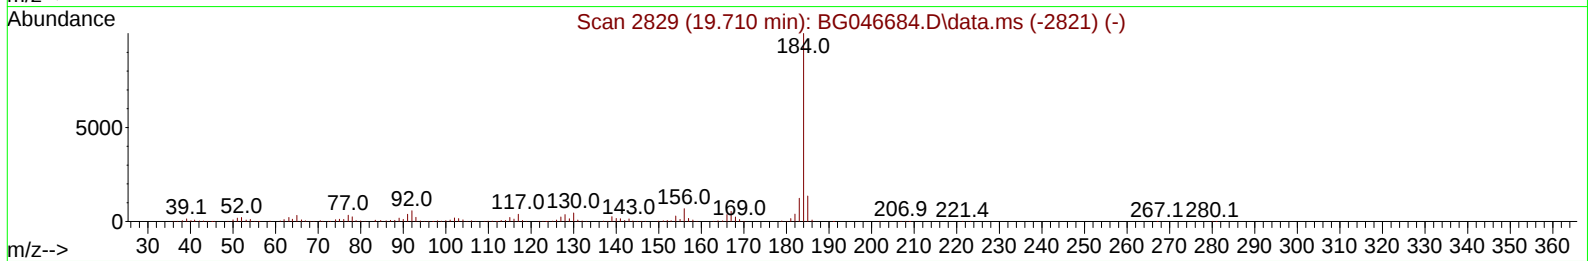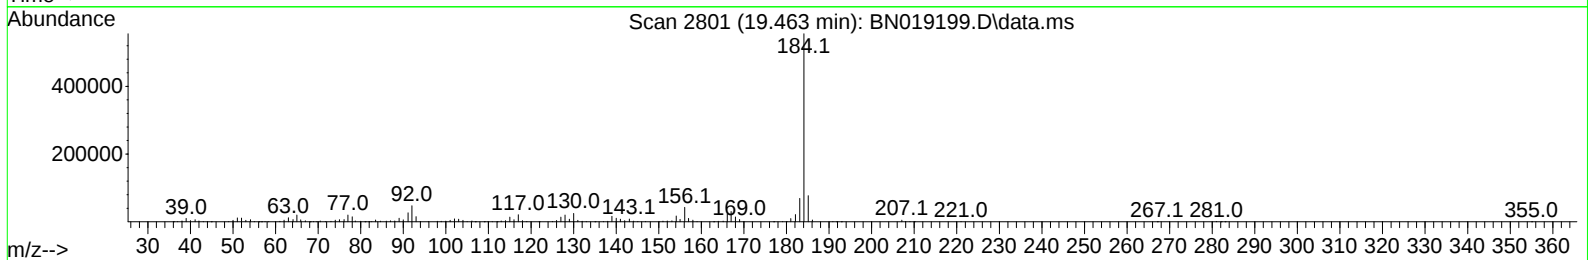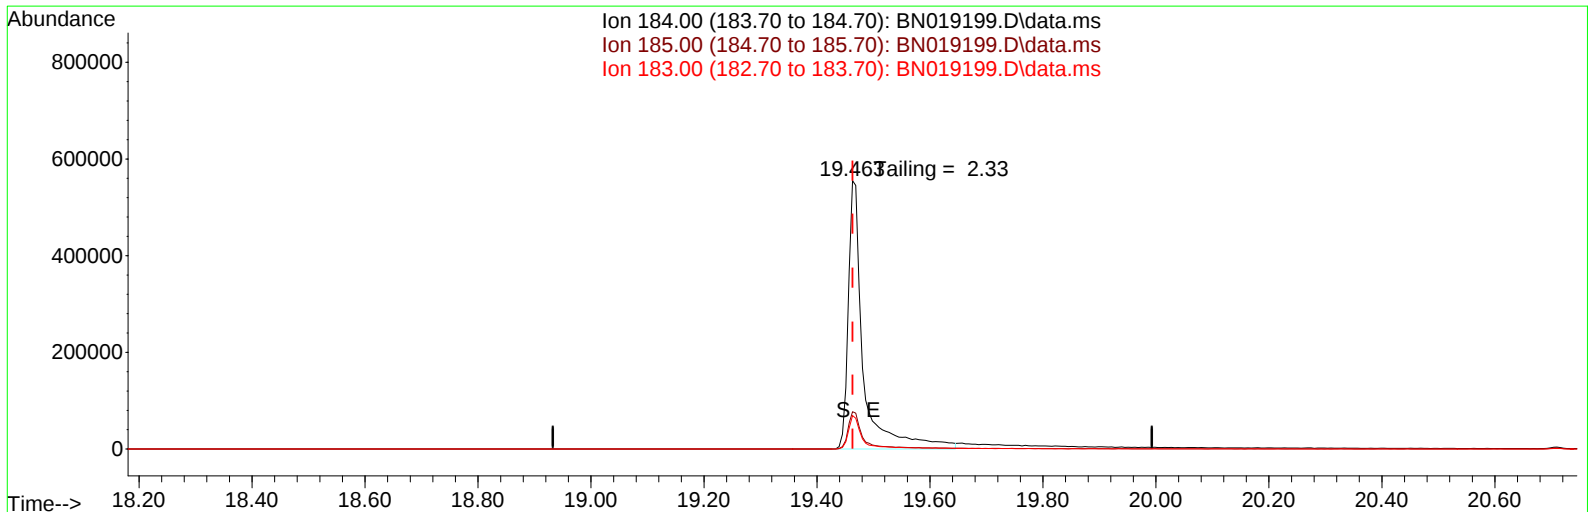

TIC: BN019199.D\data.ms

(77) Benzidine

19.463min (0.000) 0.00 ng

response 1068544

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2022	BNA_N	<u>BN019199.D</u>
Compound Name	Response	Retention Time
DDT	796572	20.71
DDD	22595	20.269
DDE	1712	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24307	820879	2.96

Instrument :
BNA_N
ClientSampleId :
DFTPP