

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024567.D
 Acq On : 27 Mar 2023 17:29
 Operator : CG/JU
 Sample : 02067-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ71

Quant Time: Mar 28 01:01:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 28 00:57:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	294028	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	1301157	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	793477	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1694771	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1577200	20.000	ng/ul	0.00
88) Perylene-d12	24.063	264	1616315	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	29420	3.903	ng/uL	0.00
4) Pyridine-d5	3.817	84	153570	7.363	ng/ul	0.00
7) Phenol-d5	7.169	99	146814	5.567	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	521985	30.906	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	441322	21.789	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	277443	13.233	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	289534	34.284	ng/ul	0.00
24) 2-Nitrophenol-d4	9.905	143	291331	31.634	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	494842	24.901	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	673242	22.707	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1854158	30.277	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	1966971	27.595	ng/ul	0.00
54) 4-Nitrophenol-d4	14.840	143	48211	4.120	ng/ul	0.00
60) Fluorene-d10	15.640	176	1575315	30.609	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	267930	29.343	ng/ul	0.00
73) Anthracene-d10	17.498	188	2735419	34.223	ng/ul	0.00
81) Pyrene-d10	19.786	212	3245757	35.212	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.904	264	2964246	36.892	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.757	113	9392	1.373	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024567.D
Acq On : 27 Mar 2023 17:29
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71

Quant Time: Mar 28 01:01:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 28 00:57:32 2023
Response via : Initial Calibration

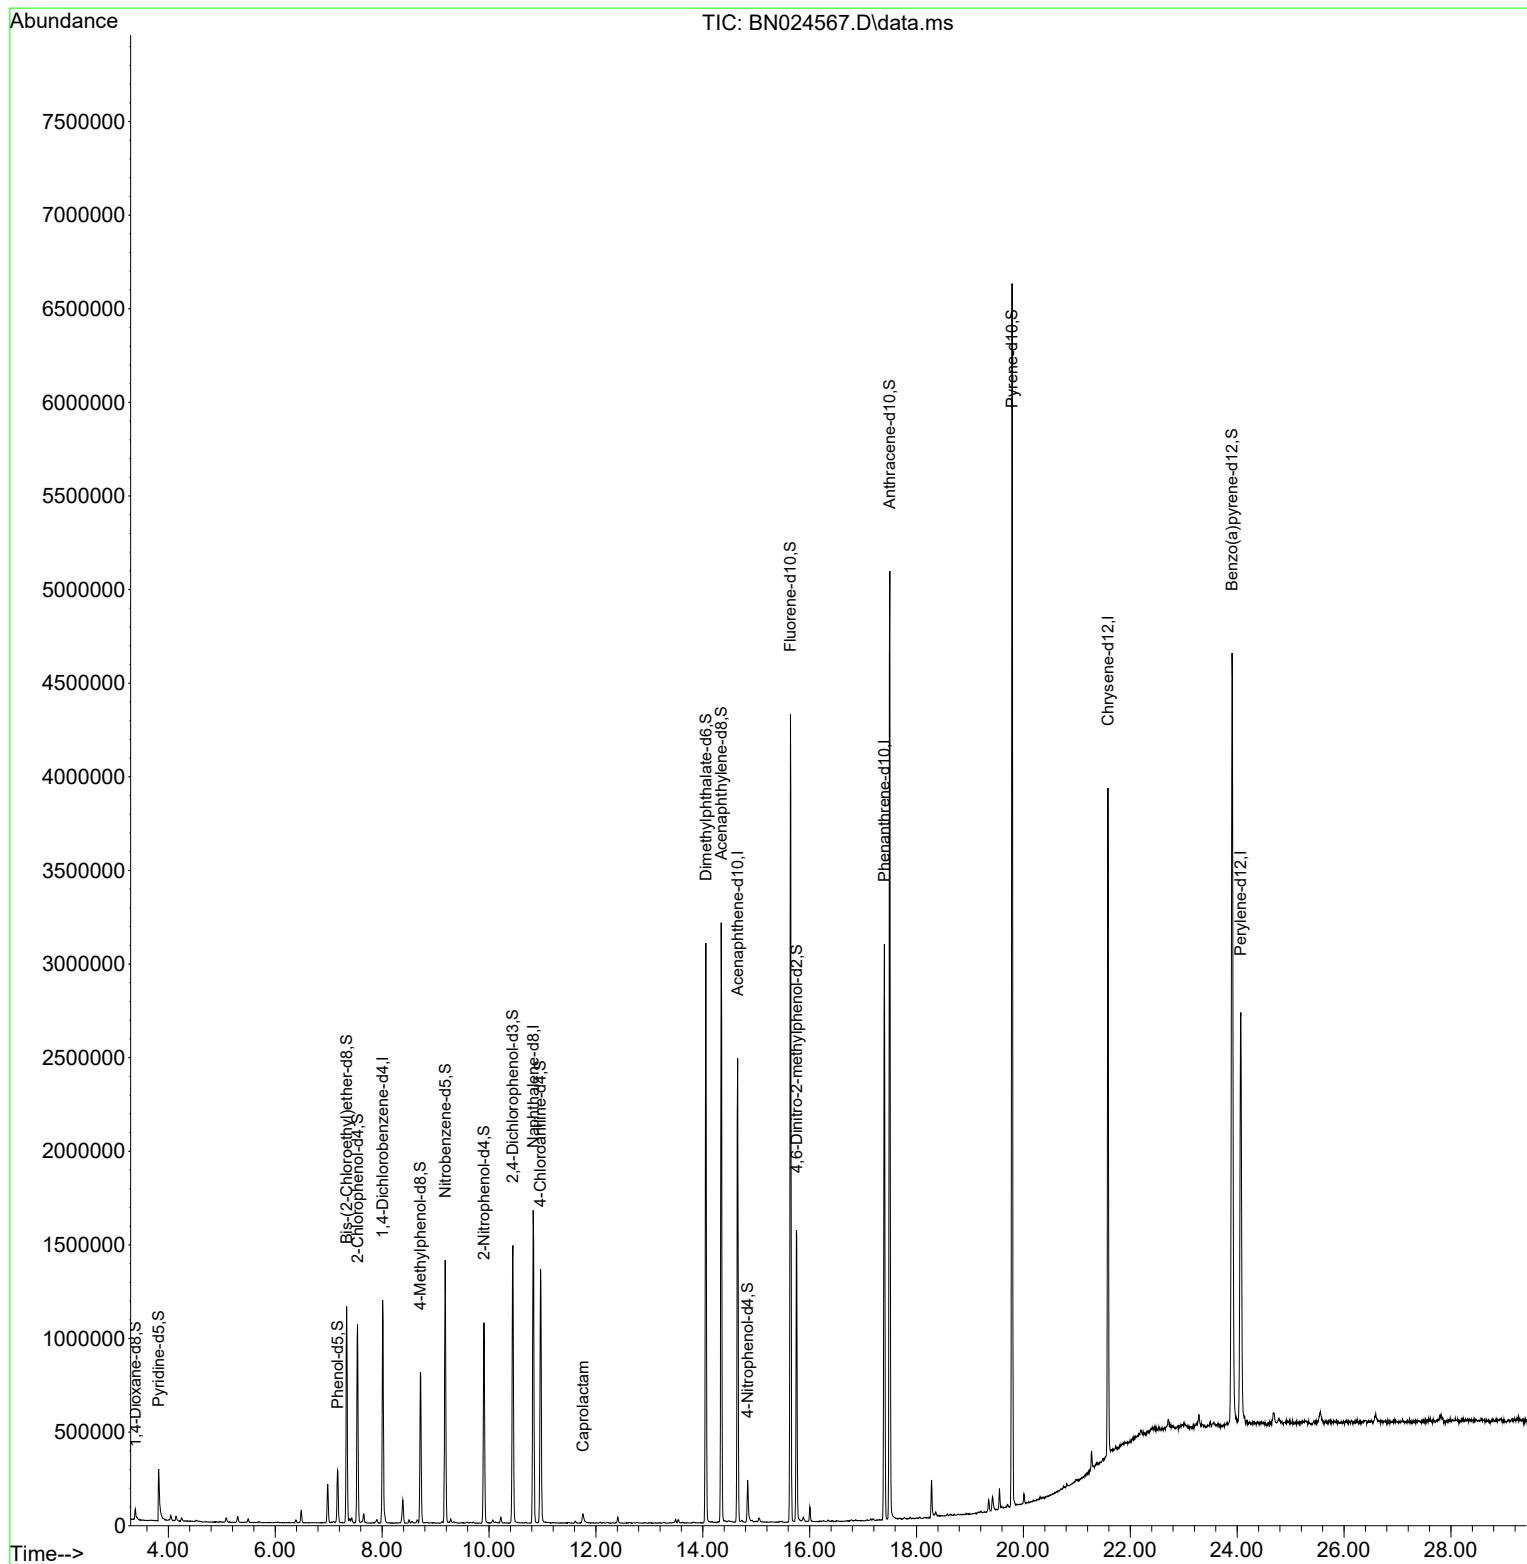

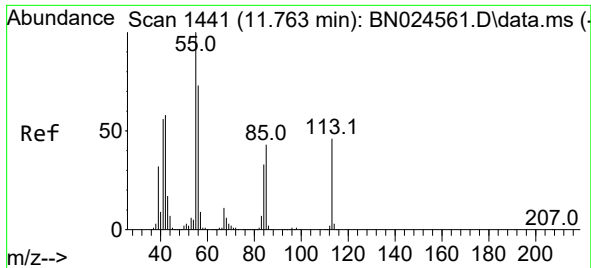

#34

Caprolactam

Concen: 1.373 ng/ul

RT: 11.757 min Scan# 14

Delta R.T. -0.006 min

Lab File: BN024567.D


Acq: 27 Mar 2023 17:29

Instrument :

BNA_N

ClientSampleId :

BFZ71

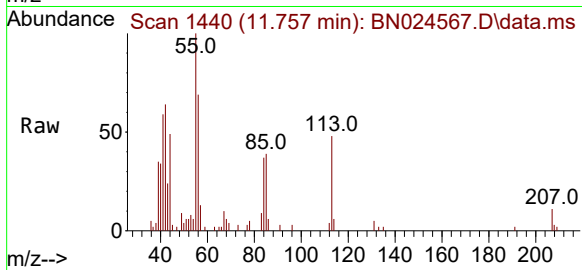

Tgt Ion:113 Resp: 9392

Ion Ratio Lower Upper

113 100

55 207.1 155.4 233.2

56 141.9 111.0 166.6

