

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024568.D
 Acq On : 27 Mar 2023 18:06
 Operator : CG/JU
 Sample : 02067-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ72

Quant Time: Mar 28 01:01:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 28 00:57:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	265866	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	1163424	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	712169	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1545822	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1399806	20.000	ng/ul	0.00
88) Perylene-d12	24.092	264	1541730	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	35296	5.179	ng/uL	0.00
4) Pyridine-d5	3.817	84	129492	6.866	ng/ul	0.00
7) Phenol-d5	7.169	99	153061	6.418	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	521533	34.150	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	448140	24.469	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	292339	15.420	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	289201	38.299	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	290309	35.255	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	491384	27.654	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	614235	23.170	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1813662	32.997	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	1990193	31.108	ng/ul	0.00
54) 4-Nitrophenol-d4	14.839	143	48414	4.610	ng/ul	0.00
60) Fluorene-d10	15.639	176	1594057	34.509	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	240614	28.891	ng/ul	0.00
73) Anthracene-d10	17.498	188	2677670	36.729	ng/ul	0.00
81) Pyrene-d10	19.786	212	3055731	37.352	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.915	264	3002876	39.181	ng/ul	0.01
Target Compounds						
34) Caprolactam	11.757	113	11034	1.804	ng/ul	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024568.D
Acq On : 27 Mar 2023 18:06
Operator : CG/JU
Sample : 02067-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ72

Quant Time: Mar 28 01:01:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 28 00:57:32 2023
Response via : Initial Calibration

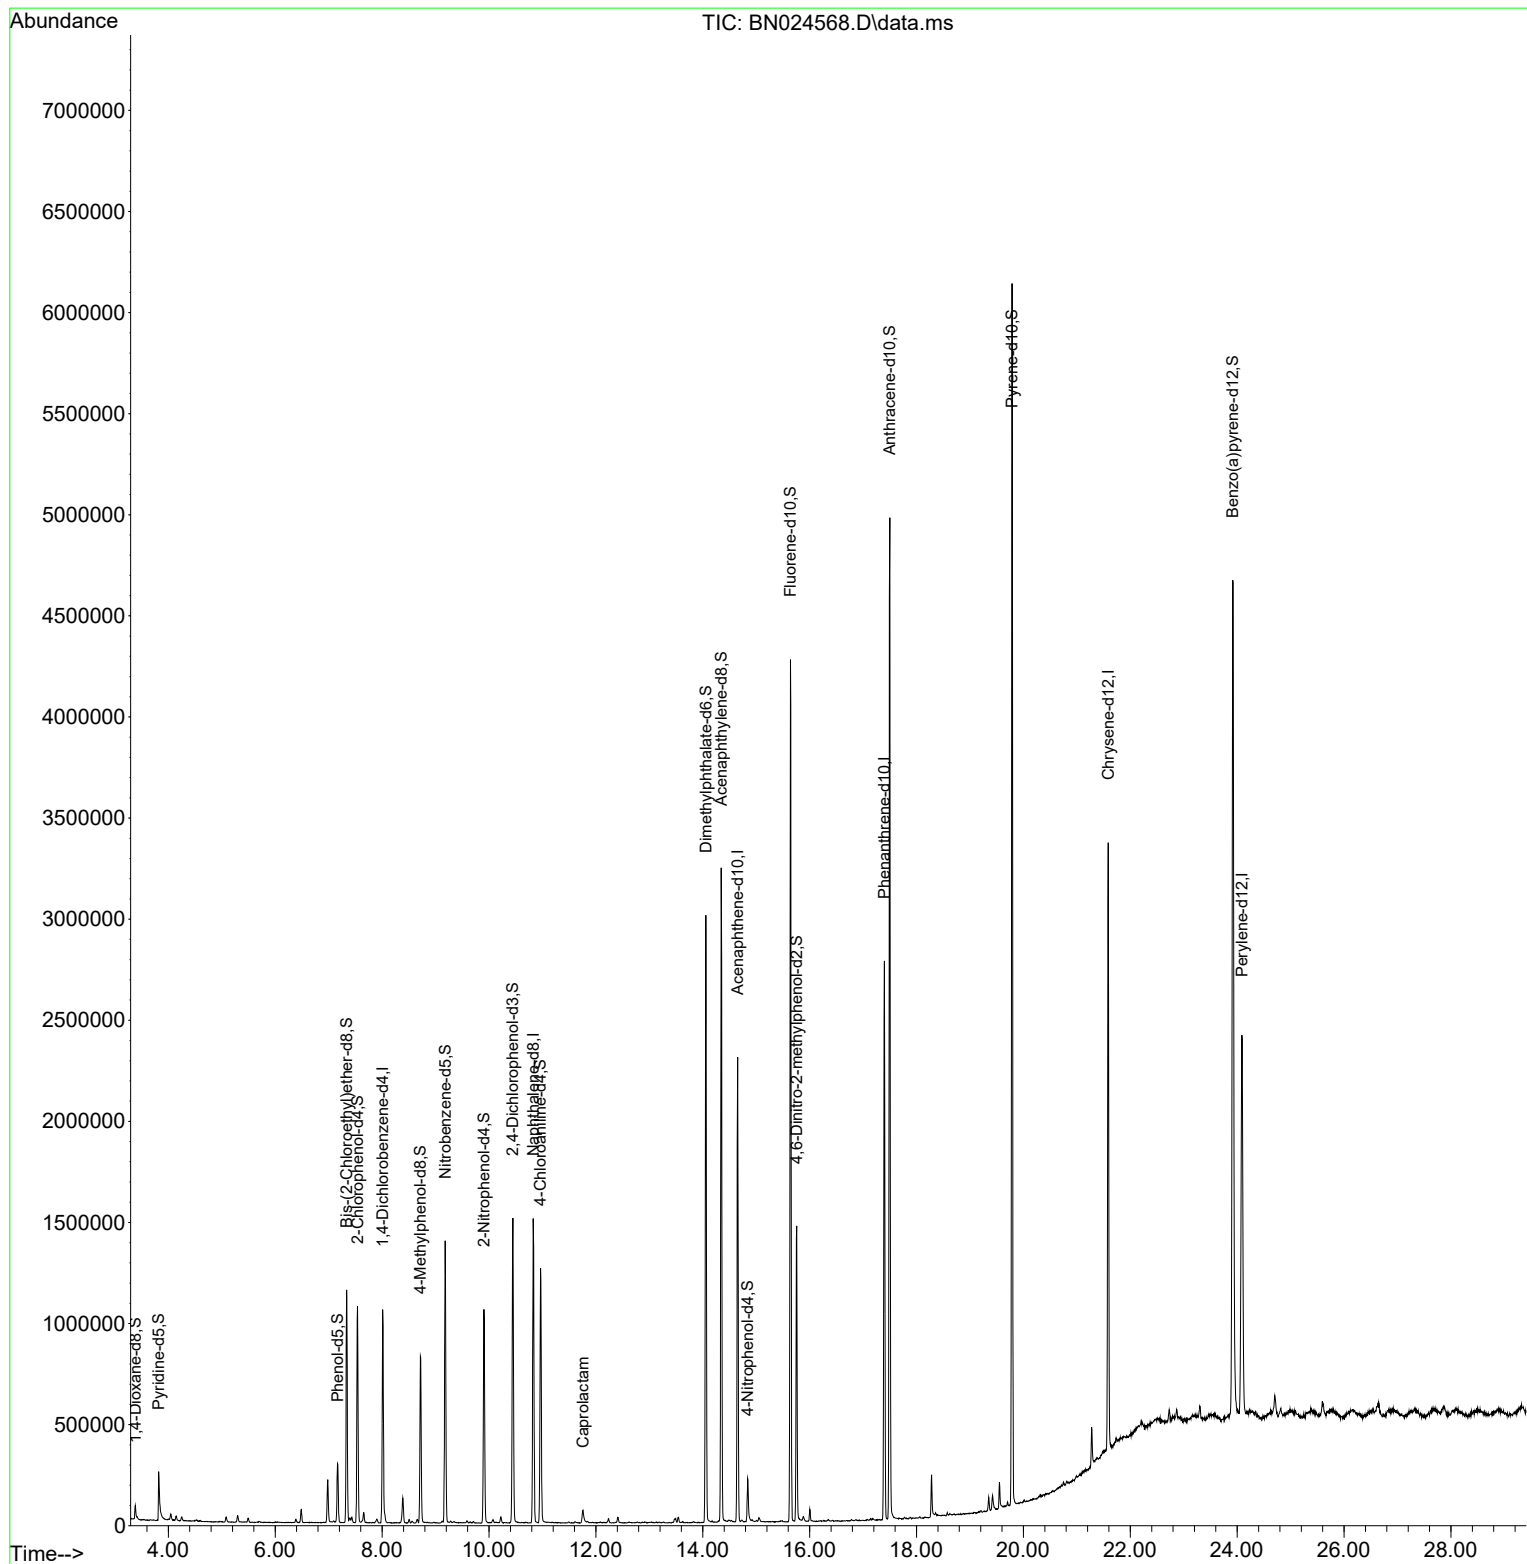

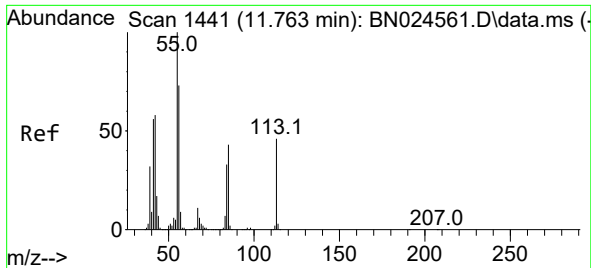

#34

Caprolactam

Concen: 1.804 ng/ul

RT: 11.757 min Scan# 14

Delta R.T. -0.006 min

Lab File: BN024568.D


Acq: 27 Mar 2023 18:06

Instrument :

BNA_N

ClientSampleId :

BFZ72

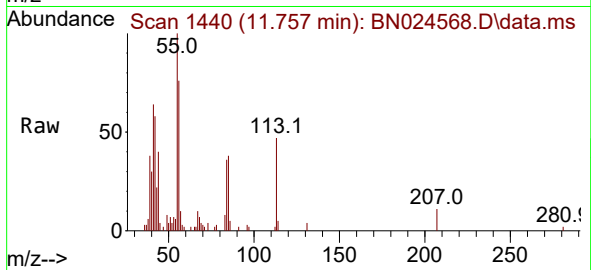

Tgt Ion:113 Resp: 11034

Ion Ratio Lower Upper

113 100

55 214.8 155.4 233.2

56 162.9 111.0 166.6

