

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024567.D
 Acq On : 27 Mar 2023 17:29
 Operator : CG/JU
 Sample : 02067-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	21	rBV	55559	79416	0.91%	0.098%
2	3.817	88	90	111	rBV	275777	527068	6.02%	0.649%
3	4.046	124	129	135	rVB2	27160	46282	0.53%	0.057%
4	4.140	141	145	157	rVB	27123	46706	0.53%	0.058%
5	4.246	159	163	169	rBV6	18352	31080	0.35%	0.038%
6	4.522	206	210	218	rVB8	6175	11527	0.13%	0.014%
7	5.081	300	305	311	rBV2	22740	38183	0.44%	0.047%
8	5.293	334	341	350	rBV	31954	57970	0.66%	0.071%
9	5.493	371	375	381	rVB2	19791	30663	0.35%	0.038%
10	6.387	522	527	533	rVB	15718	24918	0.28%	0.031%
11	6.487	538	544	552	rVB	65776	104962	1.20%	0.129%
12	6.981	621	628	636	rBV	206568	321406	3.67%	0.396%
13	7.093	642	647	651	rVB5	6045	9340	0.11%	0.012%
14	7.163	651	659	671	rVB	281739	467901	5.34%	0.576%
15	7.334	681	688	695	rBV	1154837	1820717	20.78%	2.243%
16	7.393	695	698	701	rVV	22548	35993	0.41%	0.044%
17	7.428	701	704	711	rVB	27092	42574	0.49%	0.052%
18	7.540	716	723	732	rBV	1058062	1690383	19.29%	2.083%
19	7.652	732	742	747	rVB	47162	86051	0.98%	0.106%
20	7.905	777	785	790	rVB4	17916	35665	0.41%	0.044%
21	8.011	794	803	818	rBV	1192411	1968922	22.47%	2.426%
22	8.387	859	867	875	rVB	124121	216921	2.48%	0.267%
23	8.505	882	887	892	rBV2	17826	26740	0.31%	0.033%
24	8.558	892	896	905	rVB7	9053	15465	0.18%	0.019%
25	8.652	909	912	917	rVV2	16172	25386	0.29%	0.031%
26	8.716	917	923	934	rVV	804427	1287492	14.69%	1.586%
27	9.122	986	992	995	rBV6	8526	14931	0.17%	0.018%
28	9.181	995	1002	1012	rVV	1403499	2239873	25.56%	2.760%
29	9.281	1015	1019	1025	rVV2	20766	32159	0.37%	0.040%
30	9.705	1088	1091	1098	rVB5	7295	12957	0.15%	0.016%
31	9.905	1117	1125	1137	rBV	1070945	1749099	19.96%	2.155%
32	10.069	1147	1153	1159	rBV	16272	29051	0.33%	0.036%
33	10.222	1174	1179	1185	rVB2	30428	47525	0.54%	0.059%
34	10.446	1207	1217	1229	rBV	1483663	2461341	28.09%	3.033%
35	10.828	1275	1282	1294	rBV	1670341	2809776	32.07%	3.462%
36	10.963	1297	1305	1316	rBV	1356362	2333581	26.63%	2.875%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024567.D
 Acq On : 27 Mar 2023 17:29
 Operator : CG/JU
 Sample : 02067-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ71

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

37	11.493	1390	1395	1398	rBV7	5407	9461	0.11%	0.012%
38	11.610	1410	1415	1418	rBV4	11896	18863	0.22%	0.023%
39	11.757	1433	1440	1452	rBV	47863	116943	1.33%	0.144%
40	12.410	1546	1551	1560	rVB2	30118	43299	0.49%	0.053%
41	13.493	1729	1735	1739	rVV2	17457	25027	0.29%	0.031%
42	13.540	1739	1743	1749	rVV2	17124	28019	0.32%	0.035%
43	14.057	1823	1831	1844	rBV	3097563	4167377	47.56%	5.135%
44	14.345	1873	1880	1888	rBV	3200746	4645751	53.02%	5.724%
45	14.651	1925	1932	1939	rBV	2476527	3644611	41.60%	4.490%
46	14.728	1941	1945	1953	rVB10	9441	18409	0.21%	0.023%
47	14.840	1957	1964	1974	rBV	225537	384855	4.39%	0.474%
48	14.922	1976	1978	1983	rVB5	9126	10874	0.12%	0.013%
49	15.051	1996	2000	2006	rBV6	21908	38812	0.44%	0.048%
50	15.640	2093	2100	2112	rBV	4313699	6047775	69.02%	7.451%
51	15.751	2113	2119	2132	rVV	1556574	2168021	24.74%	2.671%
52	15.881	2136	2141	2148	rVB4	23781	47505	0.54%	0.059%
53	16.004	2156	2162	2167	rBV	77311	102718	1.17%	0.127%
54	16.345	2216	2220	2223	rBV6	6712	9274	0.11%	0.011%
55	17.145	2350	2356	2358	rBV6	9840	14958	0.17%	0.018%
56	17.186	2359	2363	2369	rVB4	9553	15722	0.18%	0.019%
57	17.398	2392	2399	2409	rBV	3076503	4306943	49.16%	5.307%
58	17.498	2409	2416	2434	rVV2	5064274	7339661	83.77%	9.043%
59	17.881	2477	2481	2485	rBV5	8826	11257	0.13%	0.014%
60	18.063	2508	2512	2517	rBV7	8131	11717	0.13%	0.014%
61	18.281	2544	2549	2558	rBV	203551	309189	3.53%	0.381%
62	18.357	2560	2562	2568	rVB	24222	35975	0.41%	0.044%
63	19.351	2727	2731	2736	rVB2	60264	83633	0.95%	0.103%
64	19.422	2738	2743	2753	rBV	77056	156269	1.78%	0.193%
65	19.551	2761	2765	2769	rBV	108754	135696	1.55%	0.167%
66	19.704	2788	2791	2796	rBV5	16373	22228	0.25%	0.027%
67	19.786	2799	2805	2816	rBV	6532051	8761788	100.00%	10.795%
68	20.010	2840	2843	2848	rVB	52432	62519	0.71%	0.077%
69	21.275	3055	3058	3062	rBV2	94950	117691	1.34%	0.145%
70	21.580	3105	3110	3119	rBV	3566149	4573563	52.20%	5.635%
71	23.904	3498	3505	3518	rVB	4095158	8400661	95.88%	10.350%
72	24.068	3526	3533	3544	rVB2	2166790	4495828	51.31%	5.539%




Sum of corrected areas: 81162916

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024567.D
Acq On : 27 Mar 2023 17:29
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

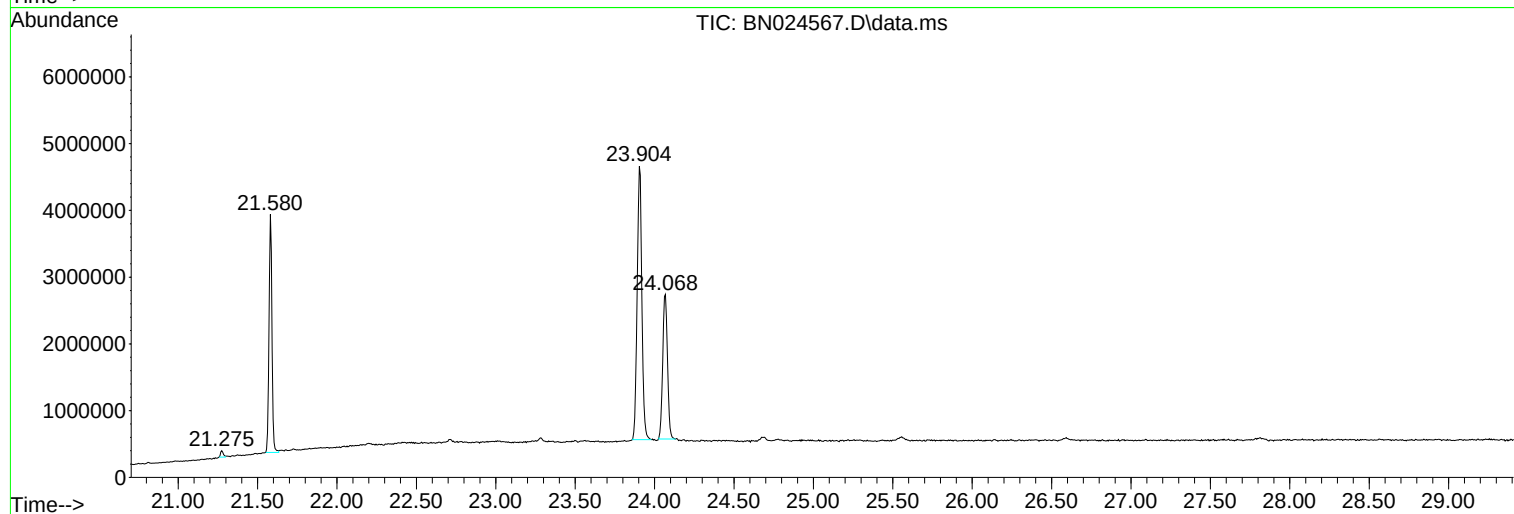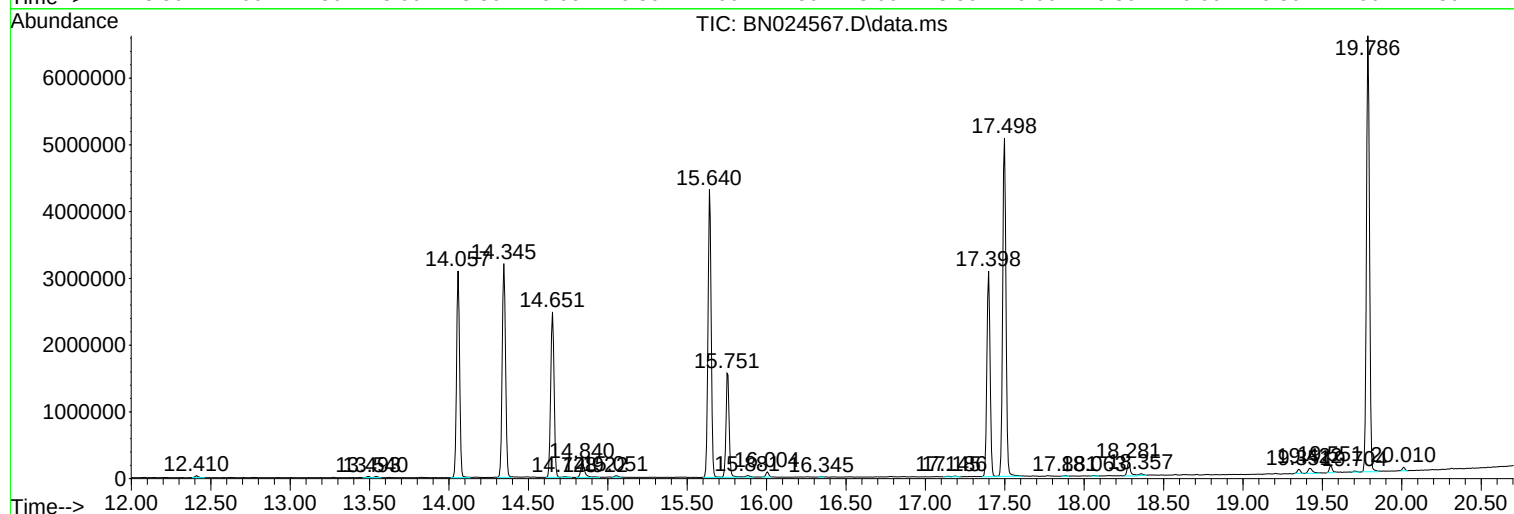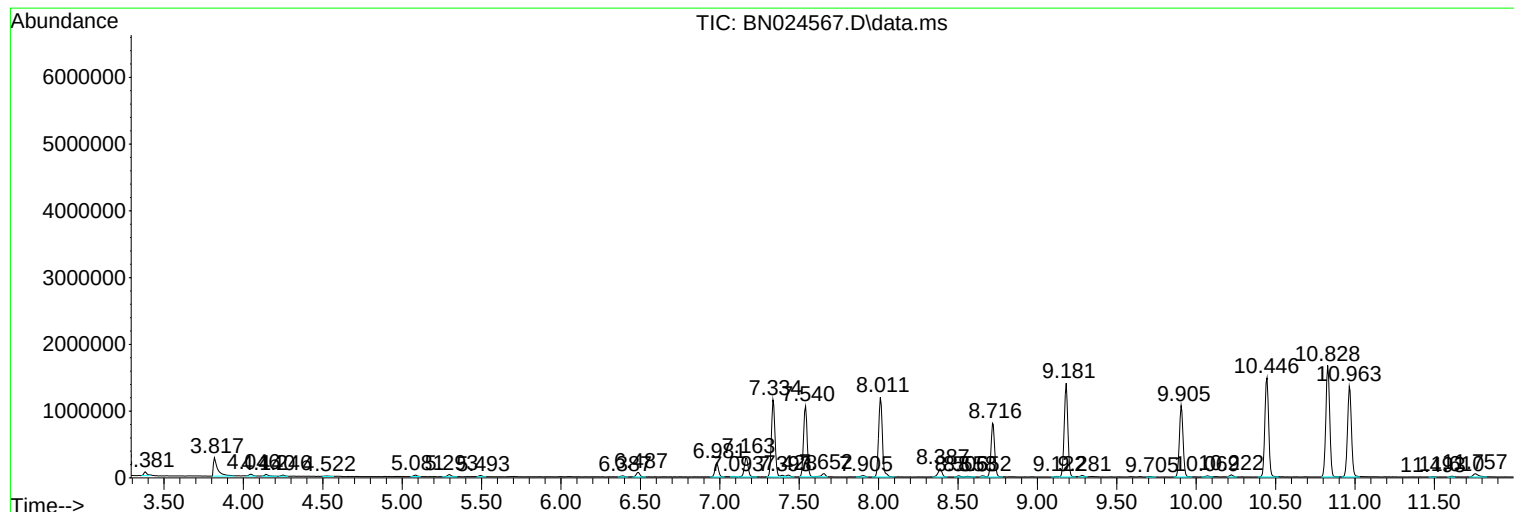

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024567.D
Acq On : 27 Mar 2023 17:29
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, propyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.981	3.26 ng/ul	321406	1,4-Dichlorobenzene-d4	8.011

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, propyl-	120	C9H12	000103-65-1	93
2			Benzene, propyl-	120	C9H12	000103-65-1	90
3			Benzene, propyl-	120	C9H12	000103-65-1	87
4			Benzene, propyl-	120	C9H12	000103-65-1	83
5			N-Benzyl-2-phenethylamine	211	C15H17N	003647-71-0	78

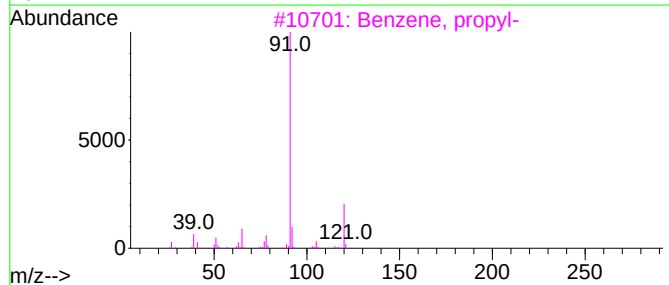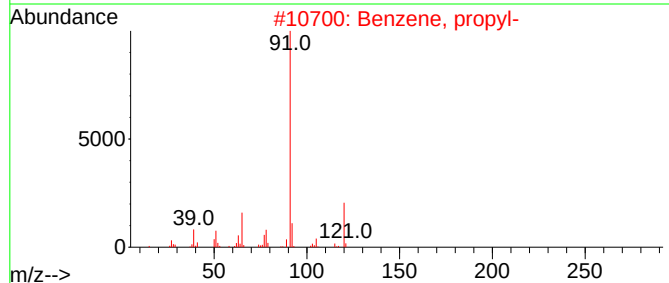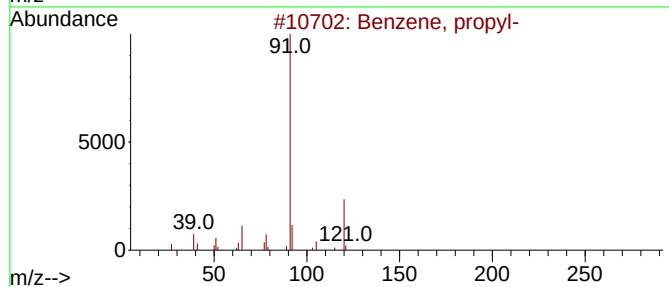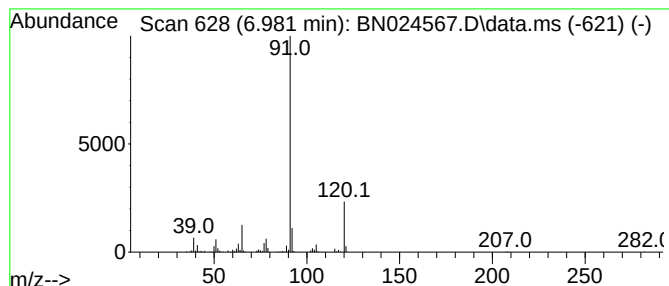

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024567.D
Acq On : 27 Mar 2023 17:29
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.387	2.20 ng/ul	216921	1,4-Dichlorobenzene-d4	8.011

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Indane			118	C9H10	000496-11-7	95
2	Indane			118	C9H10	000496-11-7	87
3	Tetracyclo[3.3.1.0(2,8).0(4,6)]-...			118	C9H10	1000191-13-7	83
4	Indane			118	C9H10	000496-11-7	81
5	Benzene, cyclopropyl-			118	C9H10	000873-49-4	80

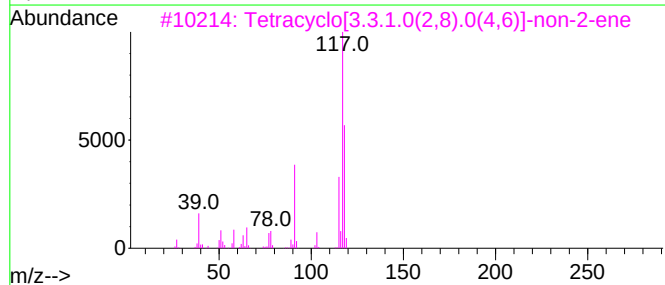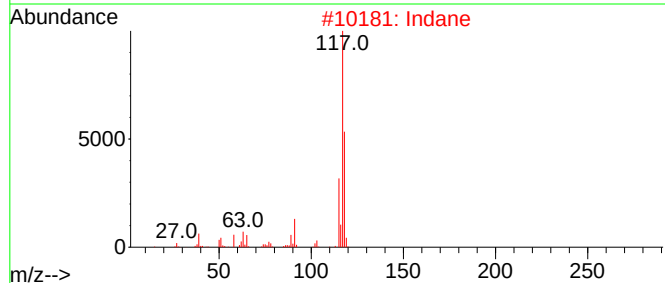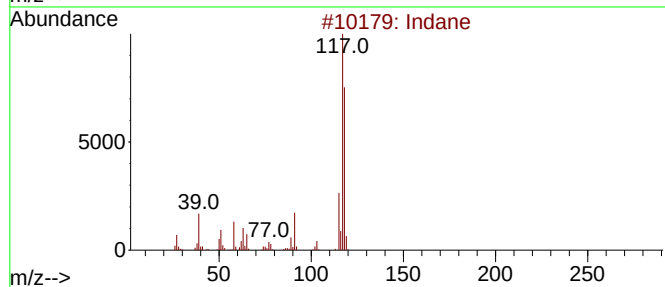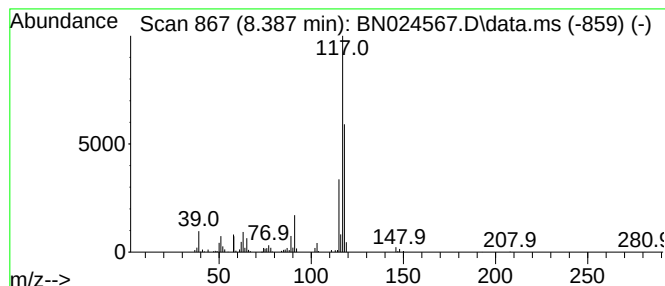

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024567.D
Acq On : 27 Mar 2023 17:29
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, propyl-	6.981	3.3	ng/u1	321406	1	8.011	1968920	20.0
Indane	8.387	2.2	ng/u1	216921	1	8.011	1968920	20.0