

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024569.D
 Acq On : 27 Mar 2023 18:42
 Operator : CG/JU
 Sample : 02067-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024569.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.382	12	16	28	rVB	60046	100544	1.24%	0.130%
2	3.817	87	90	108	rBV	283144	531038	6.54%	0.689%
3	4.046	124	129	135	rVB	31179	50080	0.62%	0.065%
4	4.146	141	146	155	rVB	23814	40246	0.50%	0.052%
5	4.246	159	163	170	rVB3	17104	27216	0.33%	0.035%
6	4.529	205	211	216	rVB8	6936	11660	0.14%	0.015%
7	5.081	299	305	315	rVB	26770	46944	0.58%	0.061%
8	5.293	337	341	346	rVB5	10972	17892	0.22%	0.023%
9	6.387	522	527	533	rVB2	20298	27235	0.34%	0.035%
10	6.981	623	628	632	rBV6	7303	13262	0.16%	0.017%
11	7.164	653	659	671	rVB	320425	531793	6.54%	0.690%
12	7.334	681	688	702	rBV	1143851	1840419	22.65%	2.388%
13	7.540	716	723	731	rBV	1134201	1783004	21.94%	2.314%
14	7.617	734	736	744	rVB5	8485	15157	0.19%	0.020%
15	7.899	780	784	790	rVB3	13406	20562	0.25%	0.027%
16	8.011	796	803	812	rBV	1034183	1669088	20.54%	2.166%
17	8.722	917	924	932	rBV	897860	1441315	17.74%	1.871%
18	9.181	993	1002	1011	rBV	1418973	2287558	28.15%	2.969%
19	9.281	1015	1019	1024	rVV3	13266	24271	0.30%	0.031%
20	9.587	1067	1071	1076	rVB5	6103	9730	0.12%	0.013%
21	9.905	1114	1125	1137	rBV	1079094	1779502	21.90%	2.309%
22	10.446	1208	1217	1230	rBV	1531426	2527612	31.11%	3.280%
23	10.693	1253	1259	1265	rVB	48160	80841	0.99%	0.105%
24	10.828	1274	1282	1290	rBV	1444870	2448476	30.13%	3.178%
25	10.963	1296	1305	1321	rBV	1416907	2481694	30.54%	3.221%
26	11.216	1341	1348	1353	rVB2	28701	46548	0.57%	0.060%
27	11.610	1410	1415	1419	rBV5	10114	16499	0.20%	0.021%
28	12.234	1516	1521	1527	rBV3	11178	19255	0.24%	0.025%
29	12.410	1546	1551	1557	rVB	32499	51886	0.64%	0.067%
30	13.469	1726	1731	1736	rVB4	10354	16574	0.20%	0.022%
31	13.540	1738	1743	1747	rVB3	7702	11985	0.15%	0.016%
32	14.057	1824	1831	1841	rBV	3121679	4162704	51.23%	5.402%
33	14.169	1847	1850	1856	rVB7	5932	10702	0.13%	0.014%
34	14.281	1864	1869	1873	rBV6	4694	9319	0.11%	0.012%
35	14.346	1873	1880	1892	rVV	3338066	4855745	59.76%	6.302%
36	14.493	1901	1905	1909	rBV5	6638	10879	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024569.D
 Acq On : 27 Mar 2023 18:42
 Operator : CG/JU
 Sample : 02067-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

37	14.534	1909	1912	1917	rVB2	16953	24889	0.31%	0.032%
38	14.652	1925	1932	1940	rBV	2184899	3177465	39.10%	4.124%
39	14.734	1943	1946	1953	rVB8	8319	15122	0.19%	0.020%
40	14.840	1958	1964	1981	rBV	237213	426191	5.24%	0.553%
41	15.063	1996	2002	2005	rBV7	7275	12404	0.15%	0.016%
42	15.151	2013	2017	2021	rBV6	6750	8443	0.10%	0.011%
43	15.487	2066	2074	2078	rVB2	53267	70019	0.86%	0.091%
44	15.640	2093	2100	2113	rBV	4392250	6193519	76.22%	8.038%
45	15.757	2113	2120	2130	rBV	1452775	2000547	24.62%	2.596%
46	15.887	2136	2142	2147	rVB4	31479	59634	0.73%	0.077%
47	16.004	2156	2162	2166	rBV	31514	46532	0.57%	0.060%
48	16.040	2166	2168	2173	rVV5	7138	10728	0.13%	0.014%
49	16.110	2176	2180	2185	rVB8	6620	8588	0.11%	0.011%
50	16.346	2215	2220	2230	rBV	83791	151658	1.87%	0.197%
51	16.422	2230	2233	2237	rVB5	6360	8729	0.11%	0.011%
52	16.693	2275	2279	2281	rBV5	5935	10005	0.12%	0.013%
53	16.857	2302	2307	2311	rBV8	8197	15050	0.19%	0.020%
54	17.140	2351	2355	2360	rVV	64633	82339	1.01%	0.107%
55	17.193	2360	2364	2369	rVB3	22179	33231	0.41%	0.043%
56	17.398	2392	2399	2408	rBV	2596045	3792981	46.68%	4.922%
57	17.498	2409	2416	2428	rVV	4899228	6990879	86.03%	9.073%
58	17.675	2442	2446	2454	rVB	81416	110500	1.36%	0.143%
59	17.881	2477	2481	2486	rBV	43566	53285	0.66%	0.069%
60	18.057	2508	2511	2517	rVB2	33454	42900	0.53%	0.056%
61	18.281	2544	2549	2554	rBV	93168	139235	1.71%	0.181%
62	18.575	2595	2599	2603	rBV	27749	30665	0.38%	0.040%
63	19.204	2703	2706	2709	rBV2	17755	20812	0.26%	0.027%
64	19.351	2726	2731	2736	rBV2	70562	105911	1.30%	0.137%
65	19.422	2738	2743	2748	rBV	67810	106637	1.31%	0.138%
66	19.551	2762	2765	2771	rBV3	48885	63471	0.78%	0.082%
67	19.787	2799	2805	2814	rBV	6139832	8083490	99.48%	10.491%
68	21.275	3056	3058	3065	rVB4	69876	82883	1.02%	0.108%
69	21.586	3105	3111	3118	rBV	2934670	3965932	48.81%	5.147%
70	23.922	3501	3508	3526	rVB	4175401	8125983	100.00%	10.546%
71	24.086	3528	3536	3546	rVB2	1720550	3964713	48.79%	5.145%




Sum of corrected areas: 77054605

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024569.D
Acq On : 27 Mar 2023 18:42
Operator : CG/JU
Sample : 02067-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

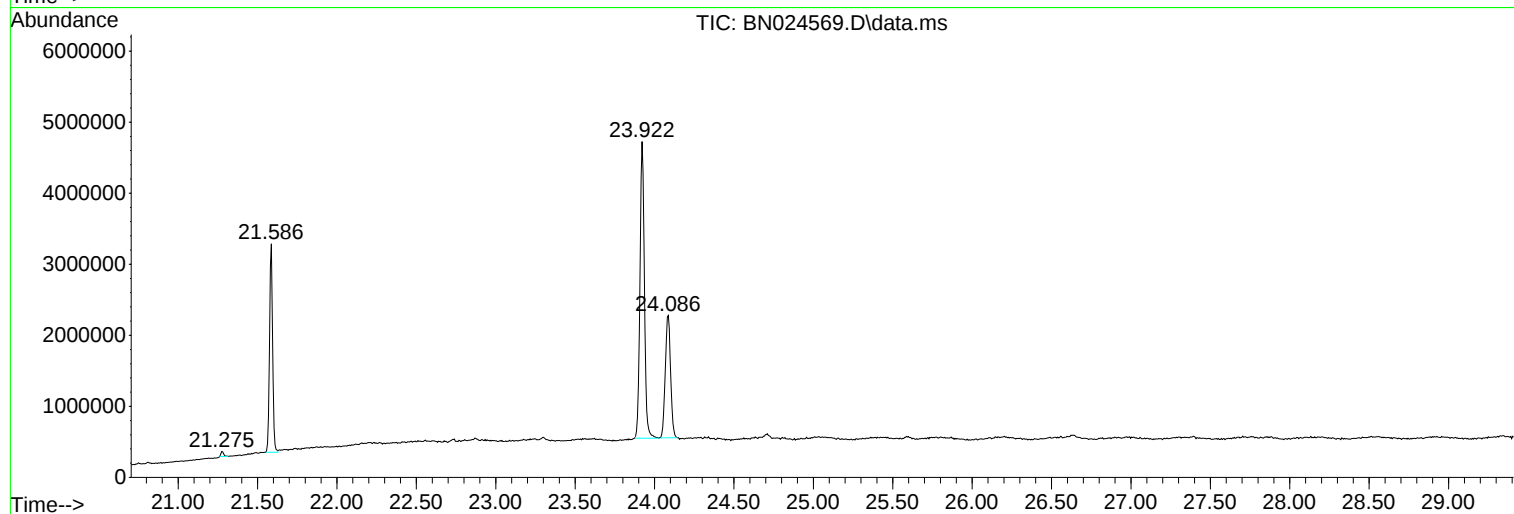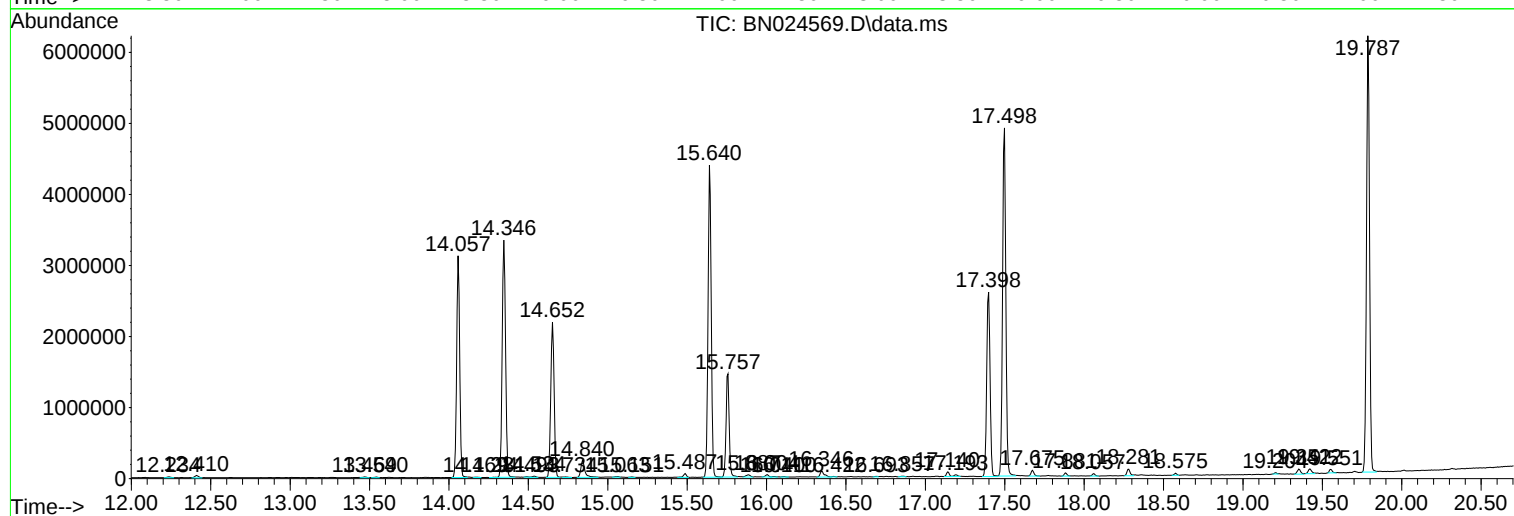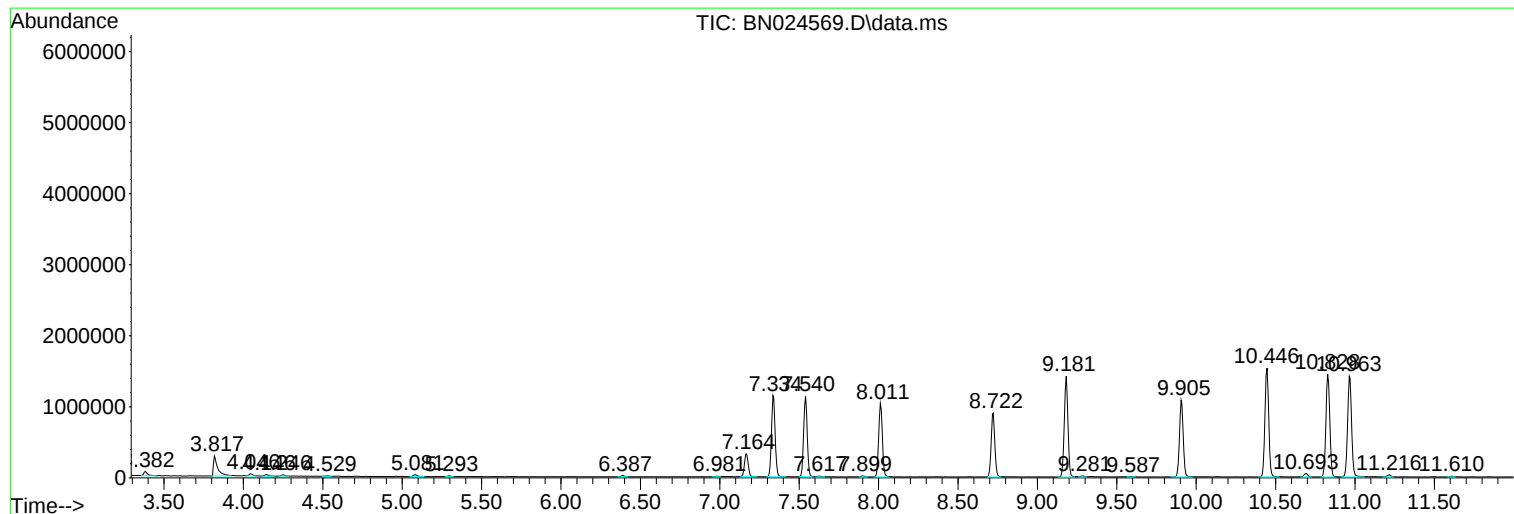

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024569.D
Acq On : 27 Mar 2023 18:42
Operator : CG/JU
Sample : 02067-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024569.D
Acq On : 27 Mar 2023 18:42
Operator : CG/JU
Sample : 02067-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc