

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024570.D
 Acq On : 27 Mar 2023 19:19
 Operator : CG/JU
 Sample : 02067-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	21	rBV	64351	92951	1.01%	0.107%
2	3.822	90	91	106	rBV	145438	258896	2.81%	0.298%
3	4.046	125	129	138	rVB	28384	48273	0.52%	0.056%
4	4.146	142	146	153	rVB2	25807	43881	0.48%	0.050%
5	4.252	159	164	172	rVB	30701	49067	0.53%	0.056%
6	4.522	208	210	216	rVB6	8420	14251	0.15%	0.016%
7	5.081	300	305	313	rBV2	22277	38732	0.42%	0.045%
8	5.299	336	342	349	rBV	58310	93879	1.02%	0.108%
9	6.005	456	462	467	rBV	14811	26092	0.28%	0.030%
10	6.387	521	527	535	rBV2	15783	28068	0.30%	0.032%
11	7.169	651	660	669	rVB	295296	482761	5.24%	0.555%
12	7.340	682	689	697	rBV	1148341	1869134	20.29%	2.149%
13	7.393	697	698	703	rVB3	11147	11268	0.12%	0.013%
14	7.540	714	723	733	rBV	1108021	1762611	19.13%	2.027%
15	7.622	733	737	741	rVB6	7725	12478	0.14%	0.014%
16	7.899	781	784	790	rVB5	8057	10567	0.11%	0.012%
17	8.010	793	803	818	rBV	1301709	2121649	23.03%	2.439%
18	8.128	818	823	827	rVB5	8919	13518	0.15%	0.016%
19	8.369	860	864	867	rBV6	6023	10358	0.11%	0.012%
20	8.440	872	876	882	rVB7	7773	13769	0.15%	0.016%
21	8.722	916	924	932	rBV	820421	1354848	14.71%	1.558%
22	9.181	994	1002	1011	rVV	1423202	2291940	24.88%	2.635%
23	9.275	1016	1018	1025	rVV7	9227	15060	0.16%	0.017%
24	9.346	1025	1030	1035	rVB6	9919	17223	0.19%	0.020%
25	9.587	1066	1071	1077	rVB3	8139	13822	0.15%	0.016%
26	9.904	1116	1125	1140	rBV	1080902	1780640	19.33%	2.047%
27	10.446	1206	1217	1228	rBV	1514403	2522550	27.38%	2.900%
28	10.693	1253	1259	1262	rBV8	6138	10167	0.11%	0.012%
29	10.828	1272	1282	1290	rBV	1830683	3074254	33.37%	3.535%
30	10.963	1298	1305	1321	rBV	1277934	2223221	24.13%	2.556%
31	11.604	1407	1414	1419	rBV6	11365	22071	0.24%	0.025%
32	12.240	1517	1522	1527	rVB	15812	24678	0.27%	0.028%
33	12.410	1546	1551	1558	rBV	27505	46102	0.50%	0.053%
34	13.469	1725	1731	1737	rVB3	17088	25789	0.28%	0.030%
35	13.545	1737	1744	1752	rBV	30469	48726	0.53%	0.056%
36	13.851	1791	1796	1801	rBV7	10384	17022	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024570.D
 Acq On : 27 Mar 2023 19:19
 Operator : CG/JU
 Sample : 02067-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

37	14.057	1823	1831	1842	rBV	3278230	4468094	48.50%	5.137%
38	14.345	1873	1880	1888	rBV2	3378805	4953690	53.77%	5.696%
39	14.481	1900	1903	1908	rBV7	5649	11691	0.13%	0.013%
40	14.539	1908	1913	1922	rVB	31082	46204	0.50%	0.053%
41	14.651	1924	1932	1943	rBV	2820524	4025021	43.69%	4.628%
42	14.739	1943	1947	1951	rVB6	7183	13451	0.15%	0.015%
43	14.839	1959	1964	1977	rBV	224819	386860	4.20%	0.445%
44	15.063	1995	2002	2011	rVB	13772	35594	0.39%	0.041%
45	15.486	2067	2074	2080	rVB	95316	123303	1.34%	0.142%
46	15.639	2093	2100	2111	rBV	4497996	6580544	71.43%	7.566%
47	15.757	2113	2120	2132	rVV	1667473	2267563	24.61%	2.607%
48	15.886	2136	2142	2147	rVB3	43807	90071	0.98%	0.104%
49	16.004	2156	2162	2166	rBV	55703	80356	0.87%	0.092%
50	16.039	2166	2168	2174	rVB5	13841	23455	0.25%	0.027%
51	16.110	2174	2180	2183	rBV6	17555	23620	0.26%	0.027%
52	16.345	2215	2220	2224	rBV	167511	254511	2.76%	0.293%
53	16.692	2274	2279	2283	rBV5	16422	29952	0.33%	0.034%
54	16.751	2287	2289	2292	rVV2	14199	15411	0.17%	0.018%
55	16.810	2296	2299	2303	rVB5	10892	13494	0.15%	0.016%
56	16.857	2303	2307	2313	rBV6	17958	30045	0.33%	0.035%
57	16.928	2315	2319	2322	rBV6	11062	16430	0.18%	0.019%
58	17.145	2351	2356	2360	rBV	161406	206402	2.24%	0.237%
59	17.192	2360	2364	2369	rVB3	53592	81658	0.89%	0.094%
60	17.398	2392	2399	2406	rBV	3351288	4812377	52.24%	5.533%
61	17.498	2409	2416	2427	rVV2	5347407	7704445	83.63%	8.859%
62	17.686	2443	2448	2455	rBV7	22856	52222	0.57%	0.060%
63	17.880	2477	2481	2487	rBV	139537	184292	2.00%	0.212%
64	18.063	2507	2512	2518	rVB	83614	111218	1.21%	0.128%
65	18.280	2544	2549	2554	rBV	193205	267587	2.90%	0.308%
66	18.575	2595	2599	2605	rBV	123639	144931	1.57%	0.167%
67	19.204	2703	2706	2709	rBV	77496	98215	1.07%	0.113%
68	19.357	2727	2732	2737	rBV3	87551	139422	1.51%	0.160%
69	19.422	2739	2743	2748	rVV2	72132	113340	1.23%	0.130%
70	19.551	2761	2765	2772	rBV	105335	151169	1.64%	0.174%
71	19.786	2799	2805	2817	rBV	6717639	9094663	98.72%	10.457%
72	20.016	2840	2844	2848	rBV	102629	126184	1.37%	0.145%
73	20.321	2893	2896	2899	rBV3	35373	41474	0.45%	0.048%
74	21.280	3055	3059	3065	rBV	195173	273176	2.97%	0.314%
75	21.586	3106	3111	3123	rBV	3701333	5032825	54.63%	5.787%
76	23.933	3502	3510	3523	rBV2	4515876	9212806	100.00%	10.593%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024570.D
Acq On : 27 Mar 2023 19:19
Operator : CG/JU
Sample : 02067-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ88

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Title : SVOA CALIBRATION

77 24.086 3529 3536 3549 rVB2 2351496 5142931 55.82% 5.913%




Sum of corrected areas: 86971013

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024570.D
Acq On : 27 Mar 2023 19:19
Operator : CG/JU
Sample : 02067-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

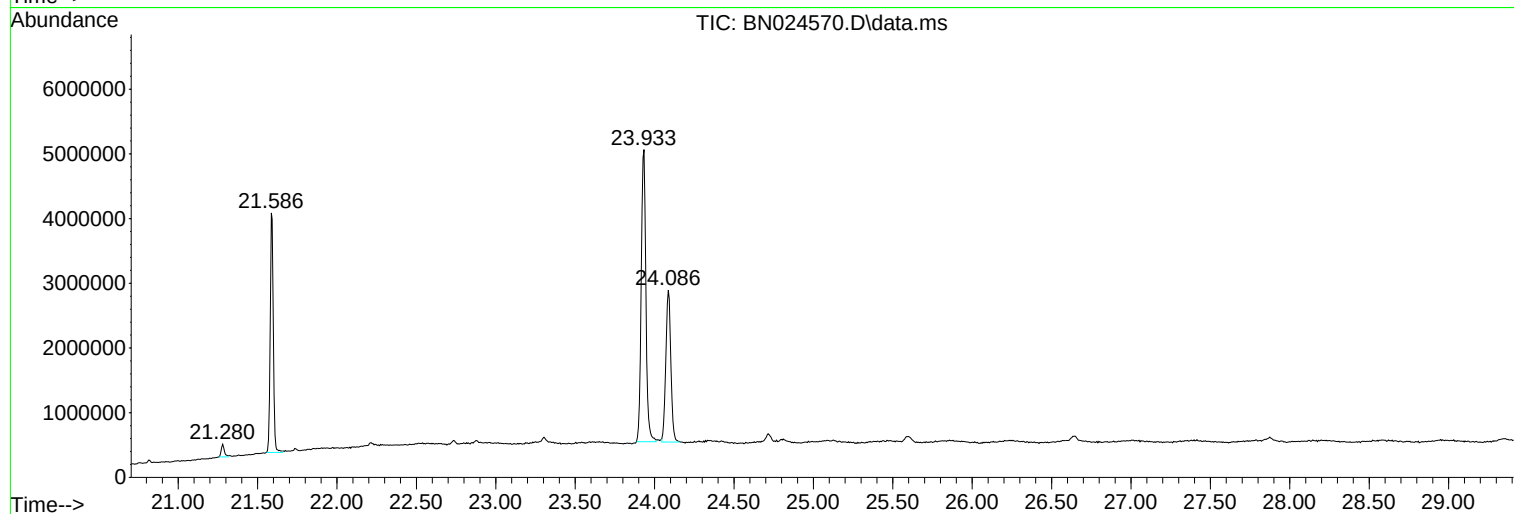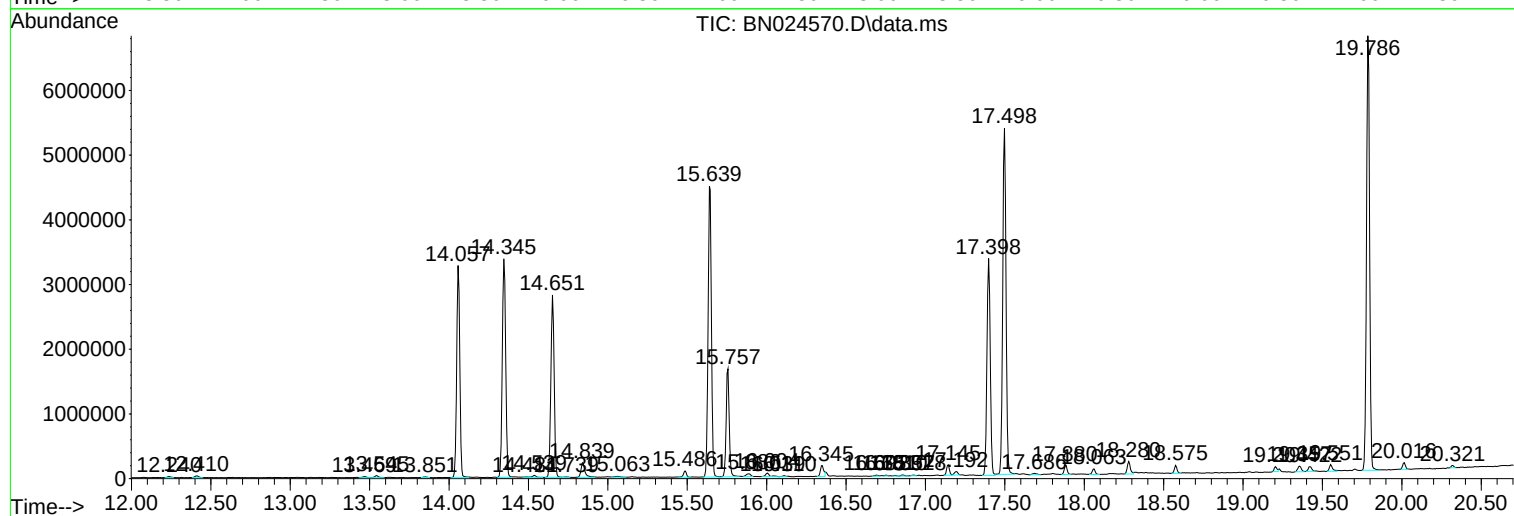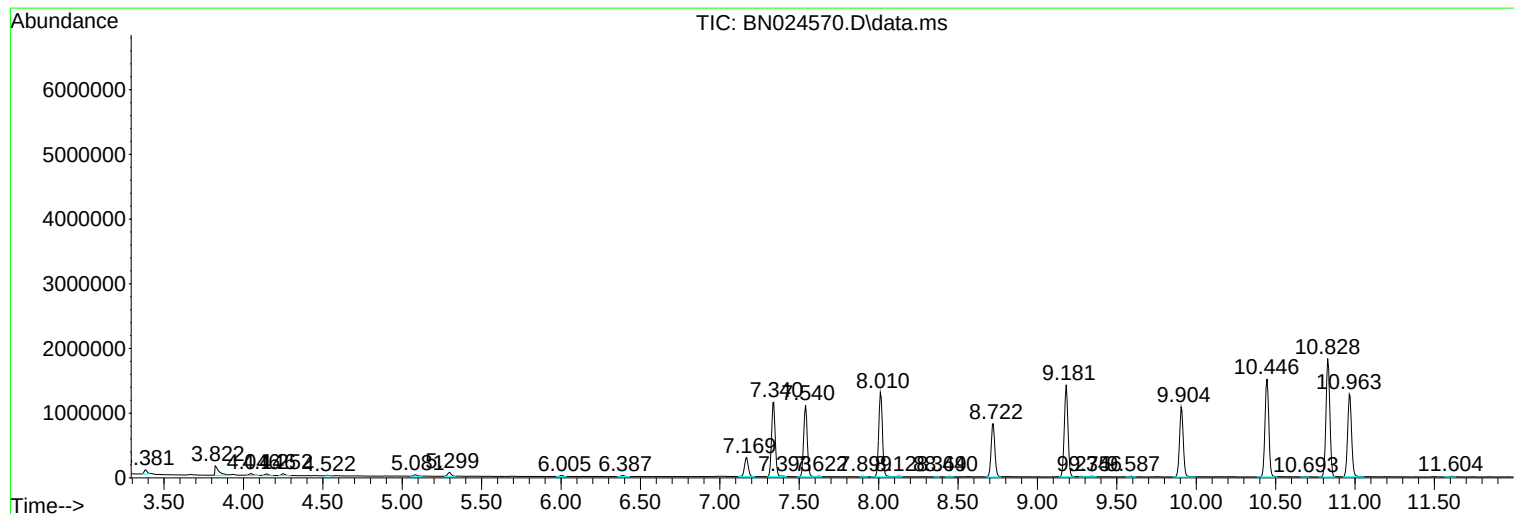

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024570.D
Acq On : 27 Mar 2023 19:19
Operator : CG/JU
Sample : 02067-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024570.D
Acq On : 27 Mar 2023 19:19
Operator : CG/JU
Sample : 02067-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc