

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024572.D
 Acq On : 27 Mar 2023 20:34
 Operator : CG/JU
 Sample : 02067-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	21	rBV	70631	99690	1.23%	0.128%
2	3.823	89	91	106	rBV	152269	265088	3.28%	0.341%
3	4.046	124	129	136	rVB	30763	51917	0.64%	0.067%
4	4.146	141	146	154	rVB	22781	36196	0.45%	0.047%
5	4.252	159	164	171	rVB	27964	47477	0.59%	0.061%
6	4.522	207	210	217	rVB7	7391	14709	0.18%	0.019%
7	5.081	299	305	313	rBV	29181	50471	0.62%	0.065%
8	5.175	315	321	325	rVB8	7707	15287	0.19%	0.020%
9	5.299	336	342	348	rVB3	35606	61142	0.76%	0.079%
10	5.999	457	461	467	rBV4	6627	10552	0.13%	0.014%
11	6.387	522	527	532	rBV	19492	28063	0.35%	0.036%
12	6.981	623	628	631	rBV6	7676	11514	0.14%	0.015%
13	7.169	650	660	671	rVB	295175	485479	6.00%	0.625%
14	7.334	681	688	697	rBV	1172283	1856581	22.94%	2.391%
15	7.540	716	723	732	rBV	1125856	1793329	22.16%	2.310%
16	7.628	734	738	743	rVB3	8361	13298	0.16%	0.017%
17	7.905	778	785	789	rBV5	8207	15186	0.19%	0.020%
18	8.011	796	803	813	rBV	1173831	1891498	23.37%	2.436%
19	8.122	819	822	827	rVB5	6480	10670	0.13%	0.014%
20	8.369	860	864	870	rBV7	5075	9946	0.12%	0.013%
21	8.434	870	875	881	rVB9	7993	17251	0.21%	0.022%
22	8.722	917	924	936	rBV	821163	1353322	16.72%	1.743%
23	9.181	995	1002	1012	rBV	1398846	2254142	27.86%	2.903%
24	9.281	1016	1019	1023	rVB5	7459	9847	0.12%	0.013%
25	9.593	1065	1072	1076	rBV7	6578	12321	0.15%	0.016%
26	9.905	1117	1125	1140	rBV	1071860	1762615	21.78%	2.270%
27	10.128	1158	1163	1167	rBV7	4678	8422	0.10%	0.011%
28	10.193	1167	1174	1178	rVV6	5119	9981	0.12%	0.013%
29	10.446	1209	1217	1230	rBV	1500043	2463513	30.44%	3.173%
30	10.693	1252	1259	1265	rBV3	22616	40215	0.50%	0.052%
31	10.828	1273	1282	1290	rBV	1657158	2774870	34.29%	3.574%
32	10.963	1297	1305	1320	rBV	1220883	2150211	26.57%	2.770%
33	11.210	1341	1347	1353	rVB3	10784	16641	0.21%	0.021%
34	11.610	1409	1415	1425	rBV6	17505	33586	0.42%	0.043%
35	11.951	1469	1473	1478	rVB4	8615	13587	0.17%	0.018%
36	12.081	1488	1495	1499	rBV8	5588	9570	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
 Data File : BN024572.D
 Acq On : 27 Mar 2023 20:34
 Operator : CG/JU
 Sample : 02067-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
 Title : SVOA CALIBRATION

37	12.410	1546	1551	1556	rBV	31038	45629	0.56%	0.059%
38	13.546	1738	1744	1748	rBV3	14480	24340	0.30%	0.031%
39	14.057	1824	1831	1842	rBV	3044120	4114003	50.84%	5.299%
40	14.345	1873	1880	1890	rBV	3372446	4779956	59.07%	6.157%
41	14.651	1925	1932	1941	rBV	2534598	3627806	44.83%	4.673%
42	14.840	1958	1964	1979	rBV	205442	363197	4.49%	0.468%
43	15.057	1996	2001	2012	rVB	13899	33696	0.42%	0.043%
44	15.640	2091	2100	2109	rBV	4270922	6139354	75.87%	7.908%
45	15.757	2113	2120	2133	rVV	1461163	2033329	25.13%	2.619%
46	15.881	2136	2141	2148	rVB	22824	38939	0.48%	0.050%
47	16.004	2157	2162	2167	rVB	55676	78120	0.97%	0.101%
48	16.339	2213	2219	2224	rVB9	5441	10402	0.13%	0.013%
49	16.428	2230	2234	2237	rBV6	5617	9734	0.12%	0.013%
50	17.045	2335	2339	2342	rBV6	7684	10880	0.13%	0.014%
51	17.139	2351	2355	2359	rBV6	6721	9775	0.12%	0.013%
52	17.181	2359	2362	2367	rBV3	8070	14168	0.18%	0.018%
53	17.269	2374	2377	2380	rBV5	6745	8155	0.10%	0.011%
54	17.398	2392	2399	2406	rBV	3104607	4315294	53.33%	5.558%
55	17.498	2409	2416	2435	rVV	4907809	6961017	86.02%	8.966%
56	17.769	2460	2462	2468	rVB6	8296	10960	0.14%	0.014%
57	18.281	2544	2549	2559	rBV	120854	185161	2.29%	0.238%
58	18.357	2559	2562	2568	rVB2	11588	18160	0.22%	0.023%
59	18.704	2619	2621	2626	rVB5	10104	9559	0.12%	0.012%
60	19.351	2727	2731	2737	rBV2	57398	78949	0.98%	0.102%
61	19.422	2738	2743	2748	rBV	62220	102797	1.27%	0.132%
62	19.551	2762	2765	2770	rBV3	68372	83267	1.03%	0.107%
63	19.786	2799	2805	2813	rBV	6067391	8092290	100.00%	10.423%
64	21.275	3055	3058	3063	rBV3	103128	143637	1.77%	0.185%
65	21.586	3106	3111	3118	rBV	3275936	4379639	54.12%	5.641%
66	23.910	3498	3506	3520	rBV2	3654217	7825197	96.70%	10.079%
67	24.068	3526	3533	3544	rVB2	2120576	4391845	54.27%	5.657%




Sum of corrected areas: 77637442

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024572.D
Acq On : 27 Mar 2023 20:34
Operator : CG/JU
Sample : 02067-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

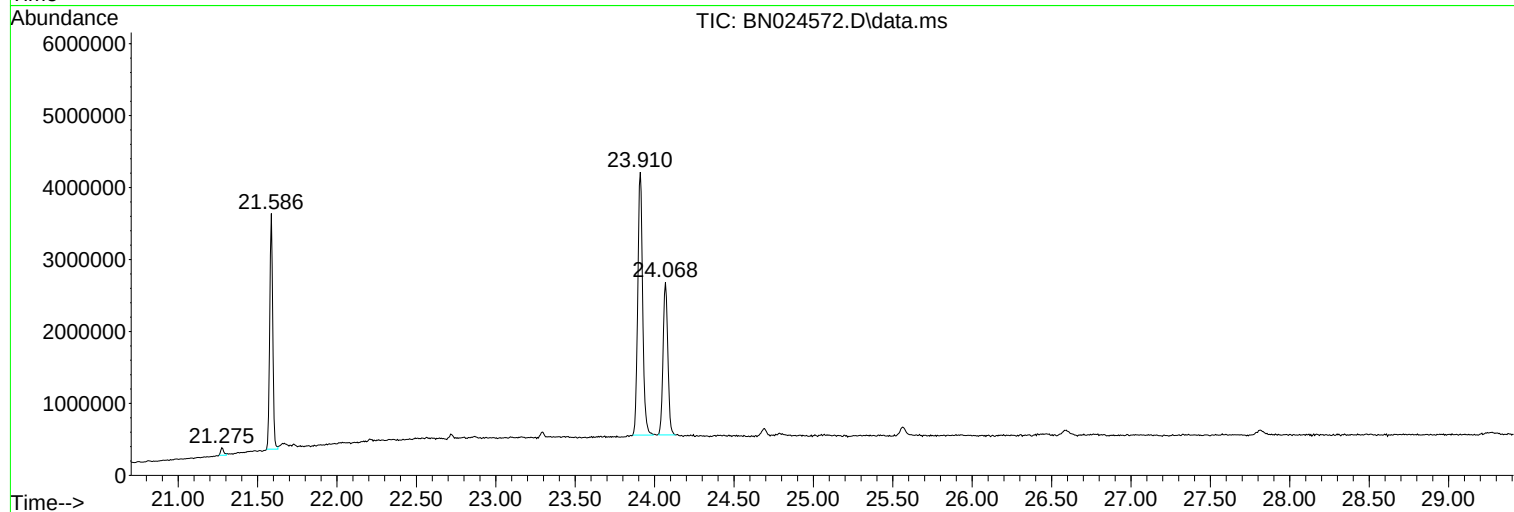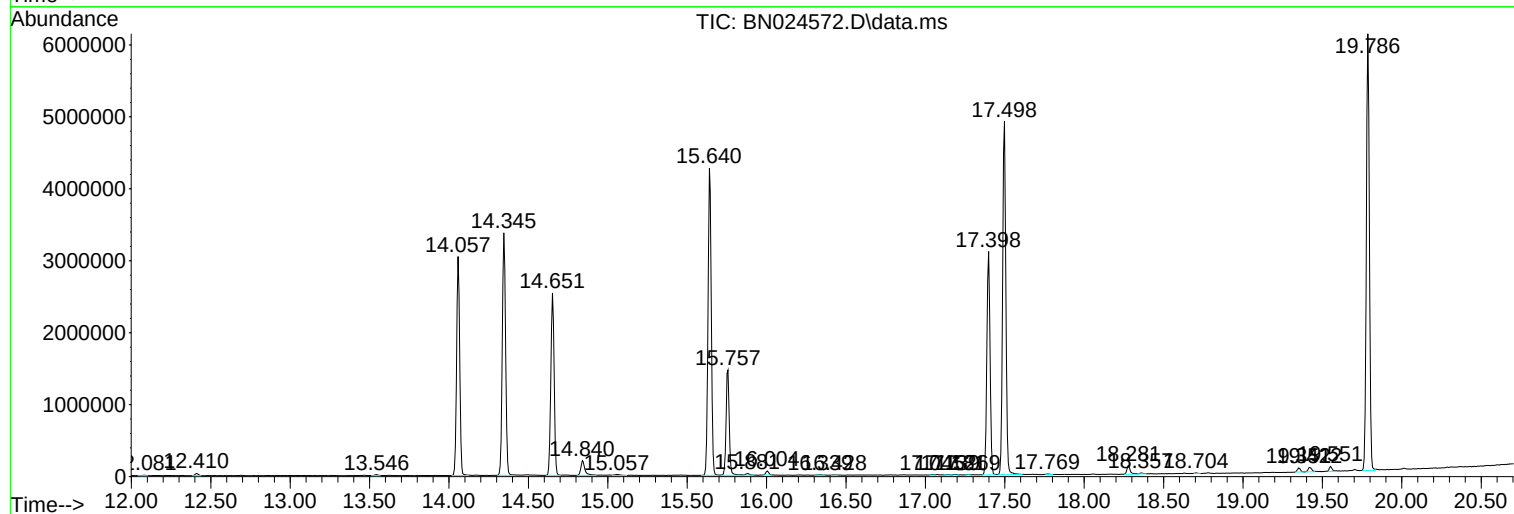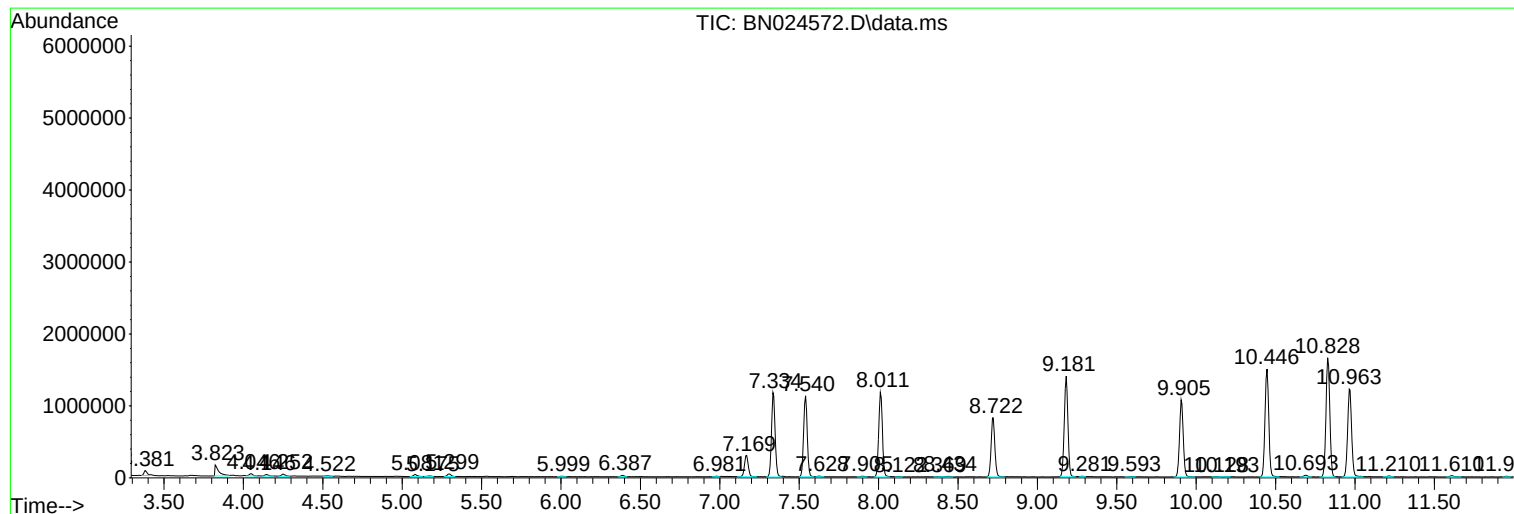

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024572.D
Acq On : 27 Mar 2023 20:34
Operator : CG/JU
Sample : 02067-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032823\
Data File : BN024572.D
Acq On : 27 Mar 2023 20:34
Operator : CG/JU
Sample : 02067-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN030323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc