
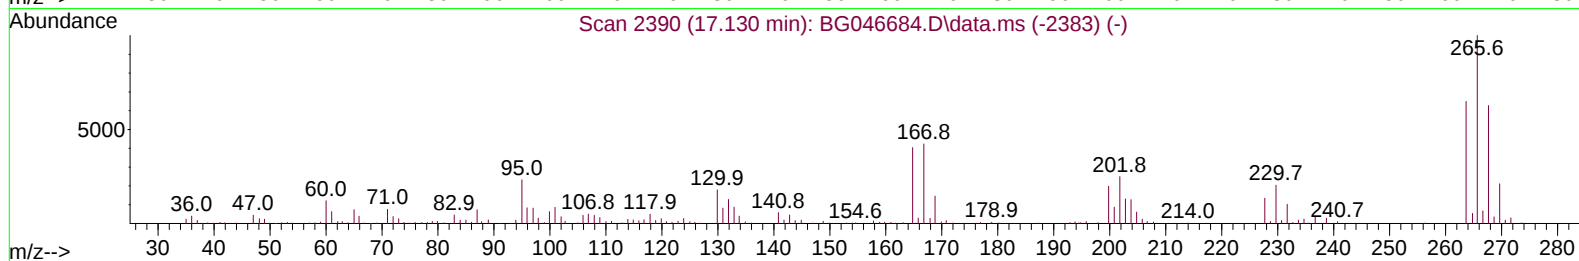
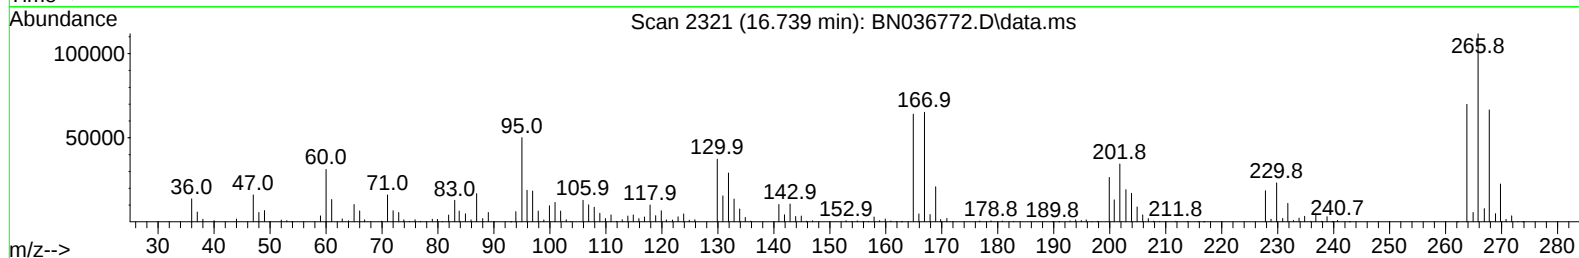


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036772.D
Acq On : 28 Mar 2025 14:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 04:37:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

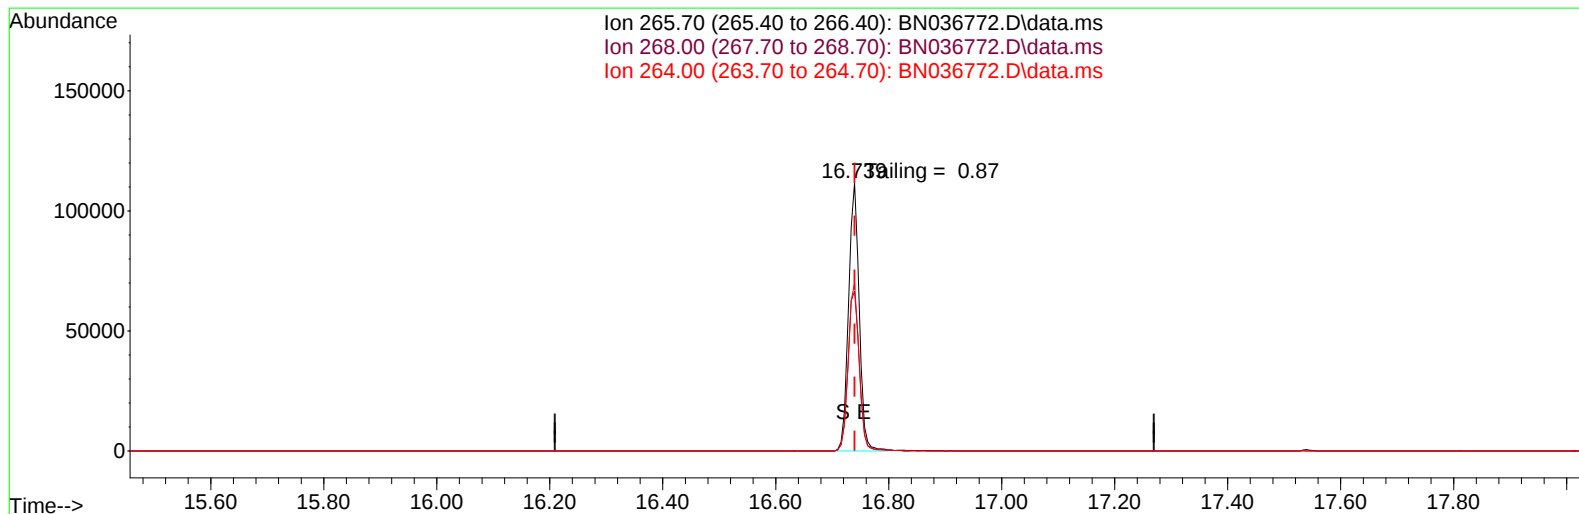

TIC: BN036772.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.000) 17915.55 ng

response 146783

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.53
264.00	61.60	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036772.D
Acq On : 28 Mar 2025 14:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 04:37:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

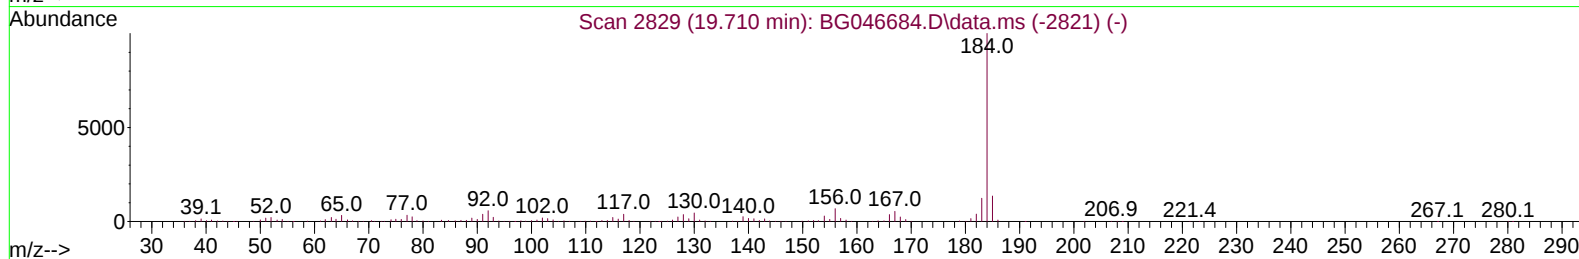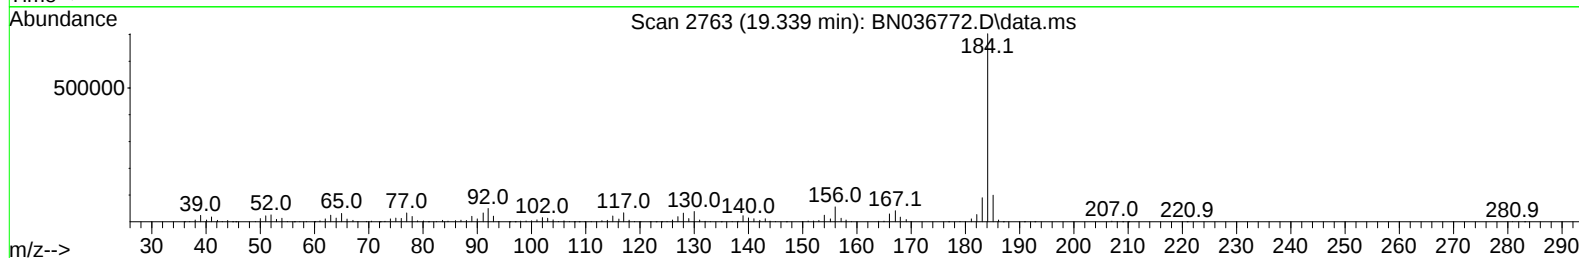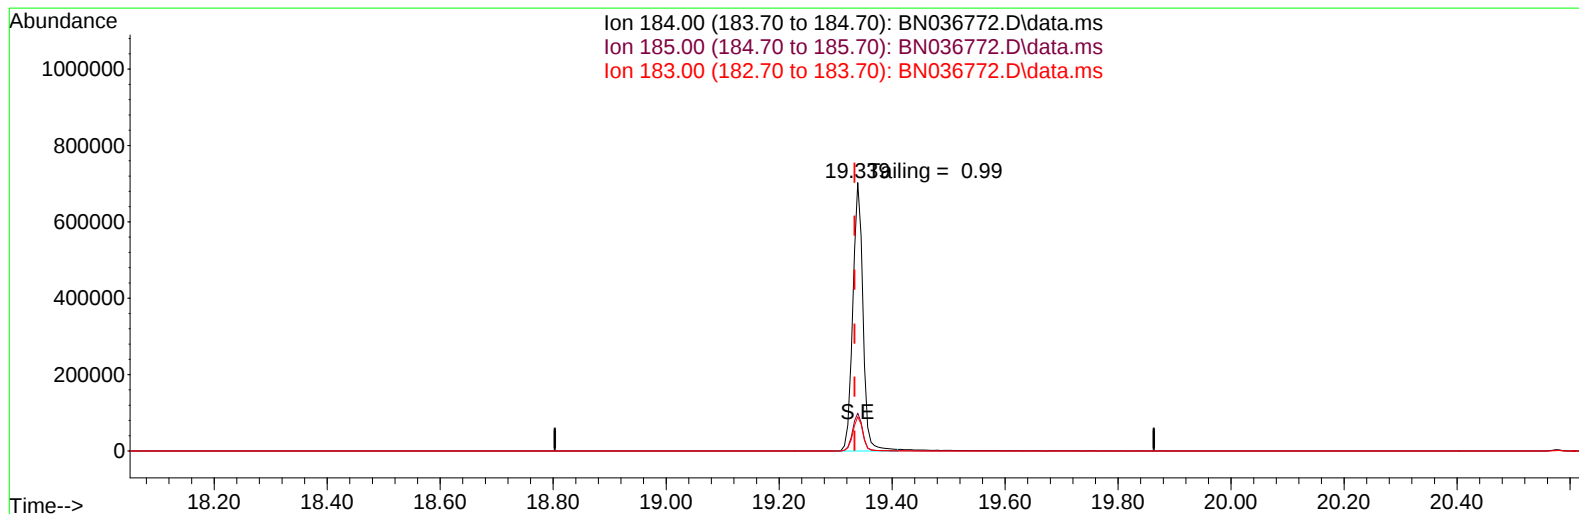

TIC: BN036772.D\data.ms

(77) Benzidine**19.339min (+ 0.006) 0.00 ng****response 891011**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	12.76
0.00	0.00	0.00