
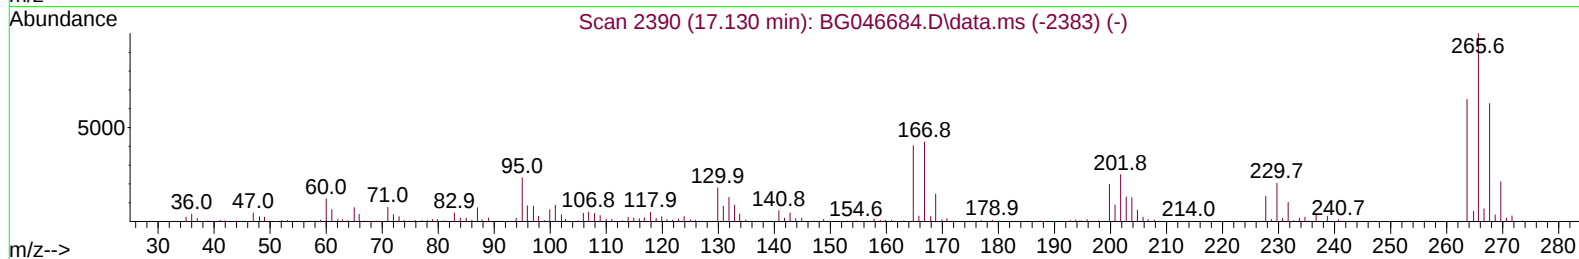
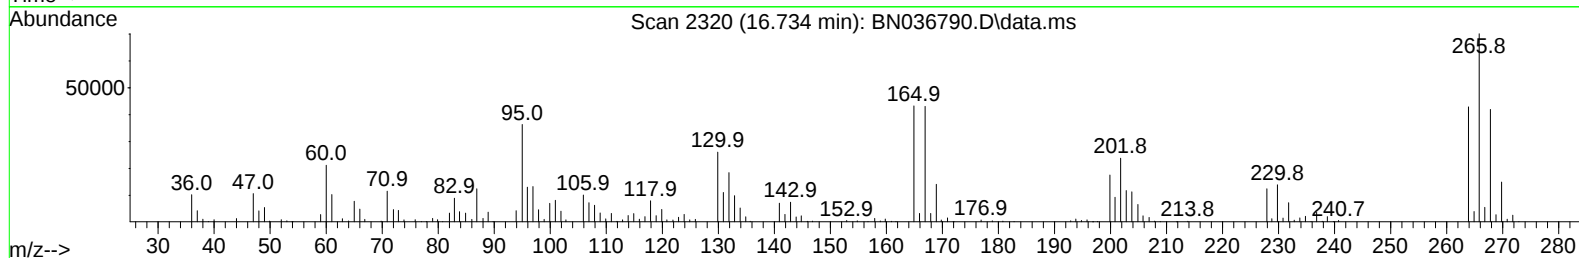


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036790.D
Acq On : 29 Mar 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Apr 01 00:17:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

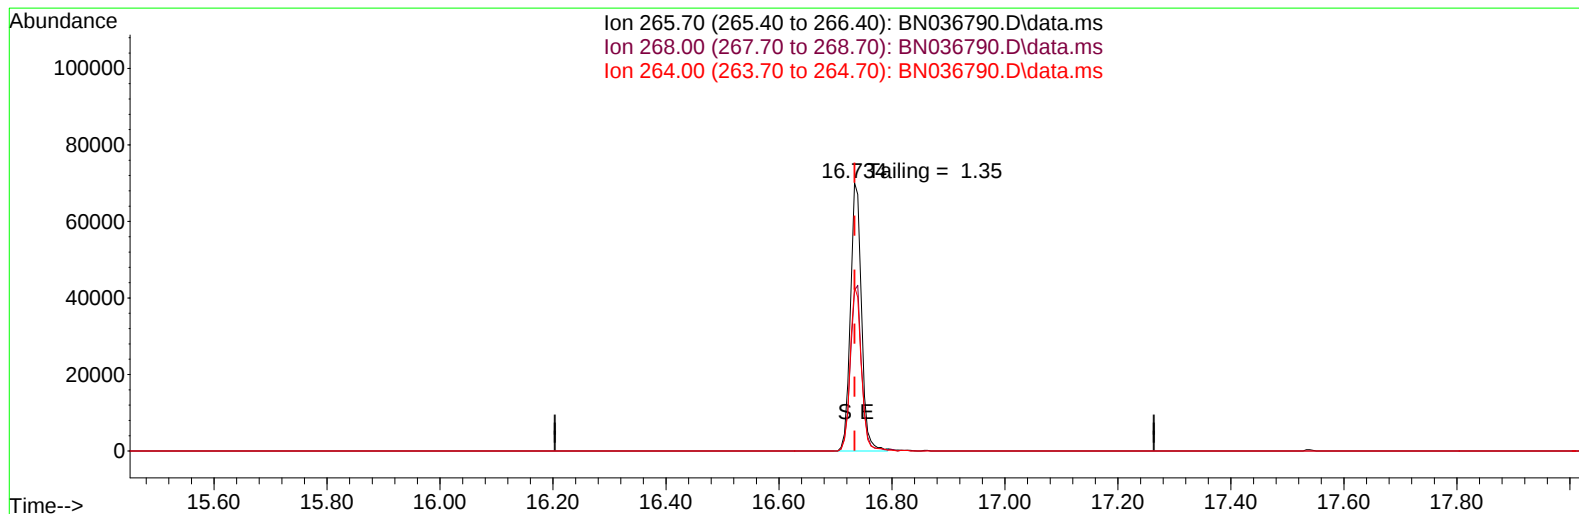

TIC: BN036790.D\data.ms

(70) Pentachlorophenol (C)




16.734min (0.000) 16501.63 ng

response 96219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.83
264.00	61.60	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036790.D
Acq On : 29 Mar 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Apr 01 00:17:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

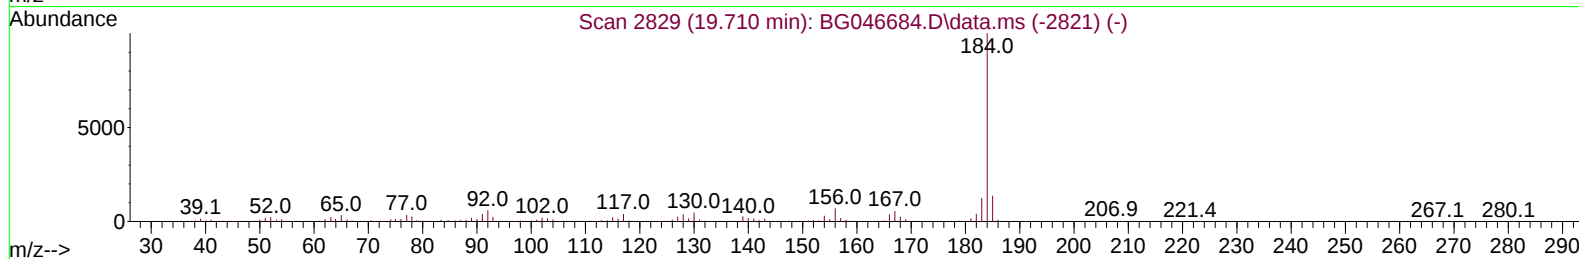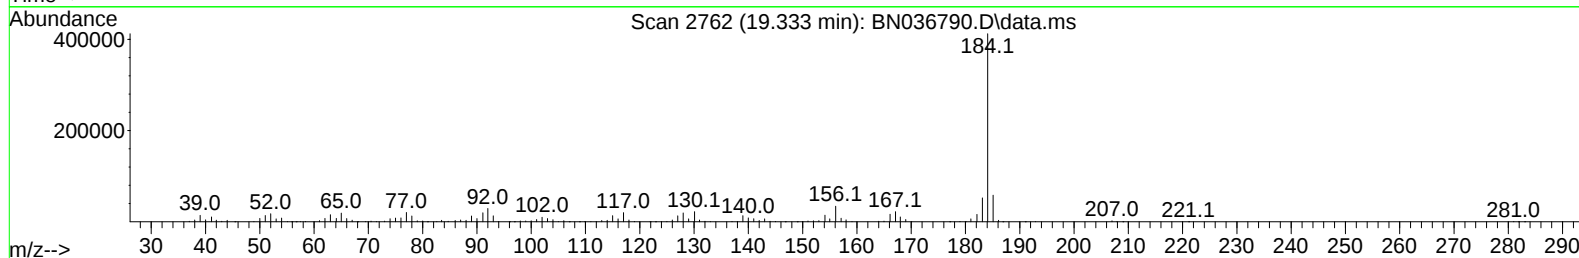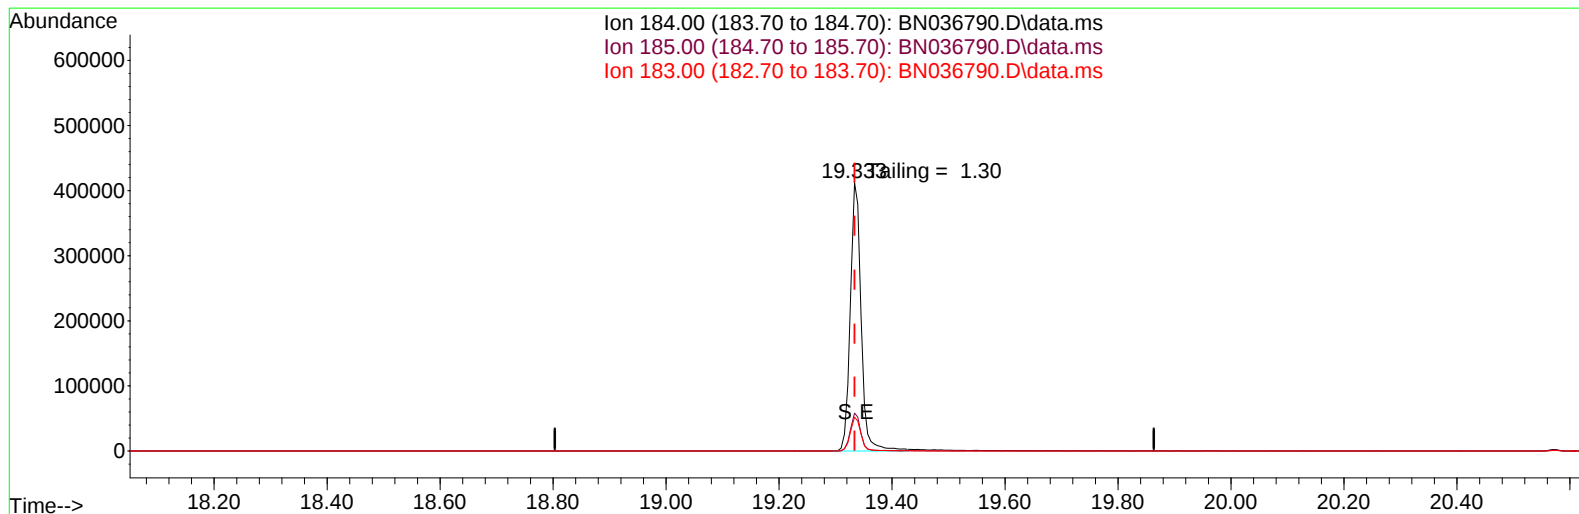

TIC: BN036790.D\data.ms

(77) Benzidine

19.333min (0.000) 0.00 ng

response 556362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	12.68
0.00	0.00	0.00