
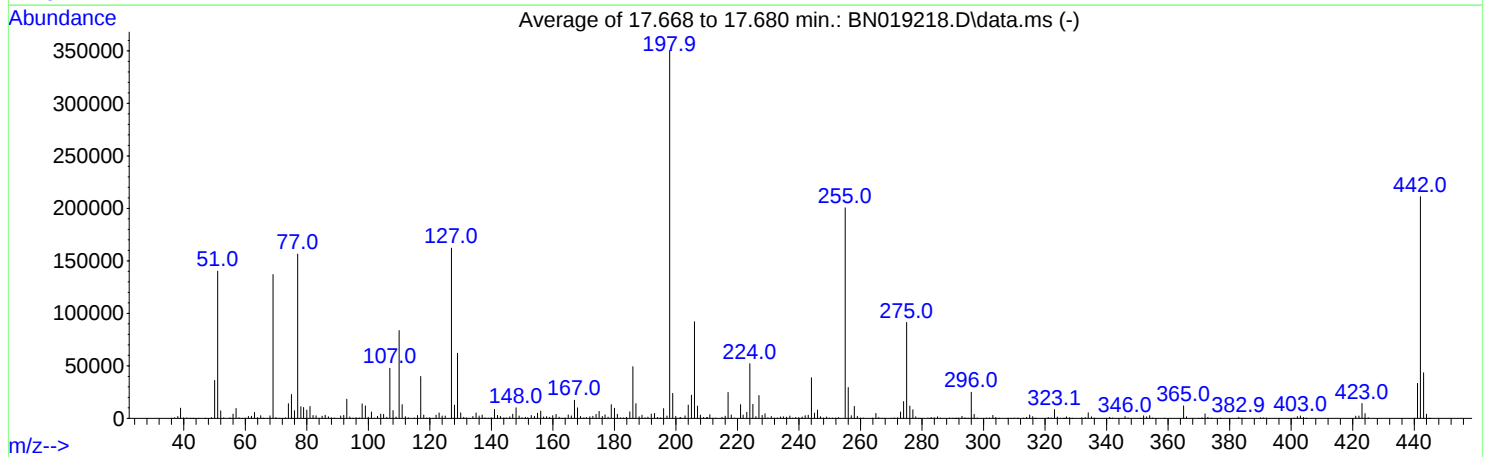


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032922\
 Data File : BN019218.D
 Acq On : 29 Mar 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 19:03:12 2022

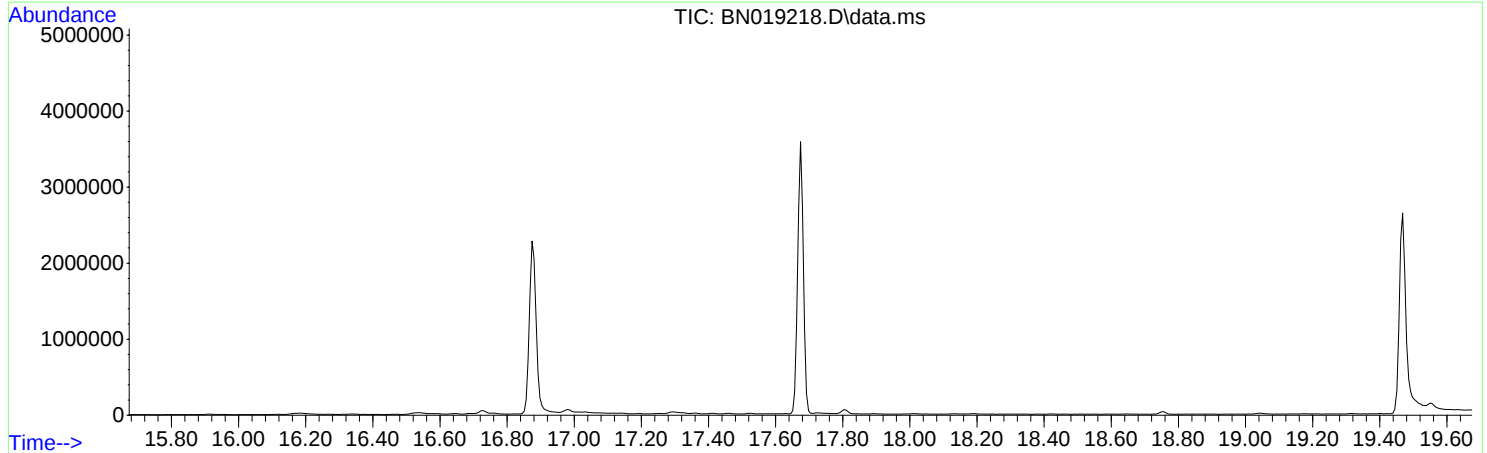




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	140169	PASS
68	69	0.00	2	1.8	2514	PASS
69	198	0.00	100	39.1	136956	PASS
70	69	0.00	2	0.5	732	PASS
127	198	10	80	46.3	162219	PASS
197	198	0.00	2	0.7	2341	PASS
198	198	100	100	100.0	350357	PASS
199	198	5	9	6.8	23811	PASS
275	198	10	60	26.1	91424	PASS
365	198	1	100	3.4	11872	PASS
441	198	0.01	100	9.5	33395	PASS
442	442	50	100	100.0	211157	PASS
443	442	15	24	20.6	43445	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032922\
 Data File : BN019218.D
 Acq On : 29 Mar 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 17:36:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

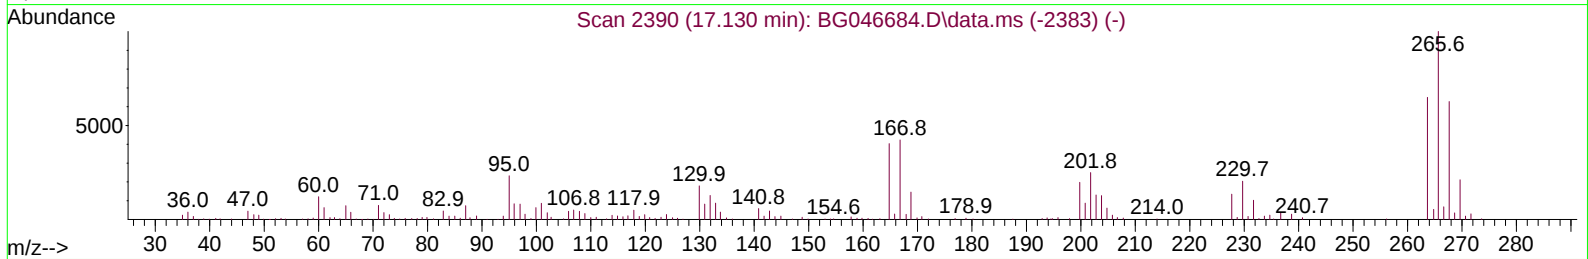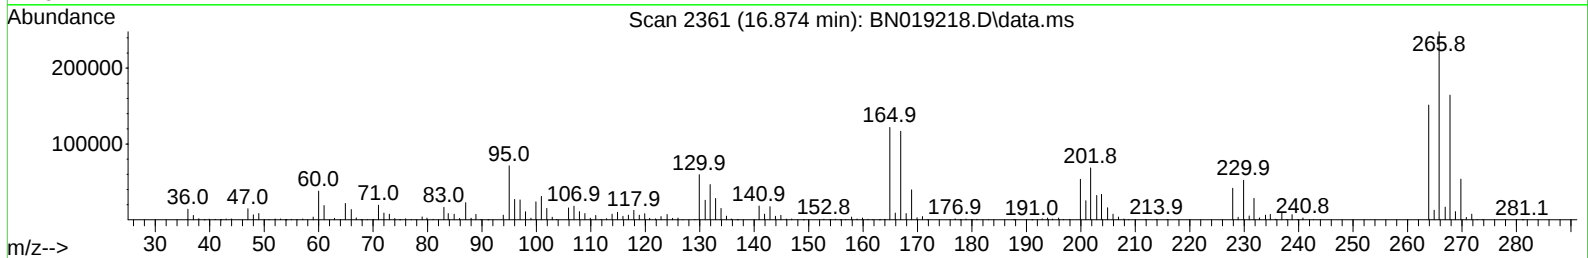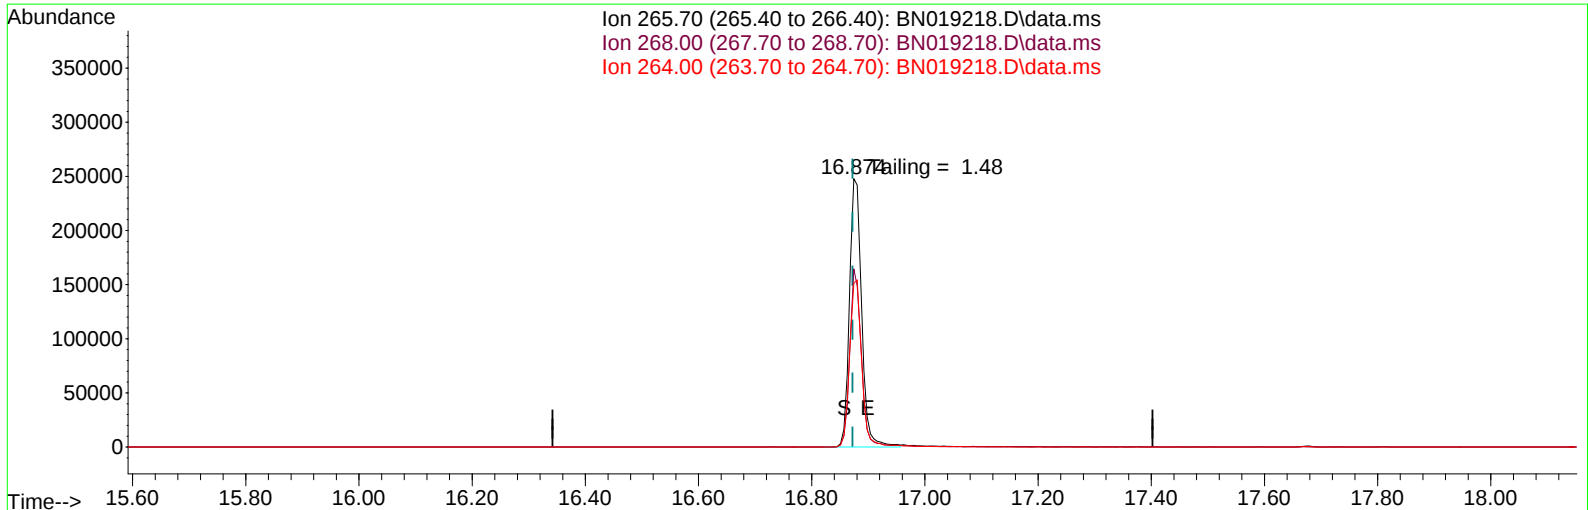

TIC: BN019218.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.002) 21388.20 ng




response 375143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.34
264.00	61.60	61.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032922\
Data File : BN019218.D
Acq On : 29 Mar 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 17:36:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

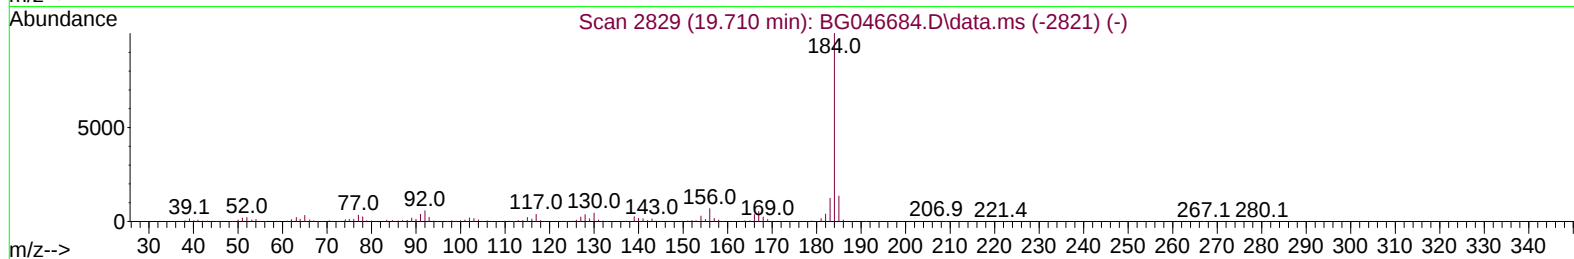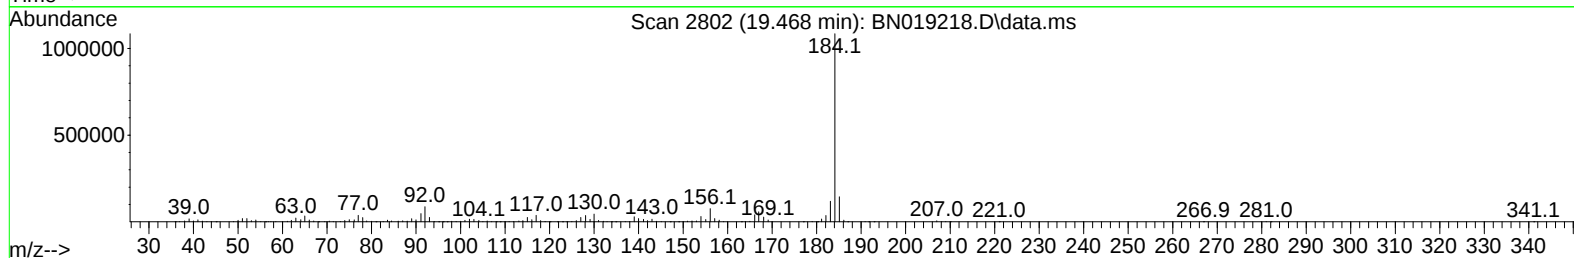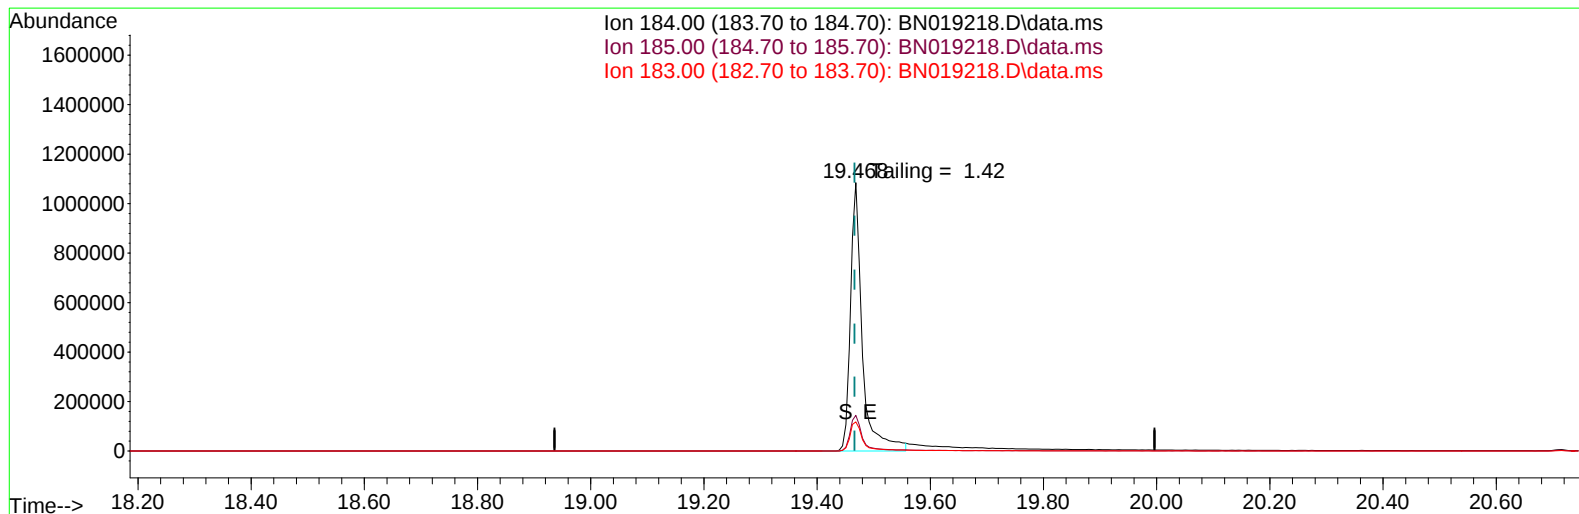

TIC: BN019218.D\data.ms

(77) Benzidine

19.468min (+ 0.002) 0.00 ng

response 1699055

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.28
183.00	13.20	10.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/29/2022	BNA_N	<u>BN019218.D</u>
Compound Name	Response	Retention Time
DDT	1193969	20.71
DDD	17255	20.26
DDE	1367	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18622	1212591	1.54

Instrument :
BNA_N
ClientSampleId :
DFTPP