
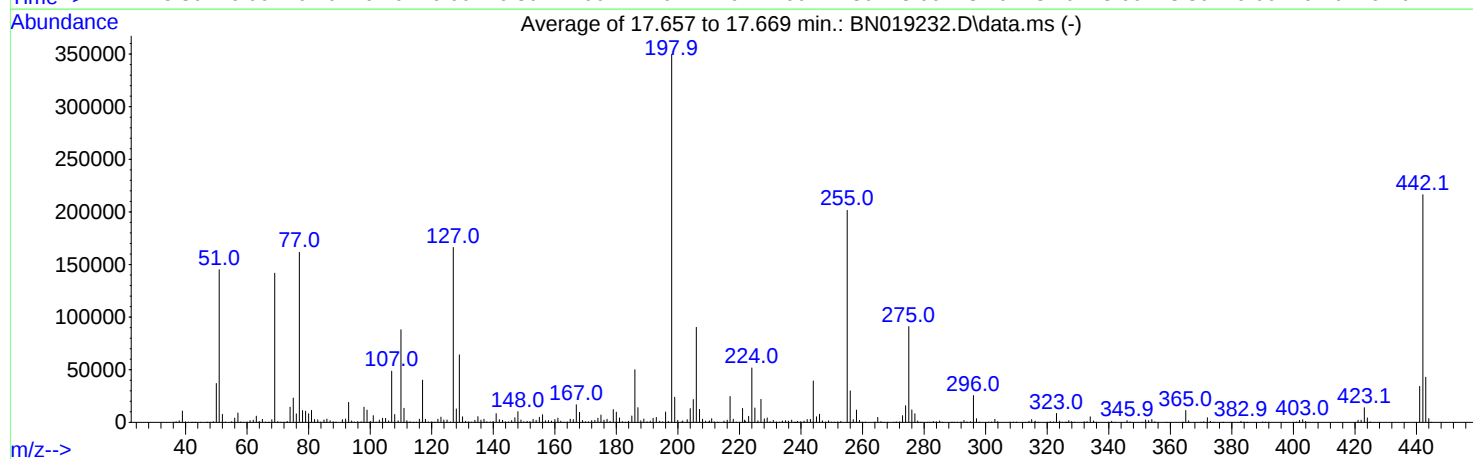


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033022\
 Data File : BN019232.D
 Acq On : 30 Mar 2022 07:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN033022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:57:13 2022

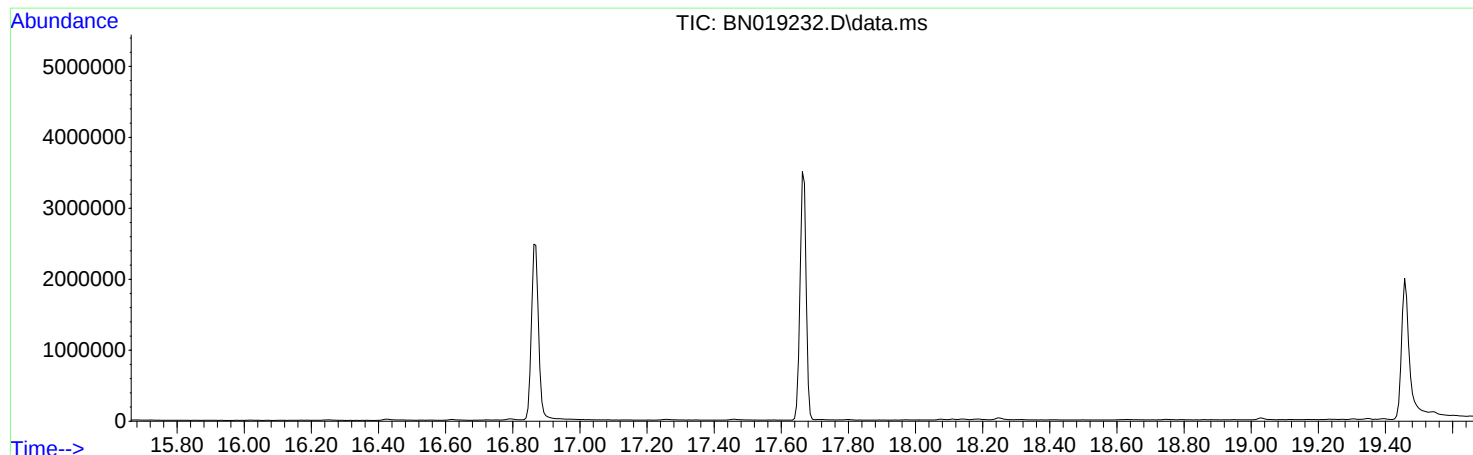




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	145045	PASS
68	69	0.00	2	1.8	2570	PASS
69	198	0.00	100	40.5	141748	PASS
70	69	0.00	2	0.6	807	PASS
127	198	10	80	47.6	166251	PASS
197	198	0.00	2	0.2	866	PASS
198	198	100	100	100.0	349589	PASS
199	198	5	9	6.8	23824	PASS
275	198	10	60	26.1	91093	PASS
365	198	1	100	3.2	11326	PASS
441	198	0.01	100	9.8	34267	PASS
442	442	50	100	100.0	216333	PASS
443	442	15	24	19.8	42827	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033022\
Data File : BN019232.D
Acq On : 30 Mar 2022 07:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 30 11:58:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

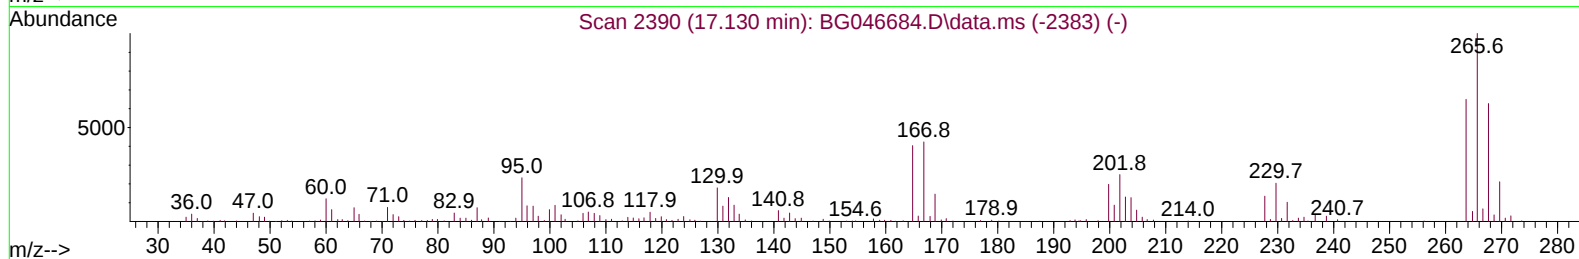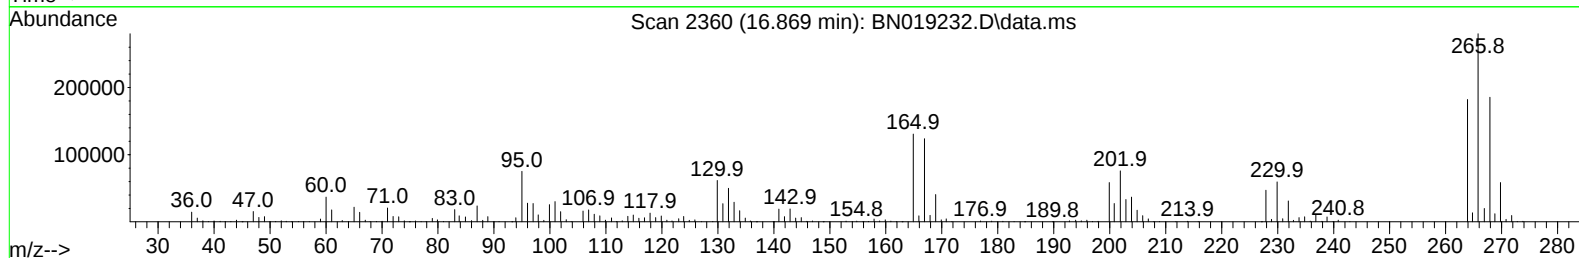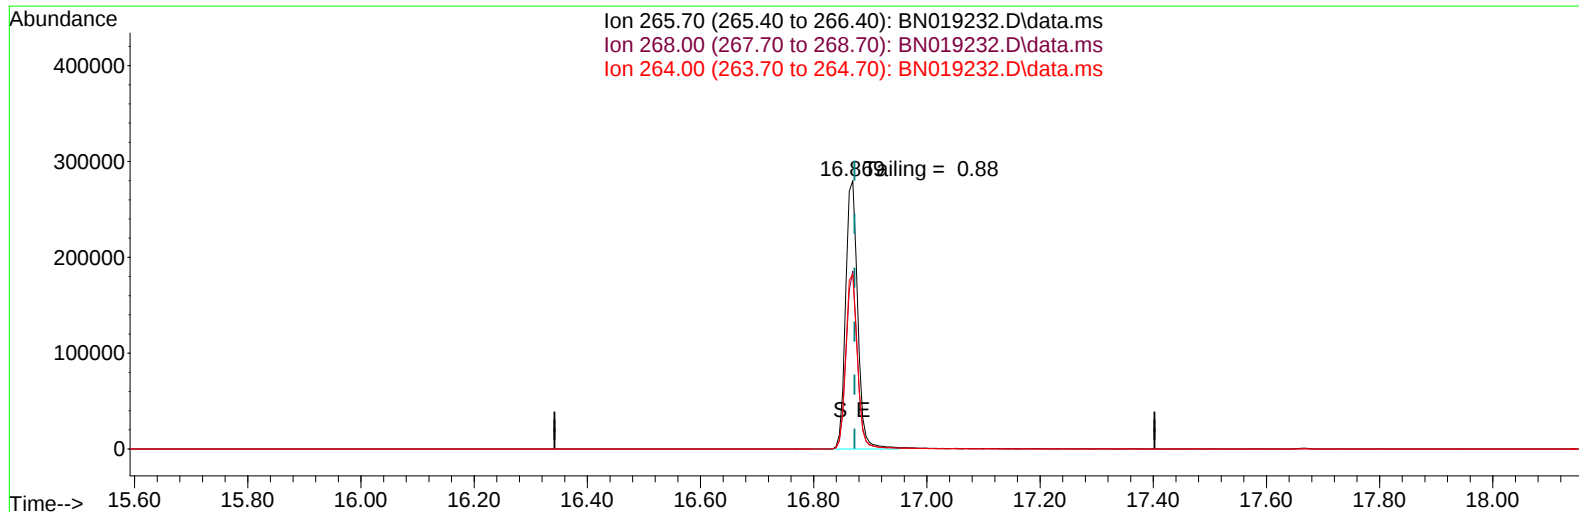

TIC: BN019232.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.003) 22649.15 ng




response 419300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.26
264.00	61.60	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033022\
Data File : BN019232.D
Acq On : 30 Mar 2022 07:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 30 11:58:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

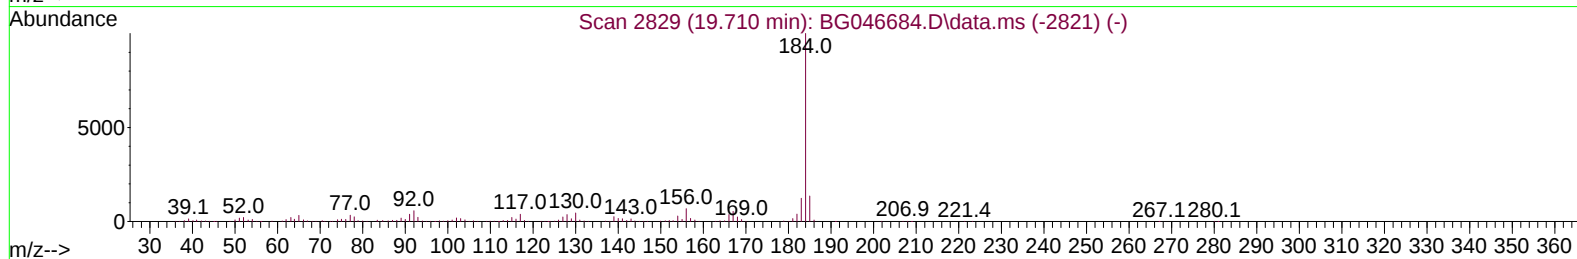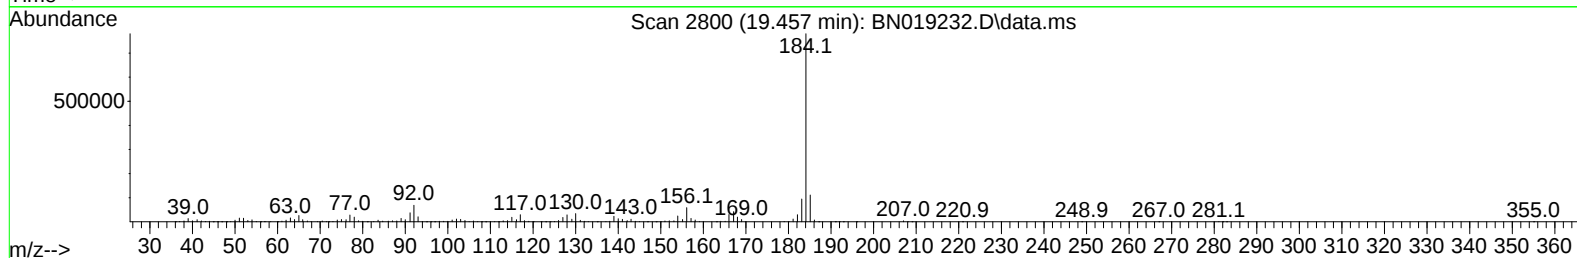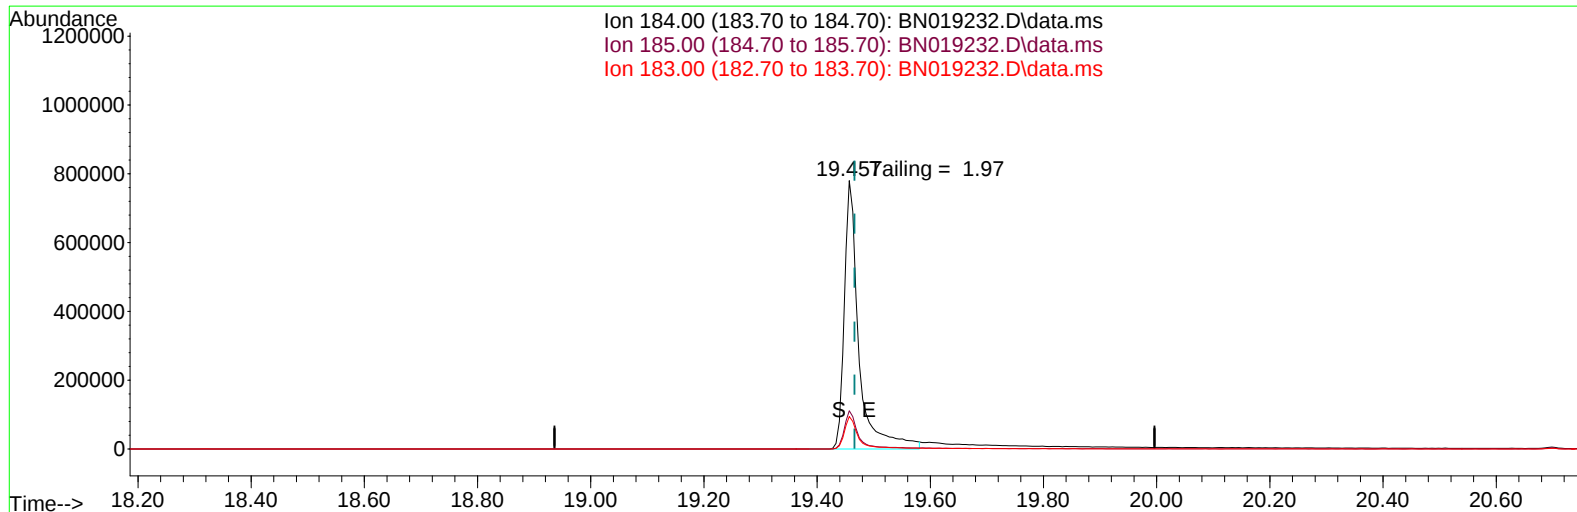

TIC: BN019232.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1491042

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2022	BNA_N	<u>BN019232.D</u>
Compound Name	Response	Retention Time
DDT	1187888	20.69
DDD	25211	20.25
DDE	1152	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26363	1214251	2.17

Instrument :
BNA_N
ClientSampleId :
DFTPP