

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024647.D
 Acq On : 30 Mar 2023 17:47
 Operator : CG/JU
 Sample : PB151685BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK685

Quant Time: Mar 30 19:14:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 30 17:06:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	8778	0.400	ng/ul	0.00
4) Naphthalene-d8	10.817	136	26604	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	15306	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	31657	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	22646	0.400	ng/ul	0.00
23) Perylene-d12	24.065	264	21350	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	69204	7.681	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	14210	0.433	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	27523	0.497	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.775	202	4704	0.058	ng/ul#	1
26) Benzo(a)pyrene	23.895	252	9127	0.131	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024647.D
Acq On : 30 Mar 2023 17:47
Operator : CG/JU
Sample : PB151685BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK685

Quant Time: Mar 30 19:14:36 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 17:06:44 2023
Response via : Initial Calibration

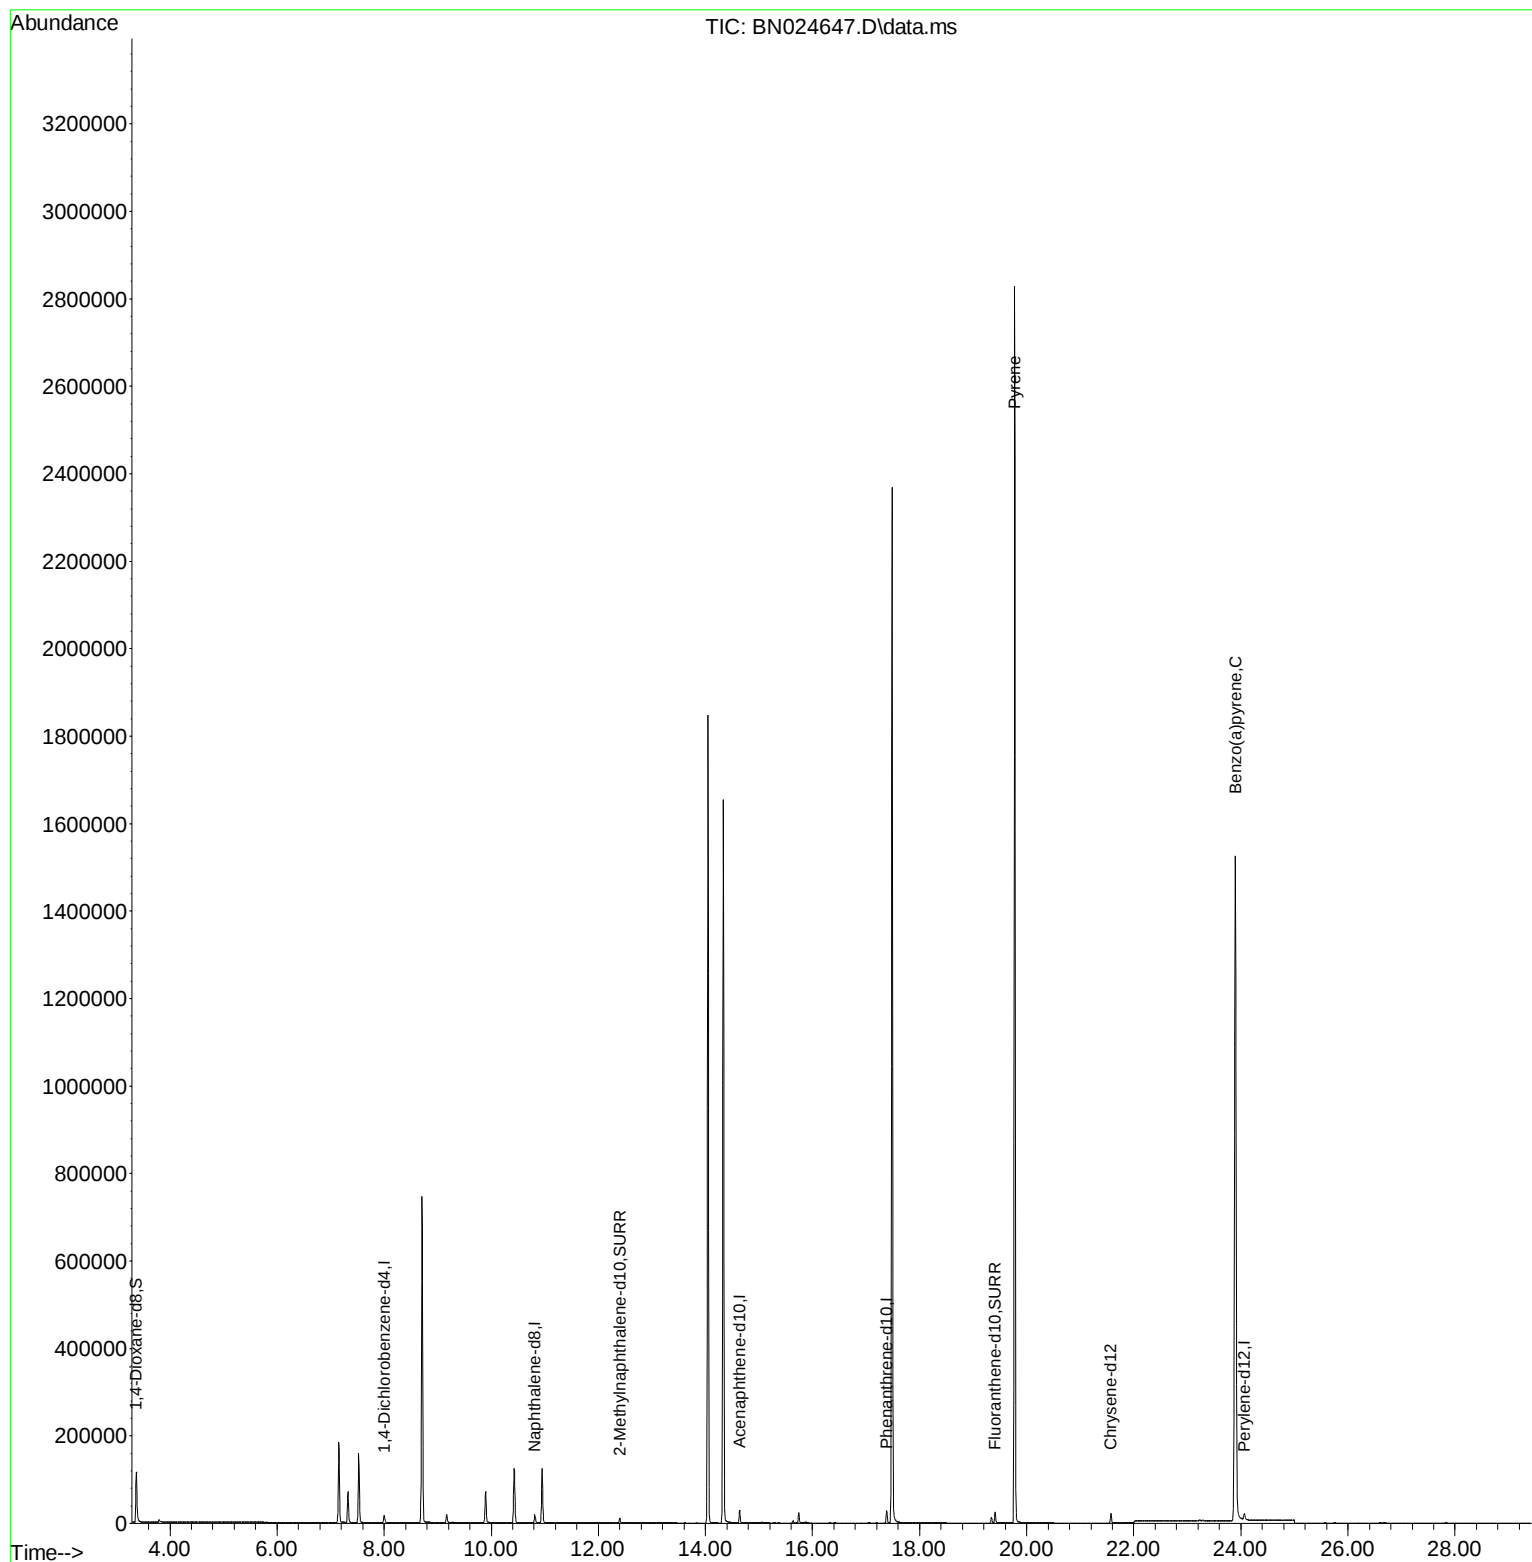

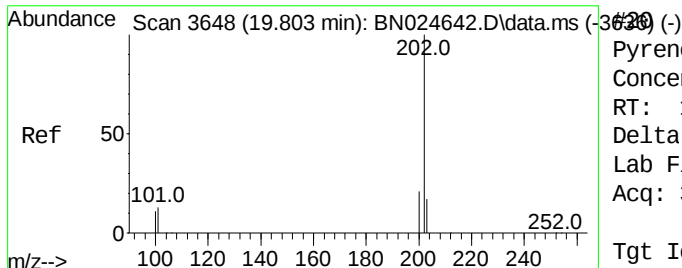

Pyrene

Concen: 0.058 ng/ul

RT: 19.775 min Scan#

Delta R.T. -0.028 min

Lab File: BN024647.D

Acq: 30 Mar 2023 17:47

Instrument :

BNA_N

ClientSampleId :

SBLK685





Tgt Ion:202 Resp: 4704

Ion Ratio Lower Upper

202 100

101 169.2 10.9 16.3#

100 1269.2 8.7 13.1#

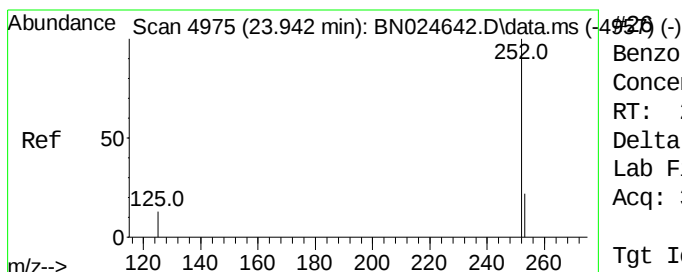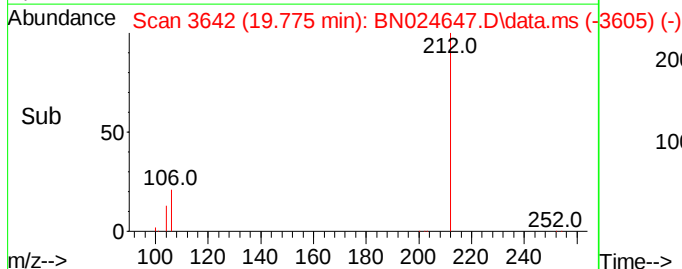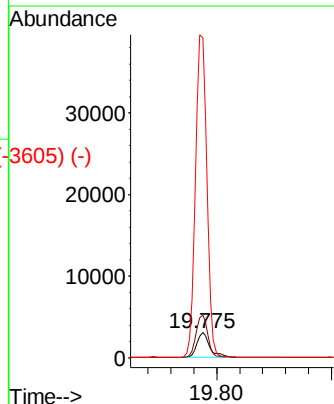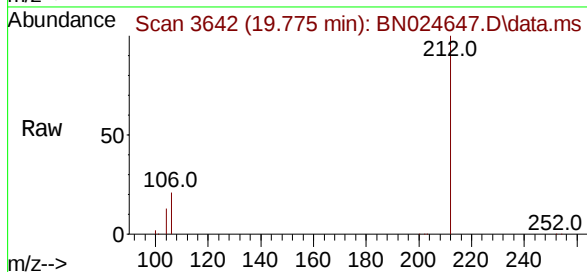

Benzo(a)pyrene

Concen: 0.131 ng/ul

RT: 23.895 min Scan# 4959

Delta R.T. -0.047 min

Lab File: BN024647.D

Acq: 30 Mar 2023 17:47

Tgt Ion:252 Resp: 9127

Ion Ratio Lower Upper

252 100

253 45.6 21.8 32.8#

125 41.7 15.4 23.0#

