

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024649.D
 Acq On : 30 Mar 2023 18:59
 Operator : CG/JU
 Sample : PB151688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK688

Quant Time: Mar 31 02:12:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	9895	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	30121	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	17154	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	35598	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	25305	0.400	ng/ul	0.00
23) Perylene-d12	24.056	264	22709	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	61666	6.072	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	12704	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	25547	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.776	202	4888	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.904	252	9151	0.123	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024649.D
Acq On : 30 Mar 2023 18:59
Operator : CG/JU
Sample : PB151688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK688

Quant Time: Mar 31 02:12:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration




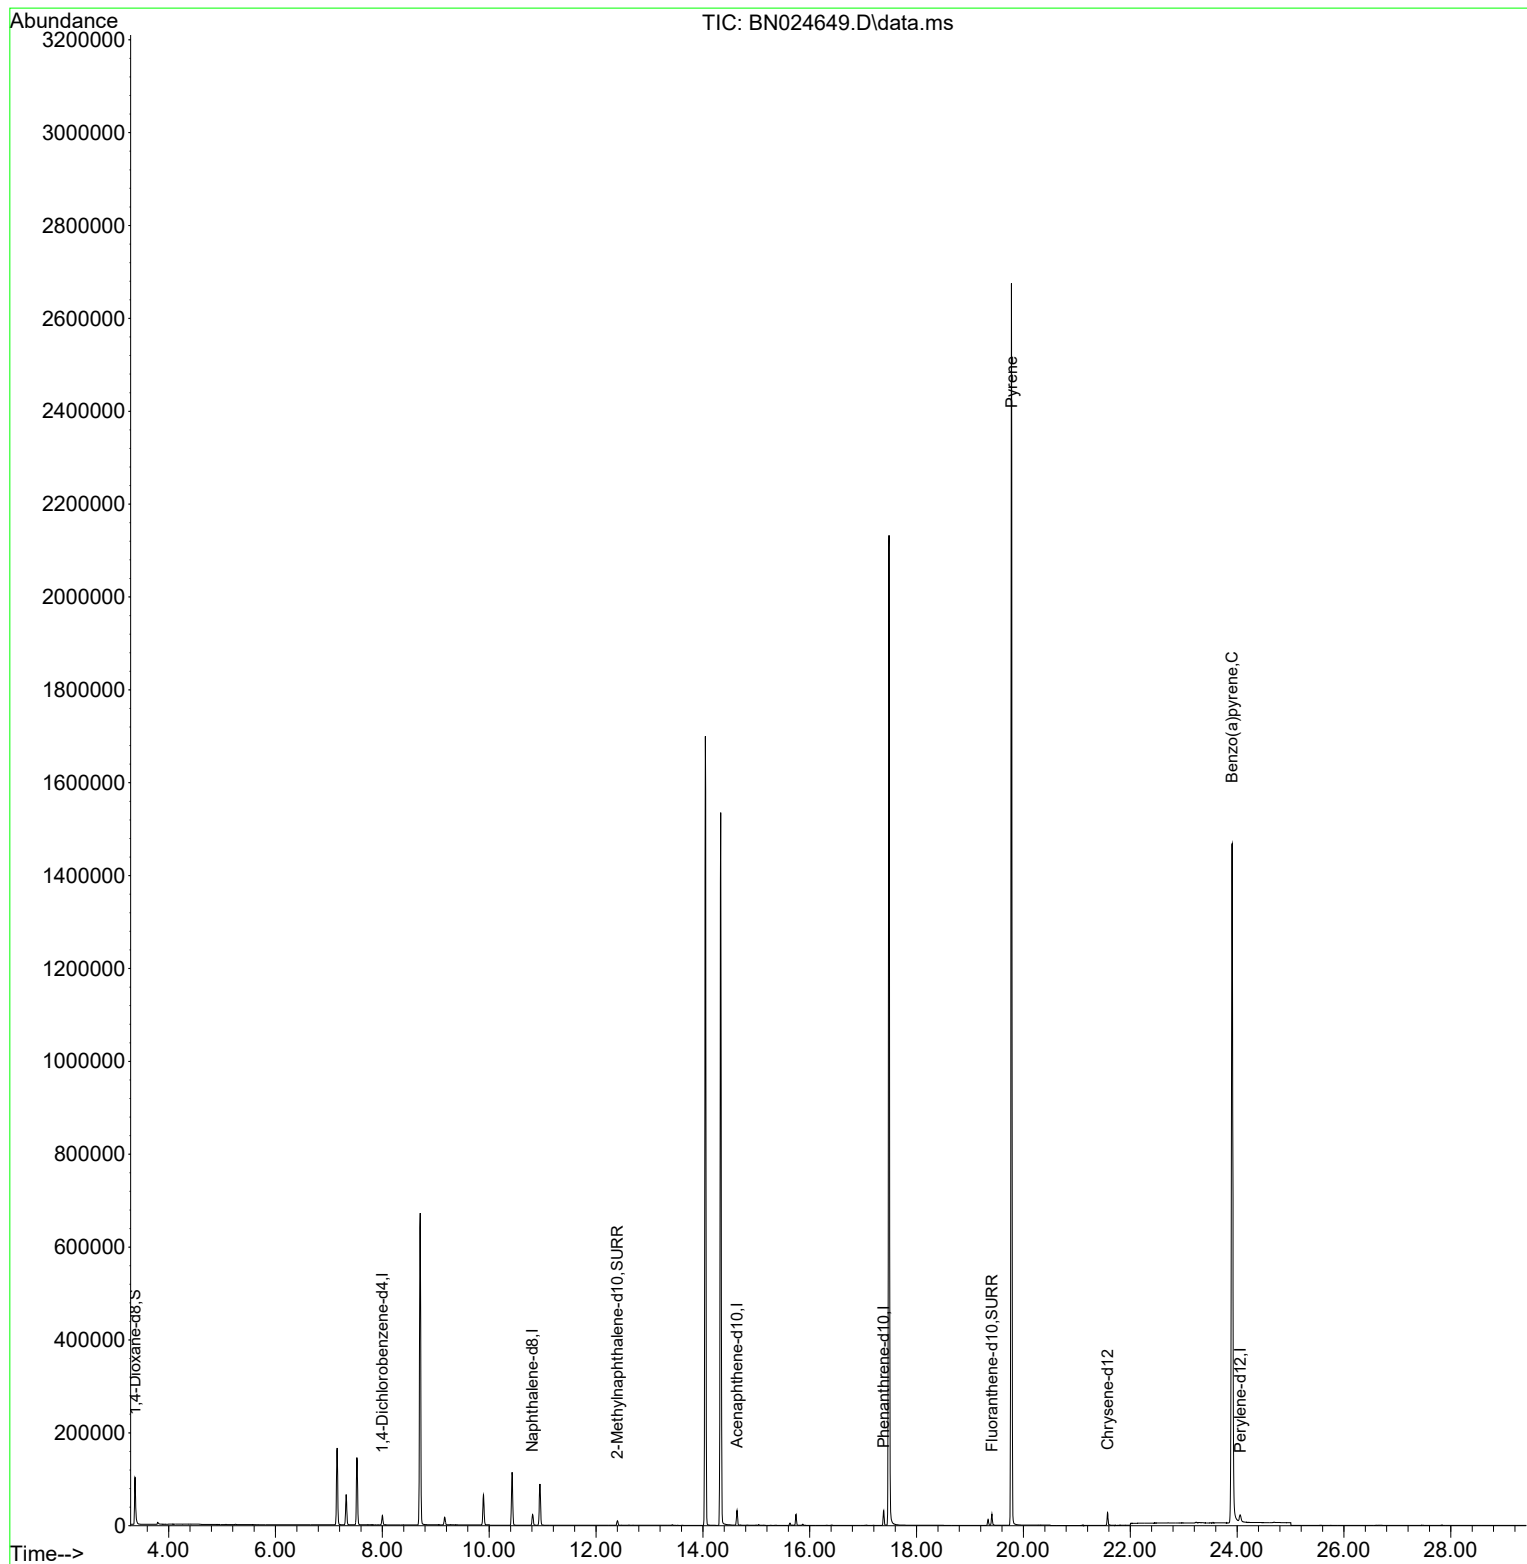


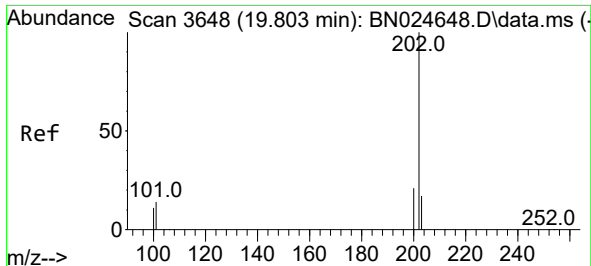

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.776 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN024649.D
Acq: 30 Mar 2023 18:59

Instrument :
BNA_N
ClientSampleId :
SBLK688

Tgt Ion:202 Resp: 4888
Ion Ratio Lower Upper
202 100
101 172.3 10.9 16.3#
100 1261.8 8.7 13.1#

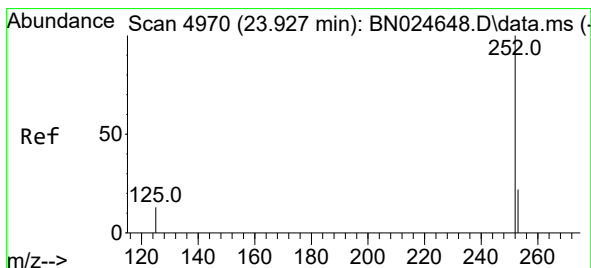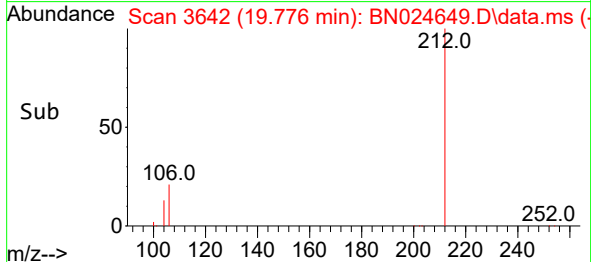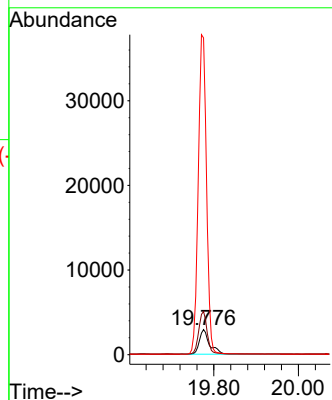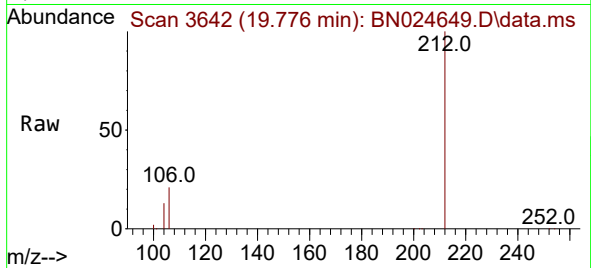

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.904 min Scan# 4962
Delta R.T. -0.023 min
Lab File: BN024649.D
Acq: 30 Mar 2023 18:59

Tgt Ion:252 Resp: 9151
Ion Ratio Lower Upper
252 100
253 44.5 21.8 32.8#
125 40.4 15.4 23.0#

