

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024650.D
 Acq On : 30 Mar 2023 19:36
 Operator : CG/JU
 Sample : PB151683BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK683

Quant Time: Mar 31 02:13:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	7888	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	23946	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	13689	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	28717	0.400	ng/ul	0.00
17) Chrysene-d12	21.574	240	21103	0.400	ng/ul	0.00
23) Perylene-d12	24.059	264	19498	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	69115	8.536	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.401	152	14326	0.485	ng/ul	0.00
18) Fluoranthene-d10	19.413	212	29085	0.563	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.633	166	4767	0.099	ng/ul#	12
20) Pyrene	19.775	202	4614	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.907	252	9997	0.157	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024650.D
Acq On : 30 Mar 2023 19:36
Operator : CG/JU
Sample : PB151683BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK683

Quant Time: Mar 31 02:13:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration




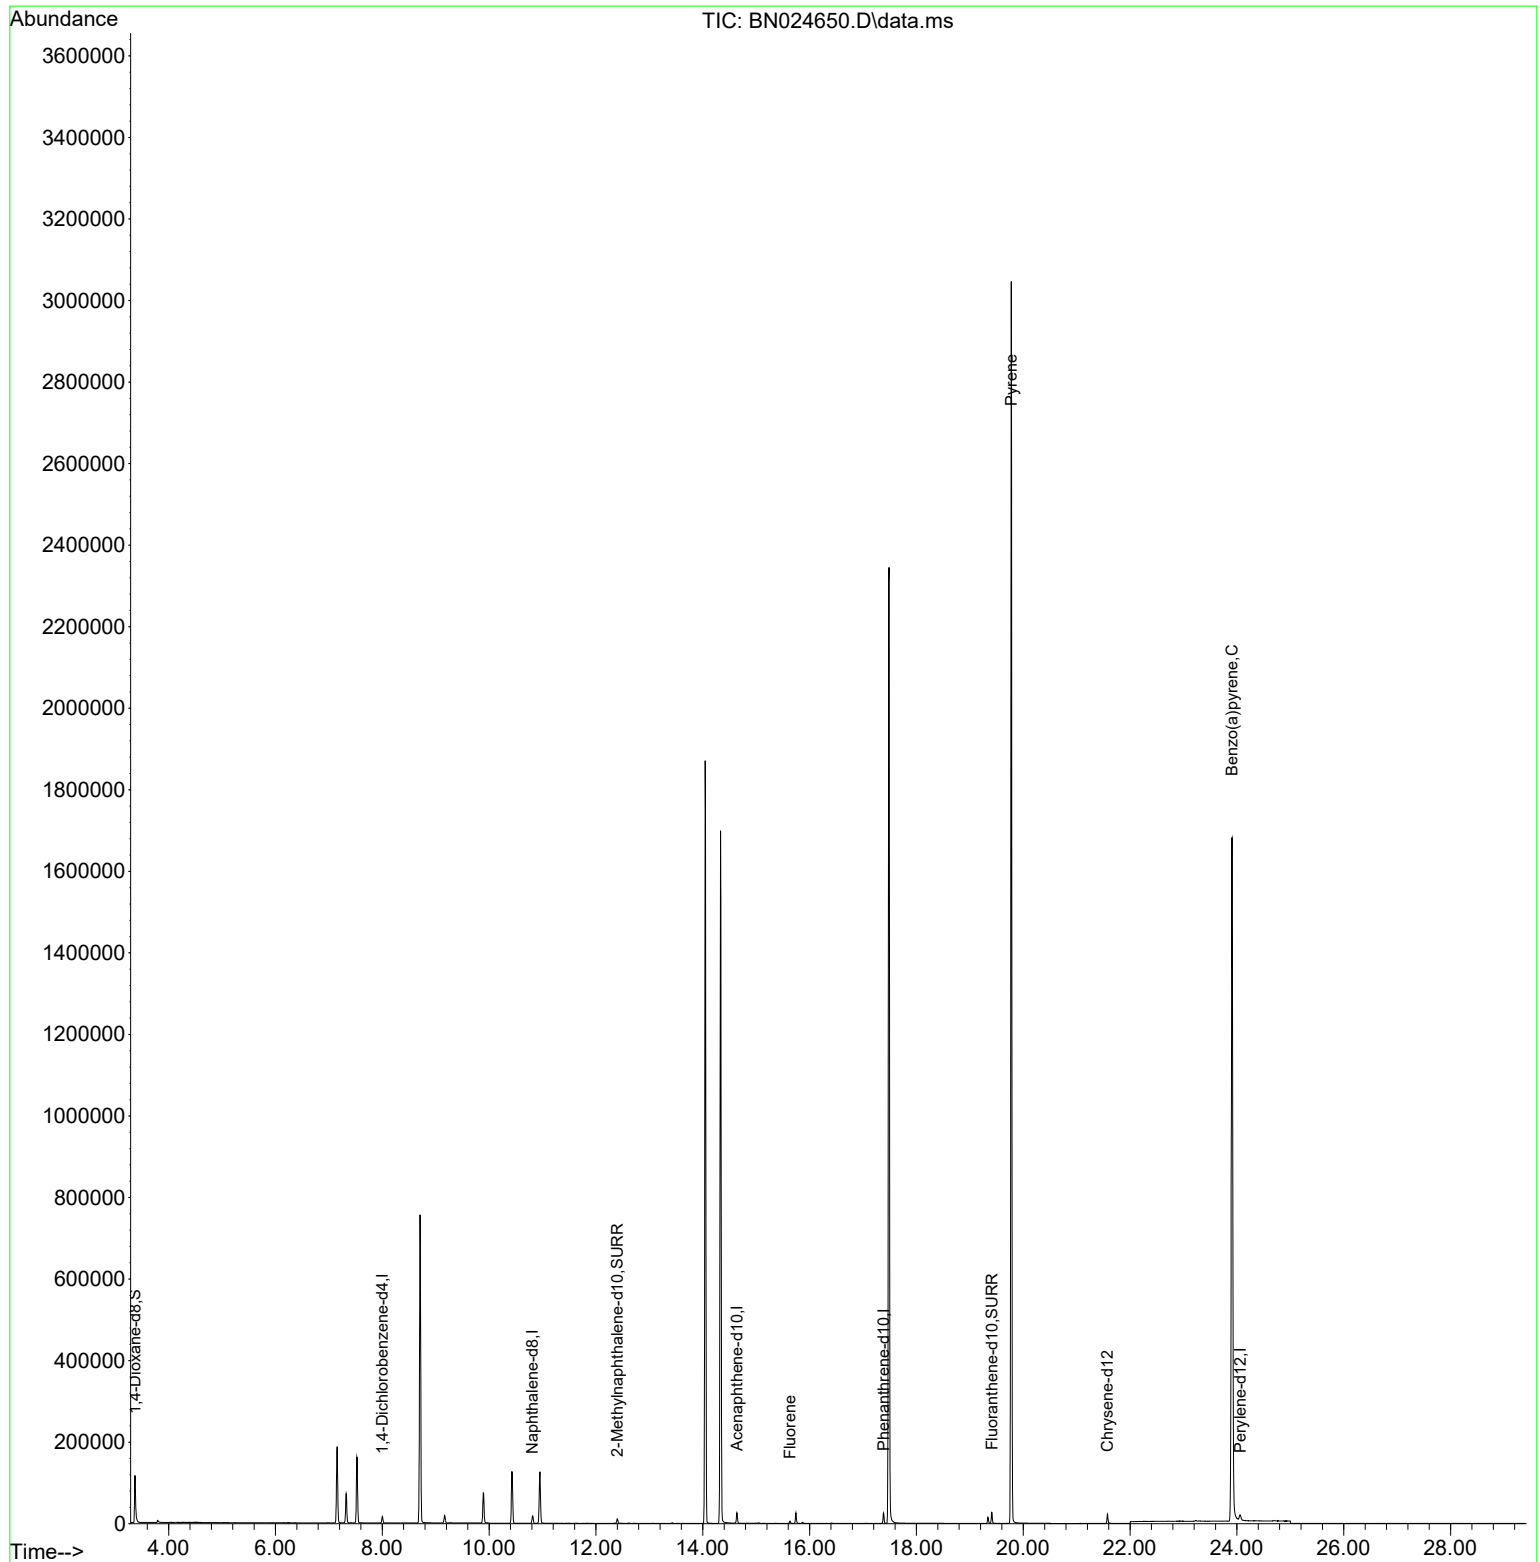


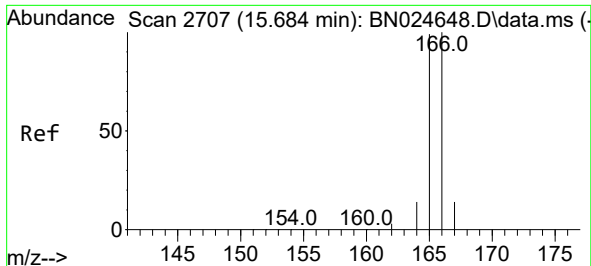

#12
Fluorene
Concen: 0.099 ng/ul
RT: 15.633 min Scan# 2696
Delta R.T. -0.051 min
Lab File: BN024650.D
Acq: 30 Mar 2023 19:36




Instrument :
BNA_N
ClientSampleId :
SBLK683


Tgt Ion:166 Resp: 4767
Ion Ratio Lower Upper
166 100
165 7.7 80.0 120.0#
167 36.0 10.8 16.2#

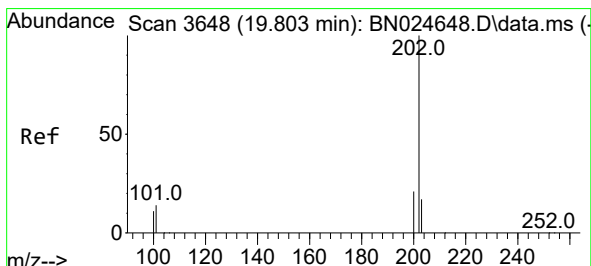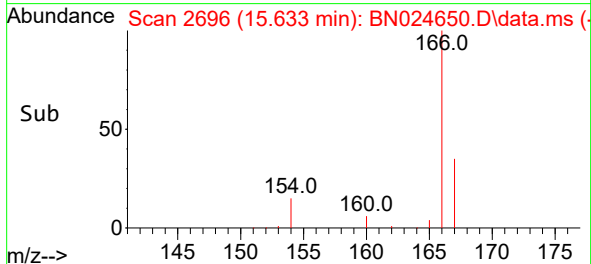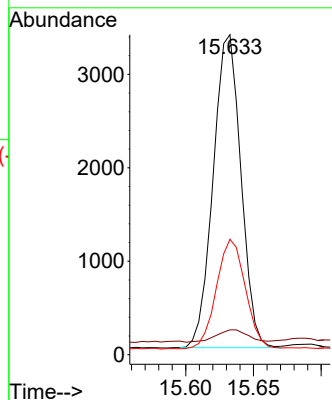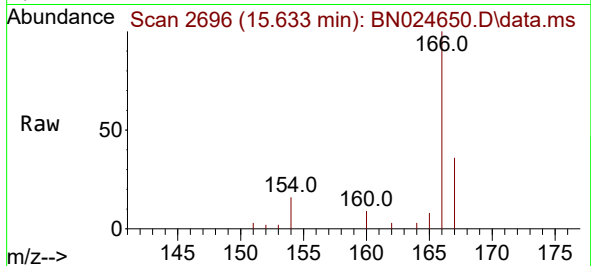

#20
Pyrene
Concen: 0.061 ng/ul
RT: 19.775 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN024650.D
Acq: 30 Mar 2023 19:36


Tgt Ion:202 Resp: 4614
Ion Ratio Lower Upper
202 100
101 172.8 10.9 16.3#
100 1282.4 8.7 13.1#

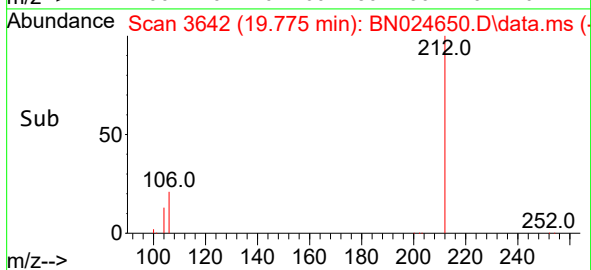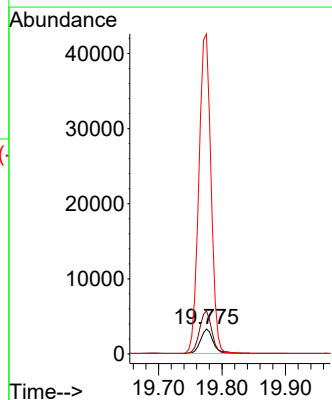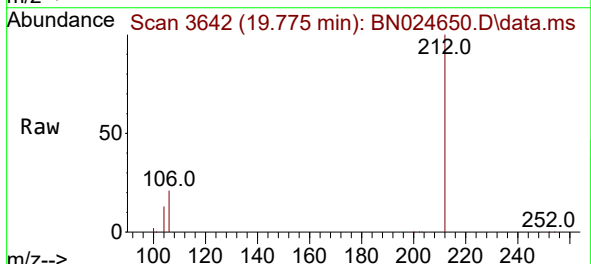

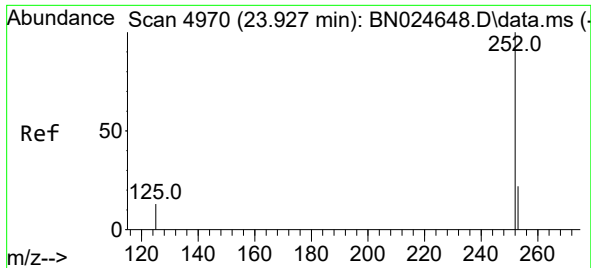

#26
Benzo(a)pyrene
Concen: 0.157 ng/ul
RT: 23.907 min Scan# 4963
Delta R.T. -0.021 min
Lab File: BN024650.D
Acq: 30 Mar 2023 19:36

Instrument :
BNA_N
ClientSampleId :
SBLK683

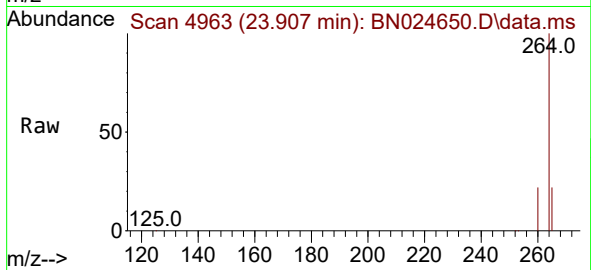

Tgt Ion:252 Resp: 9997
Ion Ratio Lower Upper
252 100
253 44.8 21.8 32.8#
125 39.7 15.4 23.0#

