

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024672.D
 Acq On : 31 Mar 2023 10:11
 Operator : CG/JU
 Sample : 02041-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB956

Quant Time: Apr 01 00:45:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	9341	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	28310	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	16400	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	35368	0.400	ng/ul	0.00
17) Chrysene-d12	21.565	240	26835	0.400	ng/ul	0.00
23) Perylene-d12	24.035	264	25692	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	48735	5.083	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	11836	0.339	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	32160	0.490	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	43152	4.278	ng/ul	90
20) Pyrene	19.771	202	4981	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.877	252	9040	0.108	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024672.D
Acq On : 31 Mar 2023 10:11
Operator : CG/JU
Sample : 02041-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB956

Quant Time: Apr 01 00:45:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration




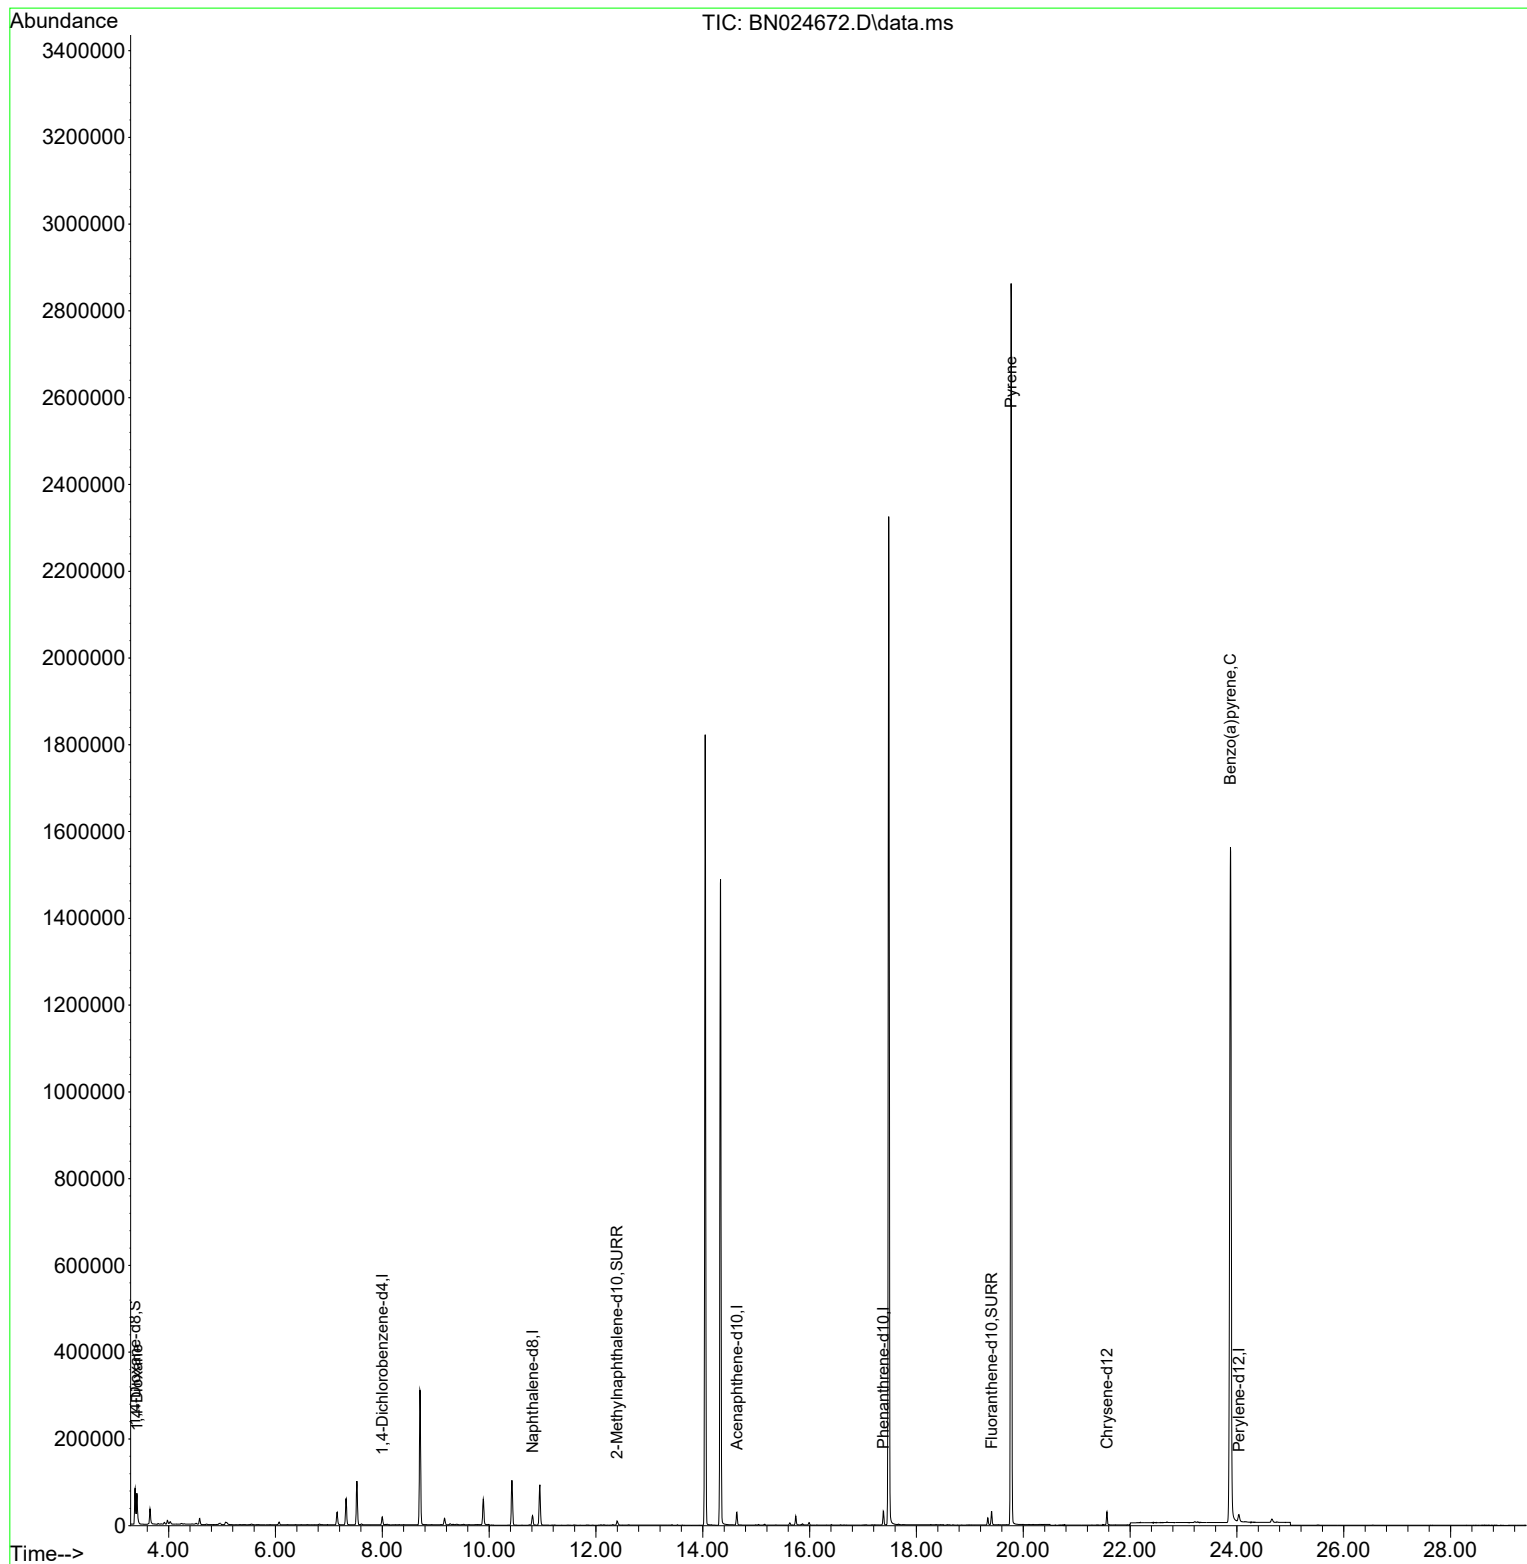


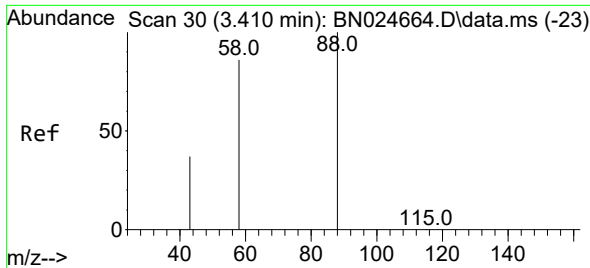

#2
1,4-Dioxane
Concen: 4.278 ng/ul
RT: 3.405 min Scan# 29
Delta R.T. -0.004 min
Lab File: BN024672.D
Acq: 31 Mar 2023 10:11




Instrument :
BNA_N
ClientSampleId :
CB956


Tgt Ion: 88 Resp: 43152
Ion Ratio Lower Upper
88 100
43 41.7 37.2 55.8
58 86.3 61.5 92.3

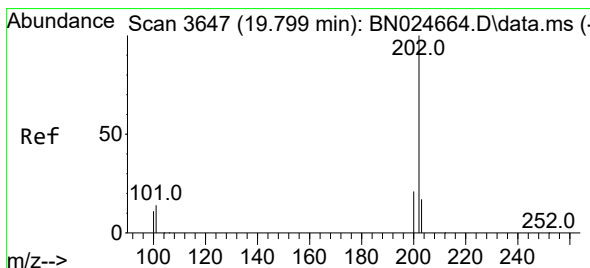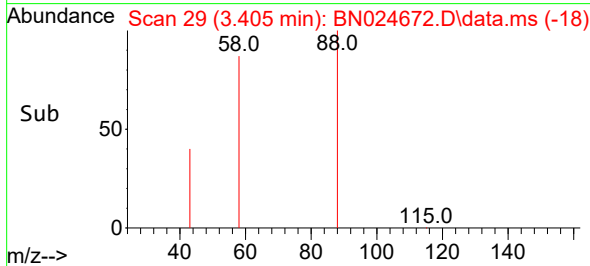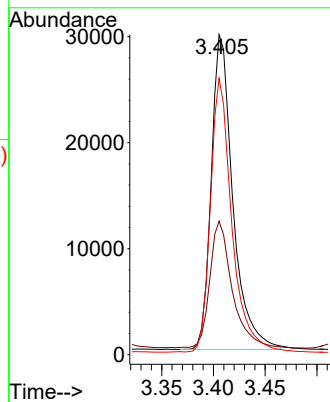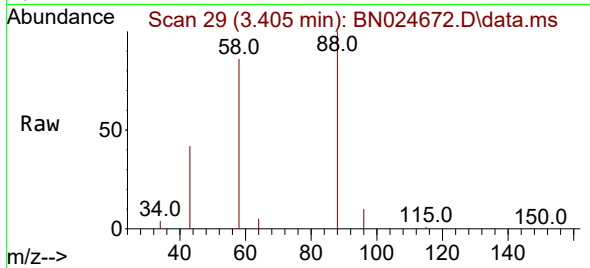

#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.771 min Scan# 3641
Delta R.T. -0.033 min
Lab File: BN024672.D
Acq: 31 Mar 2023 10:11


Tgt Ion: 202 Resp: 4981
Ion Ratio Lower Upper
202 100
101 173.7 10.9 16.3#
100 1301.7 8.7 13.1#

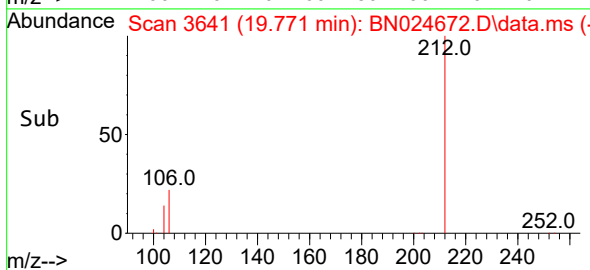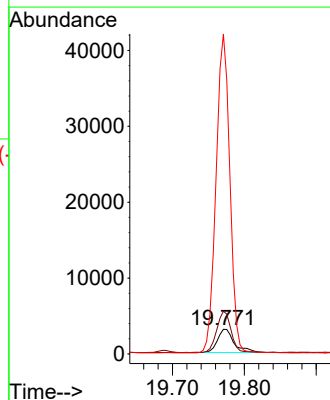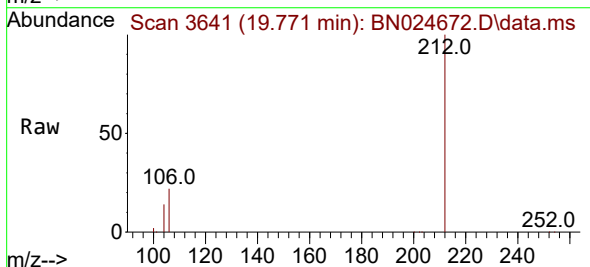

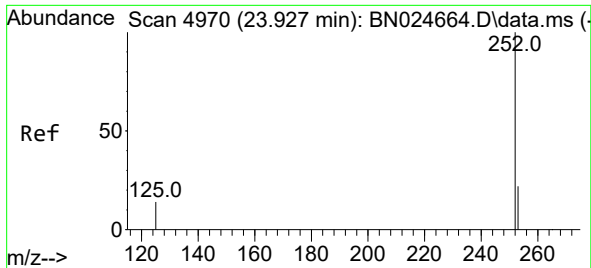

#26
 Benzo(a)pyrene
 Concen: 0.108 ng/ul
 RT: 23.877 min Scan# 4953
 Delta R.T. -0.050 min
 Lab File: BN024672.D
 Acq: 31 Mar 2023 10:11

Instrument :
 BNA_N
 ClientSampleId :
 CB956

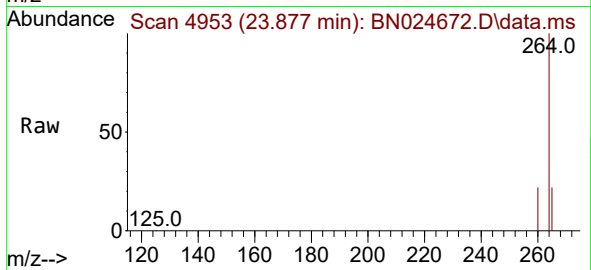

Tgt Ion:252 Resp: 9040
 Ion Ratio Lower Upper
 252 100
 253 49.3 21.8 32.8#
 125 46.9 15.4 23.0#

