

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024679.D
 Acq On : 31 Mar 2023 15:03
 Operator : CG/JU
 Sample : PB151732BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK732

Quant Time: Apr 01 01:01:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	9361	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	28283	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	16165	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	33721	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	25099	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	24677	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	61827	6.435	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13210	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	27053	0.440	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.628	166	4281	0.076	ng/ul#	14
20) Pyrene	19.771	202	4157	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.883	252	8081	0.100	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024679.D
Acq On : 31 Mar 2023 15:03
Operator : CG/JU
Sample : PB151732BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK732

Quant Time: Apr 01 01:01:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 01:00:20 2023
Response via : Initial Calibration




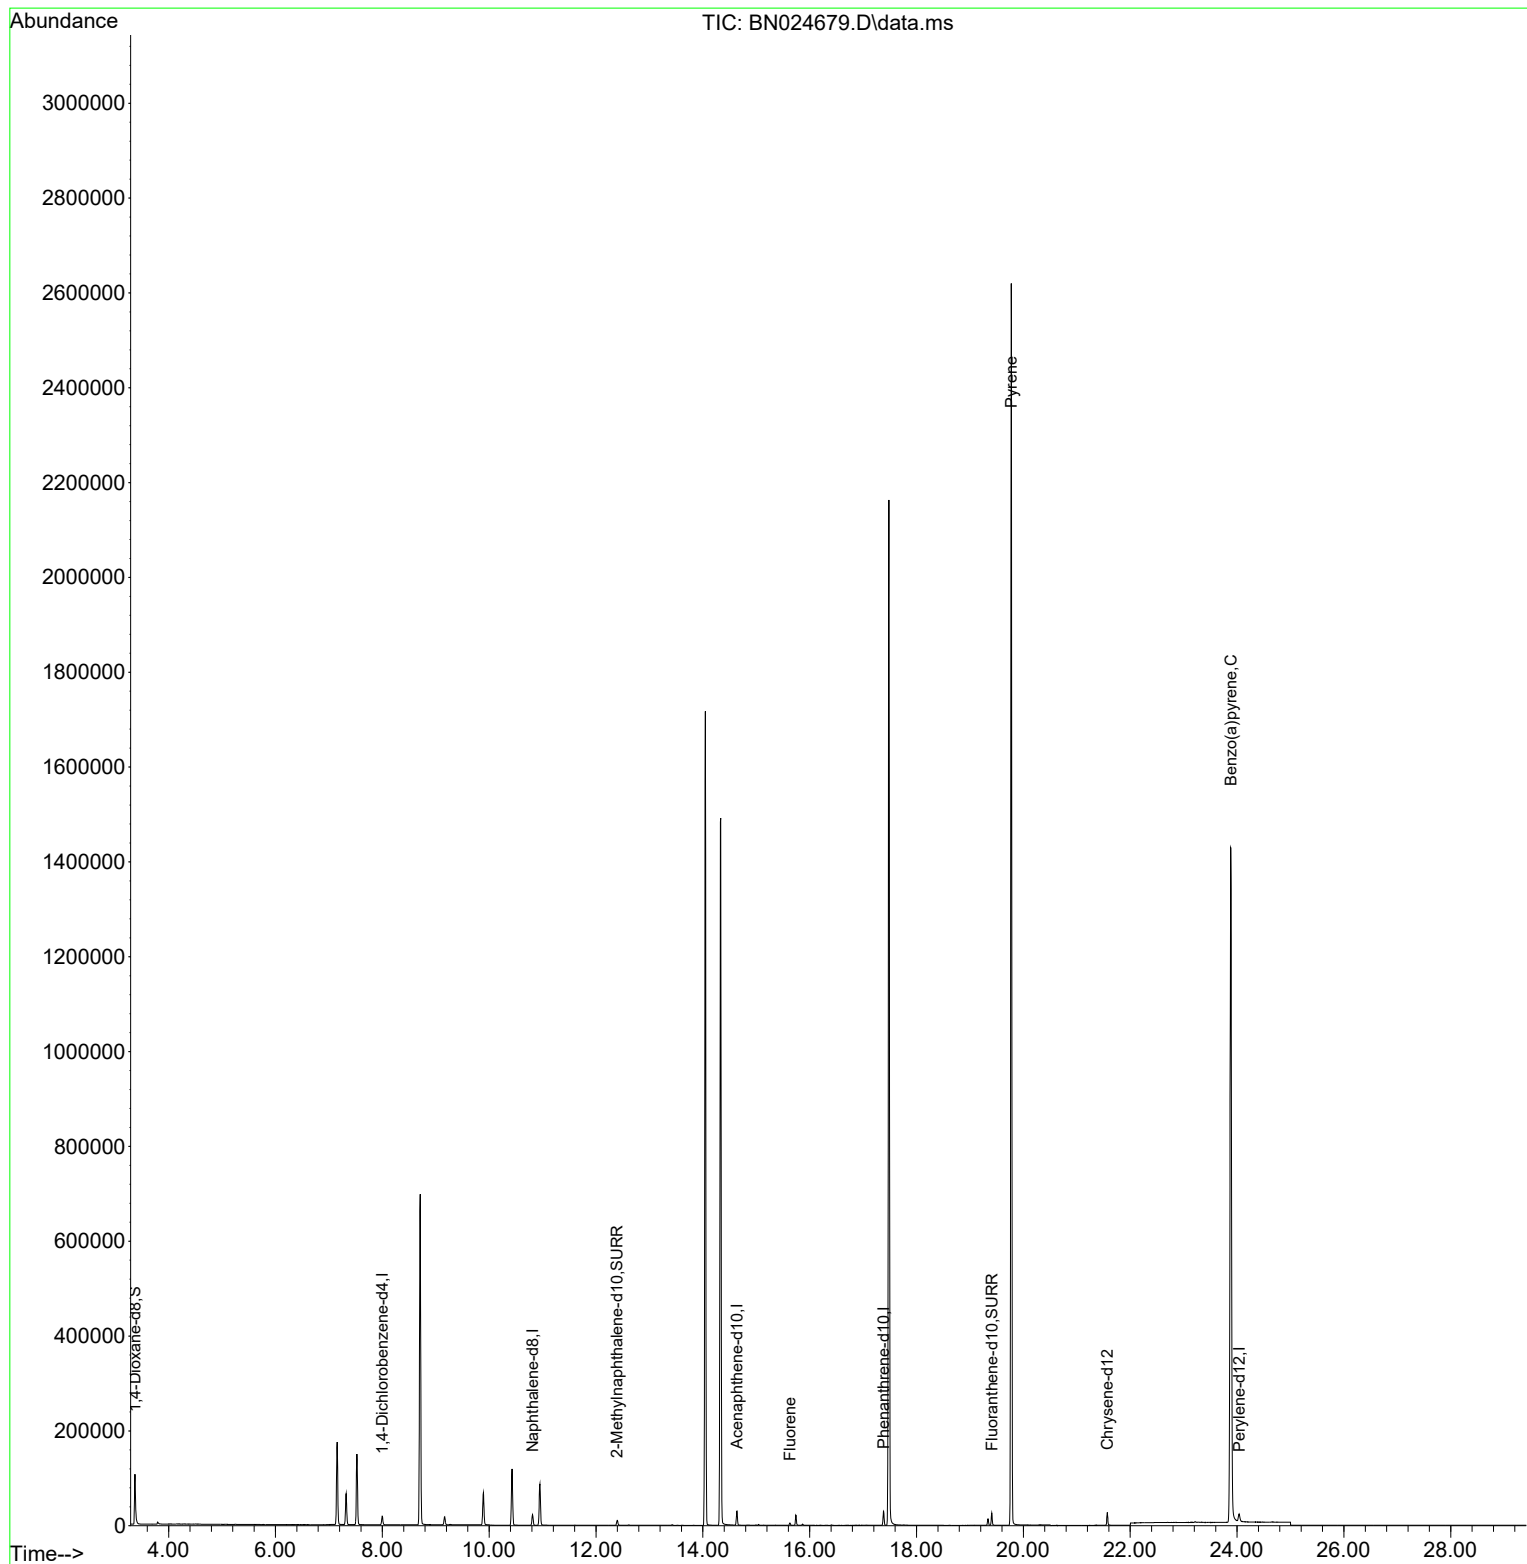


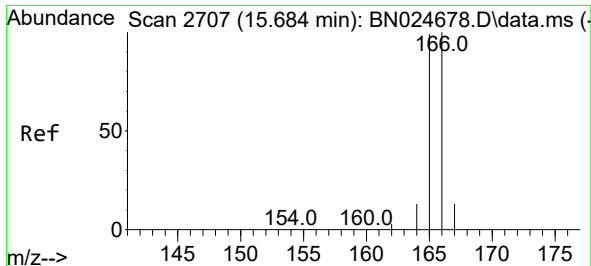

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.628 min Scan# 20
Delta R.T. -0.056 min
Lab File: BN024679.D
Acq: 31 Mar 2023 15:03




Instrument :
BNA_N
ClientSampleId :
SBLK732


Tgt Ion:166 Resp: 4281
Ion Ratio Lower Upper
166 100
165 8.7 80.0 120.0#
167 33.6 10.8 16.2#

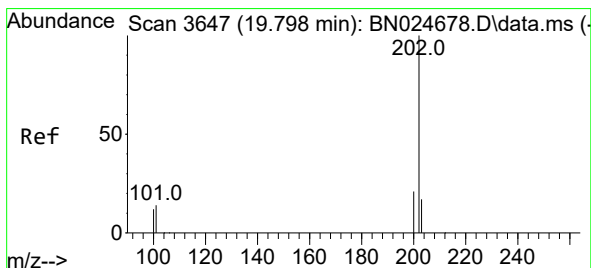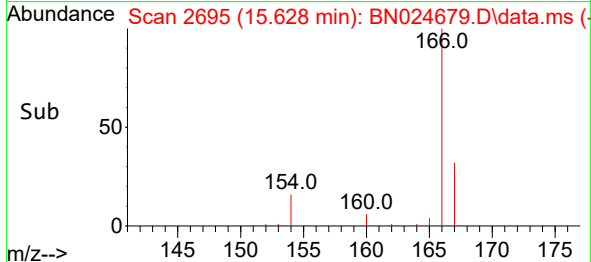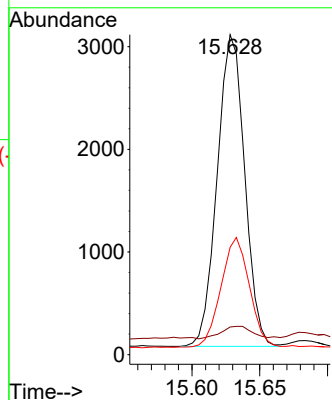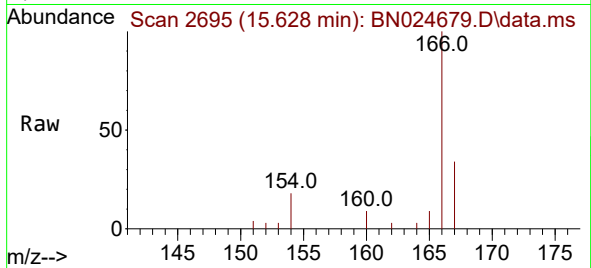

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.771 min Scan# 3641
Delta R.T. -0.028 min
Lab File: BN024679.D
Acq: 31 Mar 2023 15:03


Tgt Ion:202 Resp: 4157
Ion Ratio Lower Upper
202 100
101 175.8 10.9 16.3#
100 1337.2 8.7 13.1#

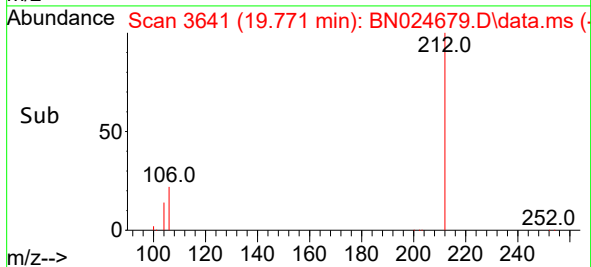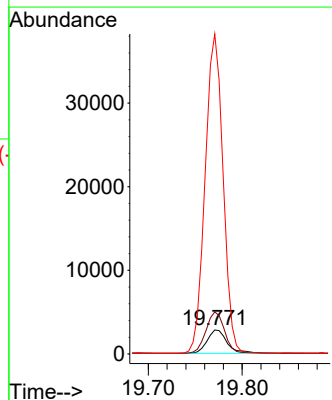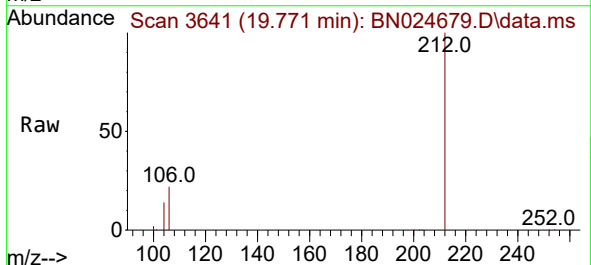

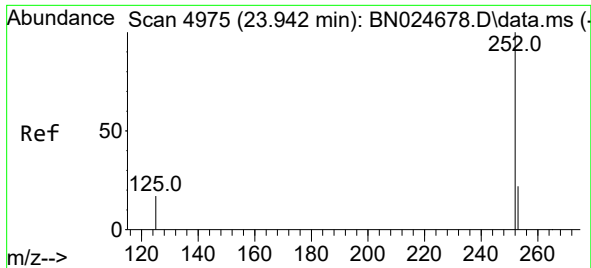

#26
Benzo(a)pyrene
Concen: 0.100 ng/ul
RT: 23.883 min Scan# 4955
Delta R.T. -0.058 min
Lab File: BN024679.D
Acq: 31 Mar 2023 15:03

Instrument :
BNA_N
ClientSampleId :
SBLK732

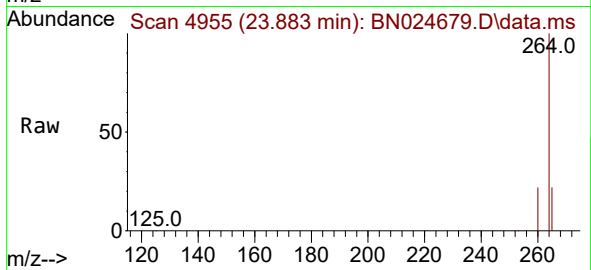

Tgt Ion:252 Resp: 8081
Ion Ratio Lower Upper
252 100
253 49.9 21.8 32.8#
125 44.5 15.4 23.0#

