

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024711.D
 Acq On : 01 Apr 2023 11:09
 Operator : CG/JU
 Sample : PB151702BL
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK702

Quant Time: Apr 03 01:36:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8205	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	25309	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.633	164	14368	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	30051	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	21937	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	20448	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	58237	6.915	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	12670	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	26086	0.486	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.628	166	4258	0.085	ng/ul#	12
20) Pyrene	19.771	202	3959	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.880	252	7489	0.112	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024711.D
Acq On : 01 Apr 2023 11:09
Operator : CG/JU
Sample : PB151702BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK702

Quant Time: Apr 03 01:36:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration




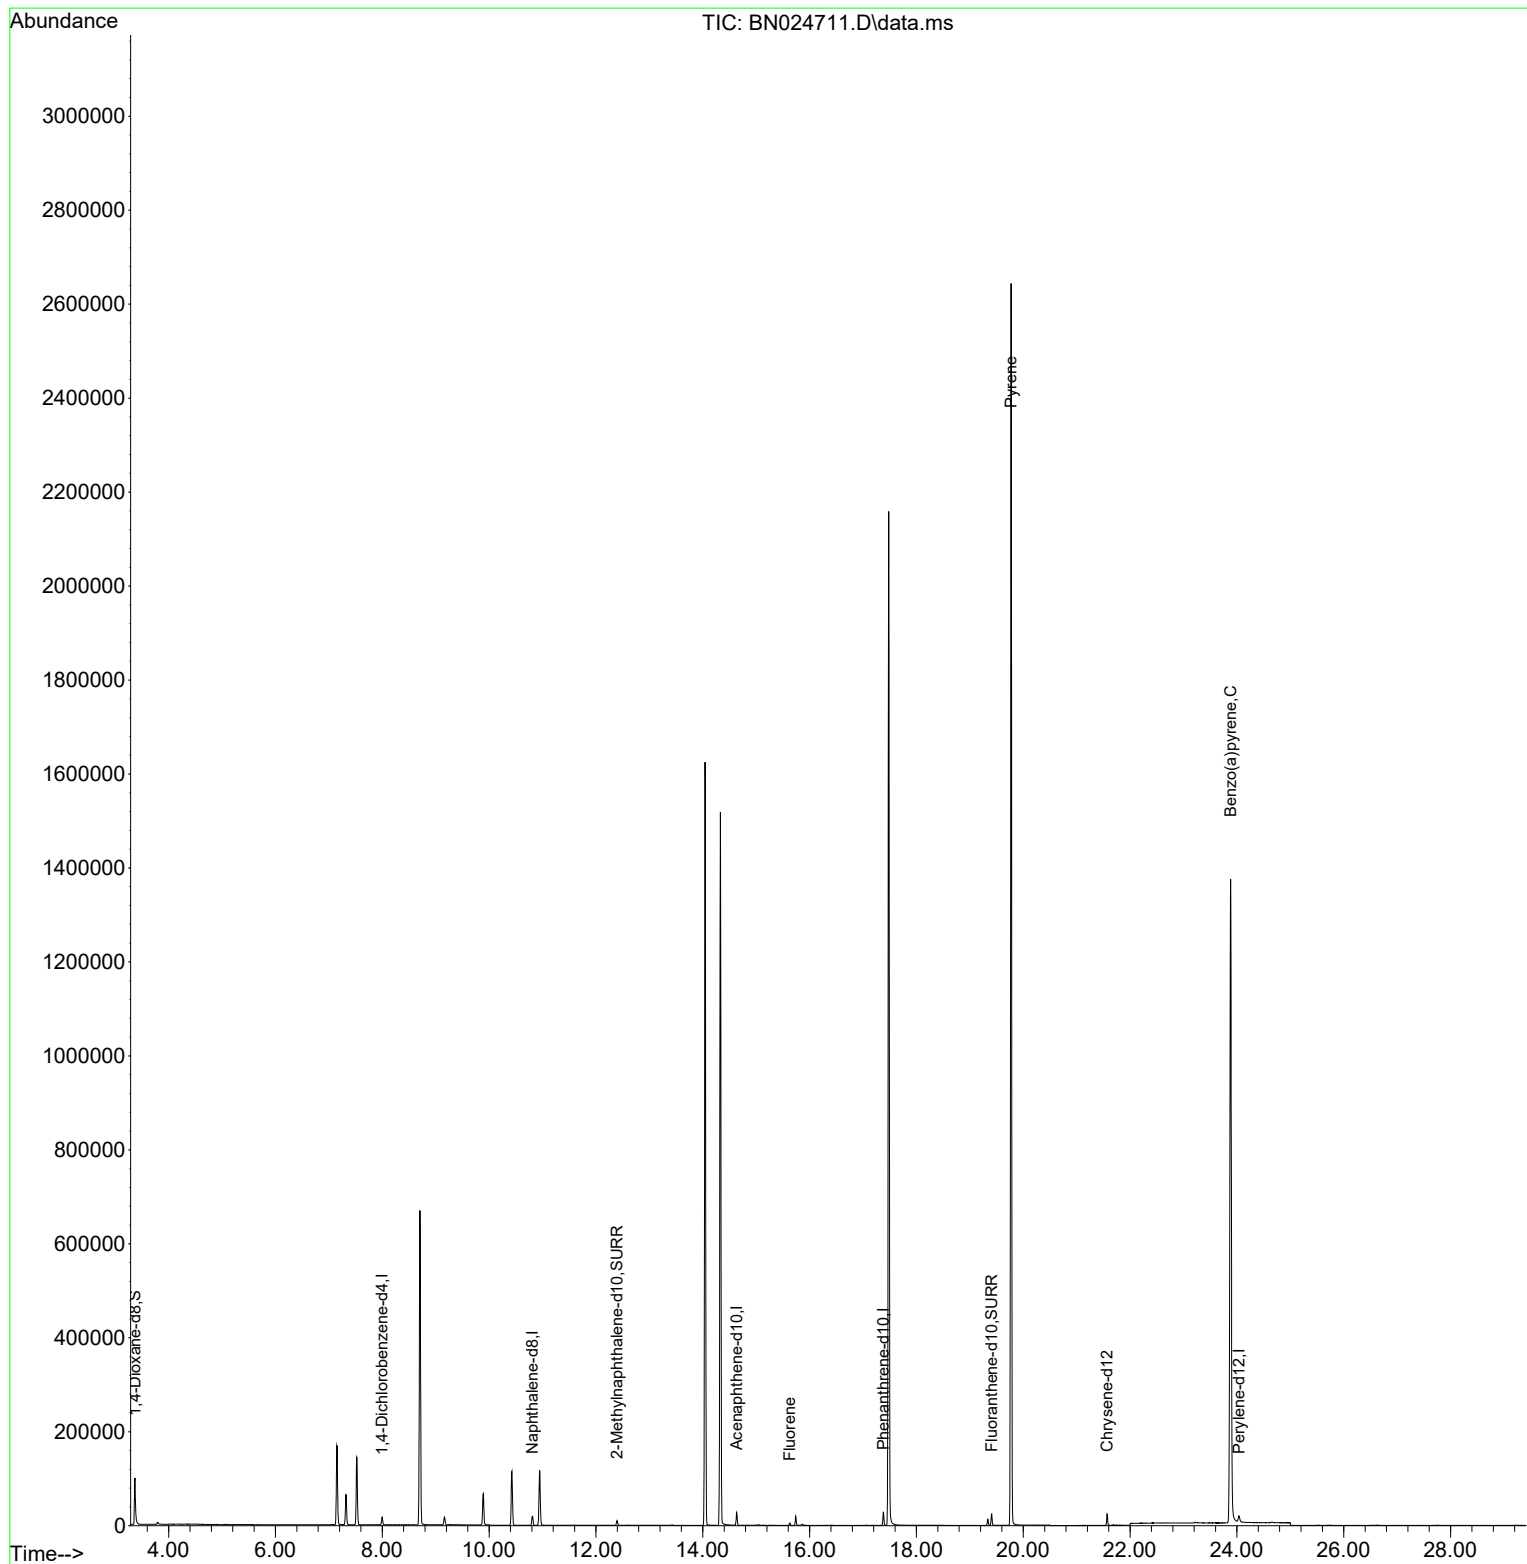


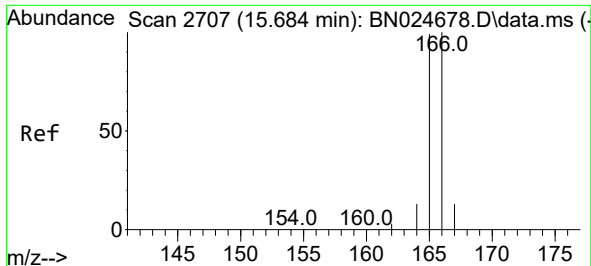

#12
Fluorene
Concen: 0.085 ng/ul
RT: 15.628 min Scan# 20
Delta R.T. -0.055 min
Lab File: BN024711.D
Acq: 01 Apr 2023 11:09




Instrument :
BNA_N
ClientSampleId :
SBLK702


Tgt Ion:166 Resp: 4258
Ion Ratio Lower Upper
166 100
165 7.9 80.0 120.0#
167 35.4 10.8 16.2#

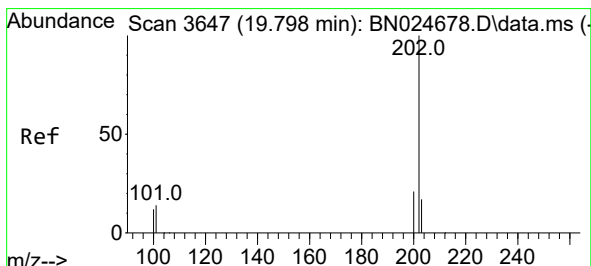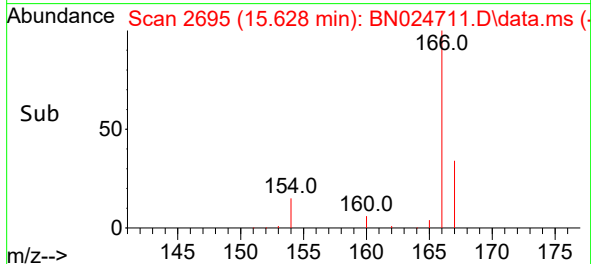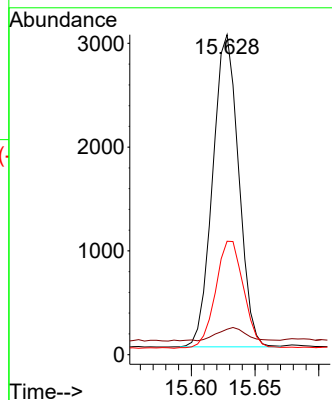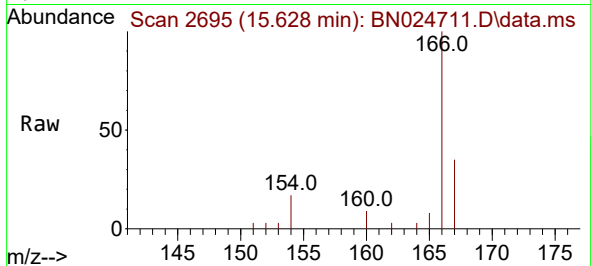

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.771 min Scan# 3641
Delta R.T. -0.028 min
Lab File: BN024711.D
Acq: 01 Apr 2023 11:09


Tgt Ion:202 Resp: 3959
Ion Ratio Lower Upper
202 100
101 177.9 10.9 16.3#
100 1346.6 8.7 13.1#

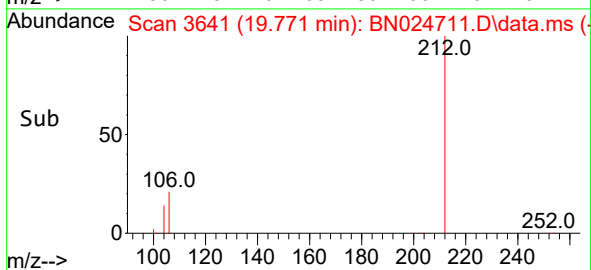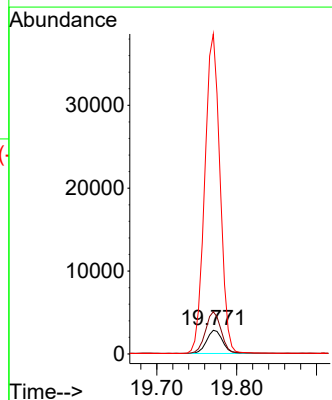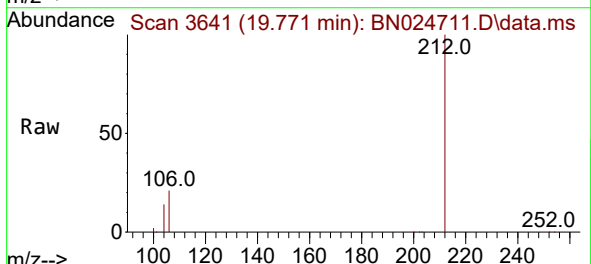

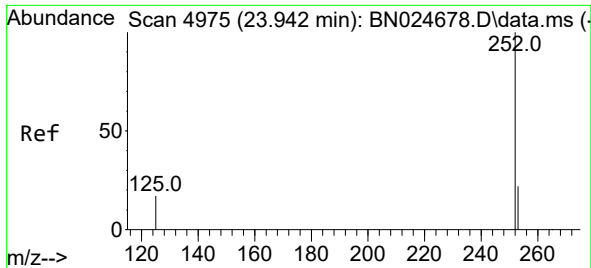

#26
Benzo(a)pyrene
Concen: 0.112 ng/ul
RT: 23.880 min Scan# 4954
Delta R.T. -0.058 min
Lab File: BN024711.D
Acq: 01 Apr 2023 11:09

Instrument :
BNA_N
ClientSampleId :
SBLK702

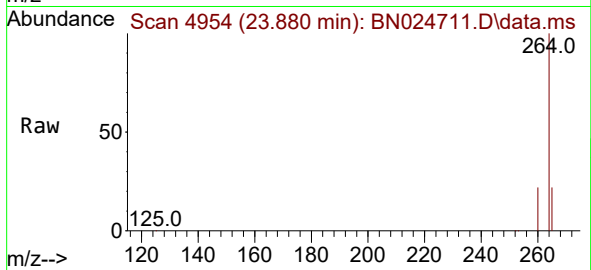

Tgt Ion:252 Resp: 7489
Ion Ratio Lower Upper
252 100
253 45.7 21.8 32.8#
125 42.6 15.4 23.0#

