




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024687.D
 Acq On : 31 Mar 2023 19:55
 Operator : CG/JU
 Sample : 02010-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB944

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:02:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

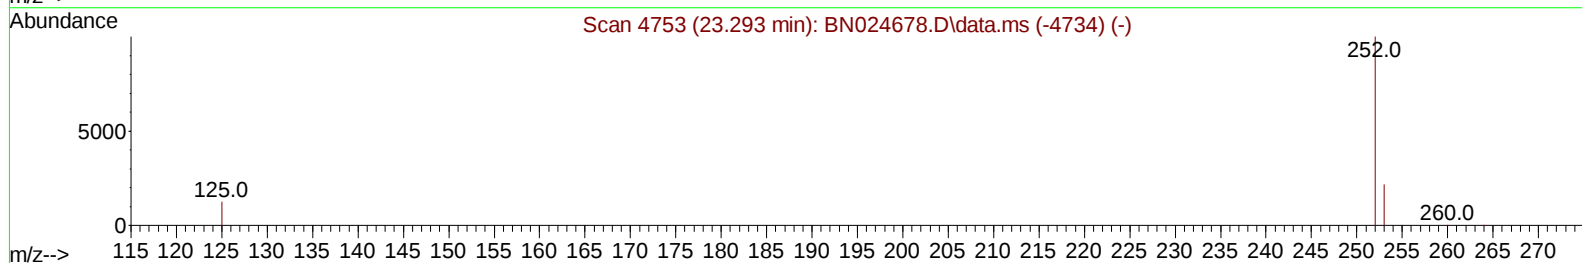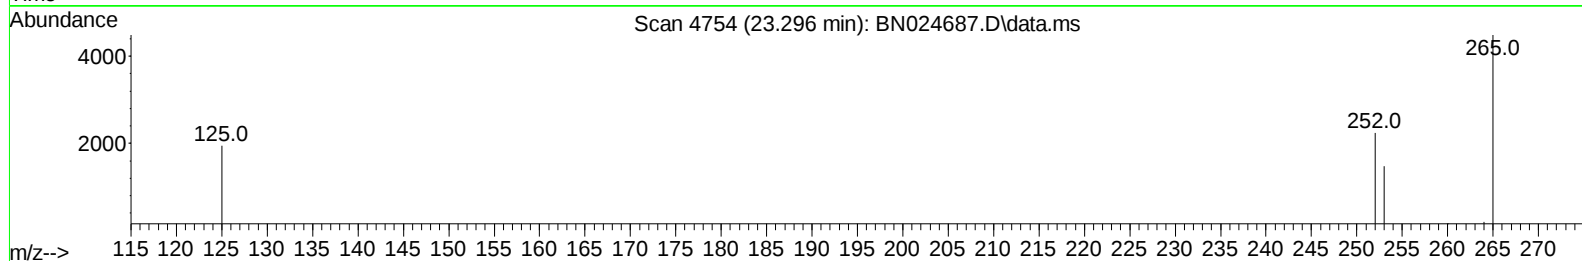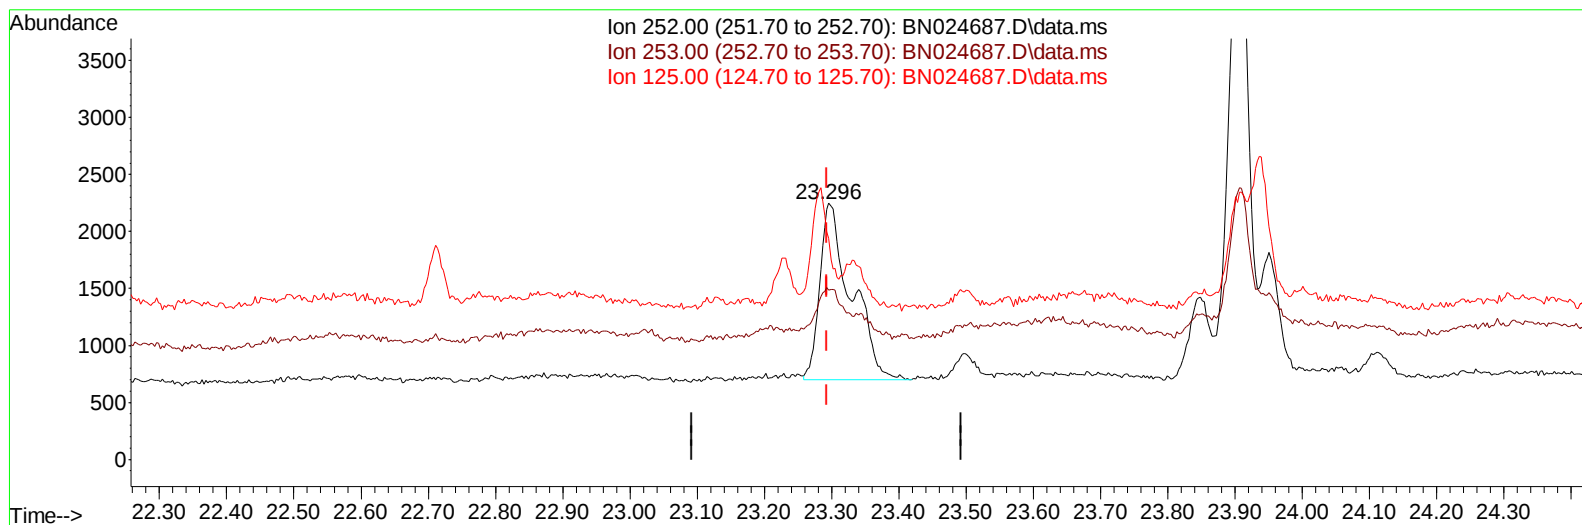

TIC: BN024687.D\data.ms

(24) Benzo(b)fluoranthene

23.296min (+ 0.003) 0.05 ng/u1

response 4990

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.80	66.06#
125.00	16.20	86.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024687.D
 Acq On : 31 Mar 2023 19:55
 Operator : CG/JU
 Sample : 02010-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB944

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:02:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

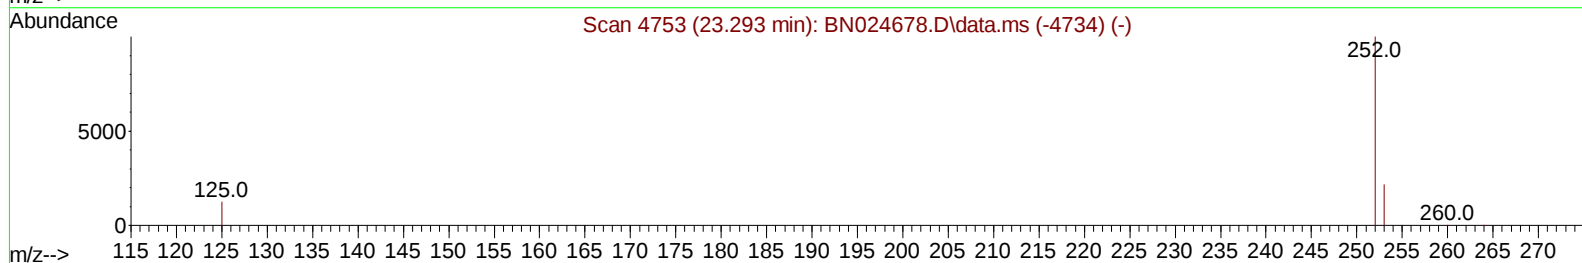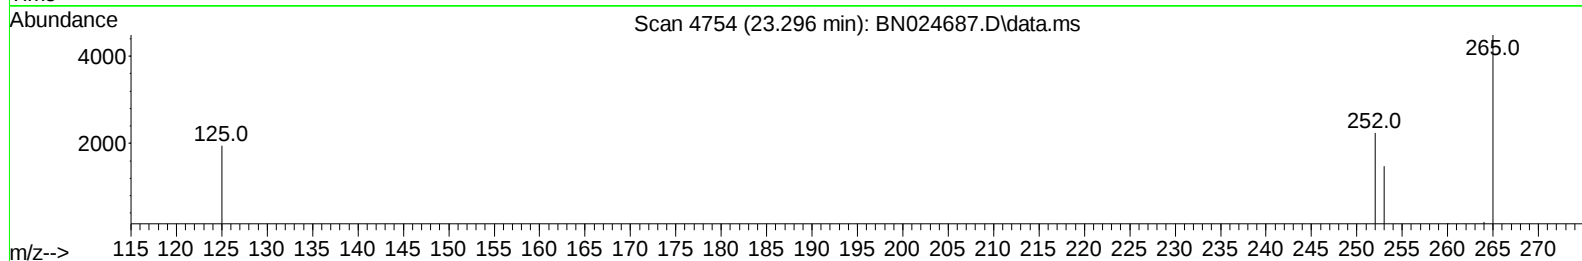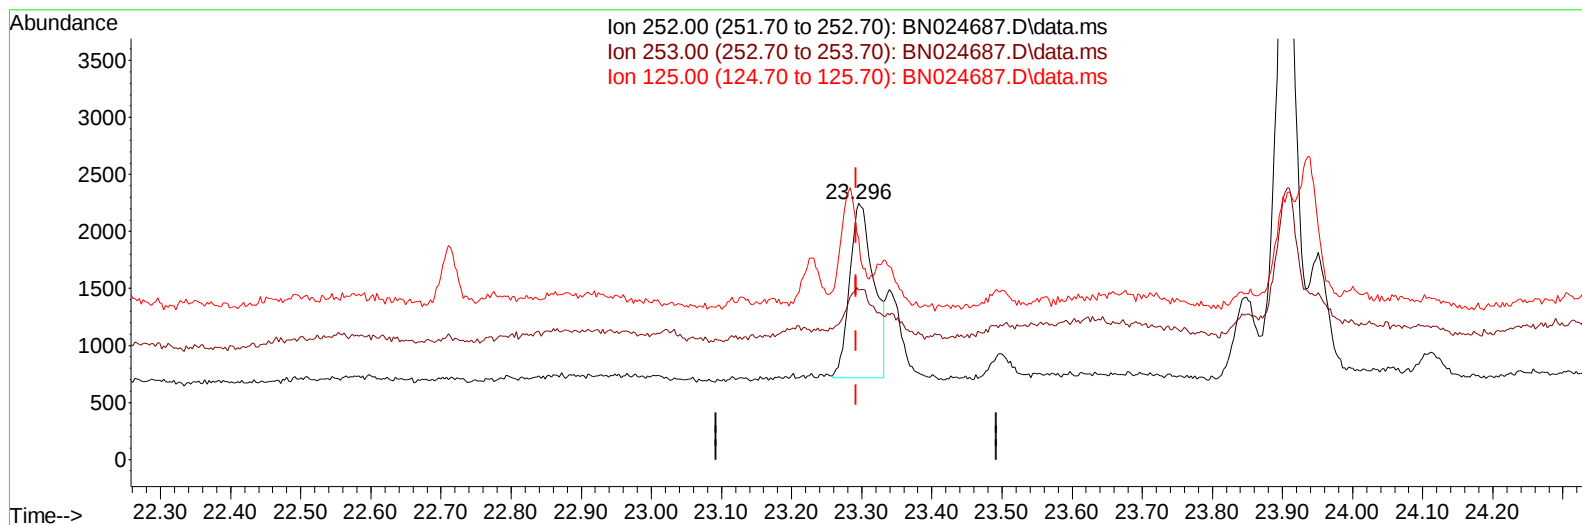

TIC: BN024687.D\data.ms

(24) Benzo(b)fluoranthene

23.296min (+ 0.003) 0.03 ng/u1 m

response 3636

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.80	66.06#
125.00	16.20	86.34#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024687.D
 Acq On : 31 Mar 2023 19:55
 Operator : CG/JU
 Sample : 02010-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB944

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 01:02:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	8657	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	26852	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	15859	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	33251	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	25792	0.400	ng/ul	0.00
23) Perylene-d12	24.056	264	25047	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	53491	6.020	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13841	0.418	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	33754	0.535	ng/ul	0.00
Target Compounds						Qvalue
15) Phenanthrene	17.422	178	2422	0.027	ng/ul#	81
19) Fluoranthene	19.436	202	5086	0.056	ng/ul#	90
21) Benzo(a)anthracene	21.554	228	2056	0.027	ng/ul#	77
22) Chrysene	21.609	228	2895	0.034	ng/ul#	80
24) Benzo(b)fluoranthene	23.296	252	3636m	0.035	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024687.D
Acq On : 31 Mar 2023 19:55
Operator : CG/JU
Sample : 02010-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB944

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:02:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 01:00:20 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

