

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024661.D
 Acq On : 31 Mar 2023 02:14
 Operator : CG/JU
 Sample : 02067-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ78

Quant Time: Mar 31 02:44:00 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	9880	0.400	ng/ul	0.00
4) Naphthalene-d8	10.811	136	30032	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	17434	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	37350	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	28901	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	27862	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	52322	5.159	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	14211	0.383	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	36967	0.523	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.409	88	1009	0.095	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024661.D
Acq On : 31 Mar 2023 02:14
Operator : CG/JU
Sample : 02067-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ78


Quant Time: Mar 31 02:44:00 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration

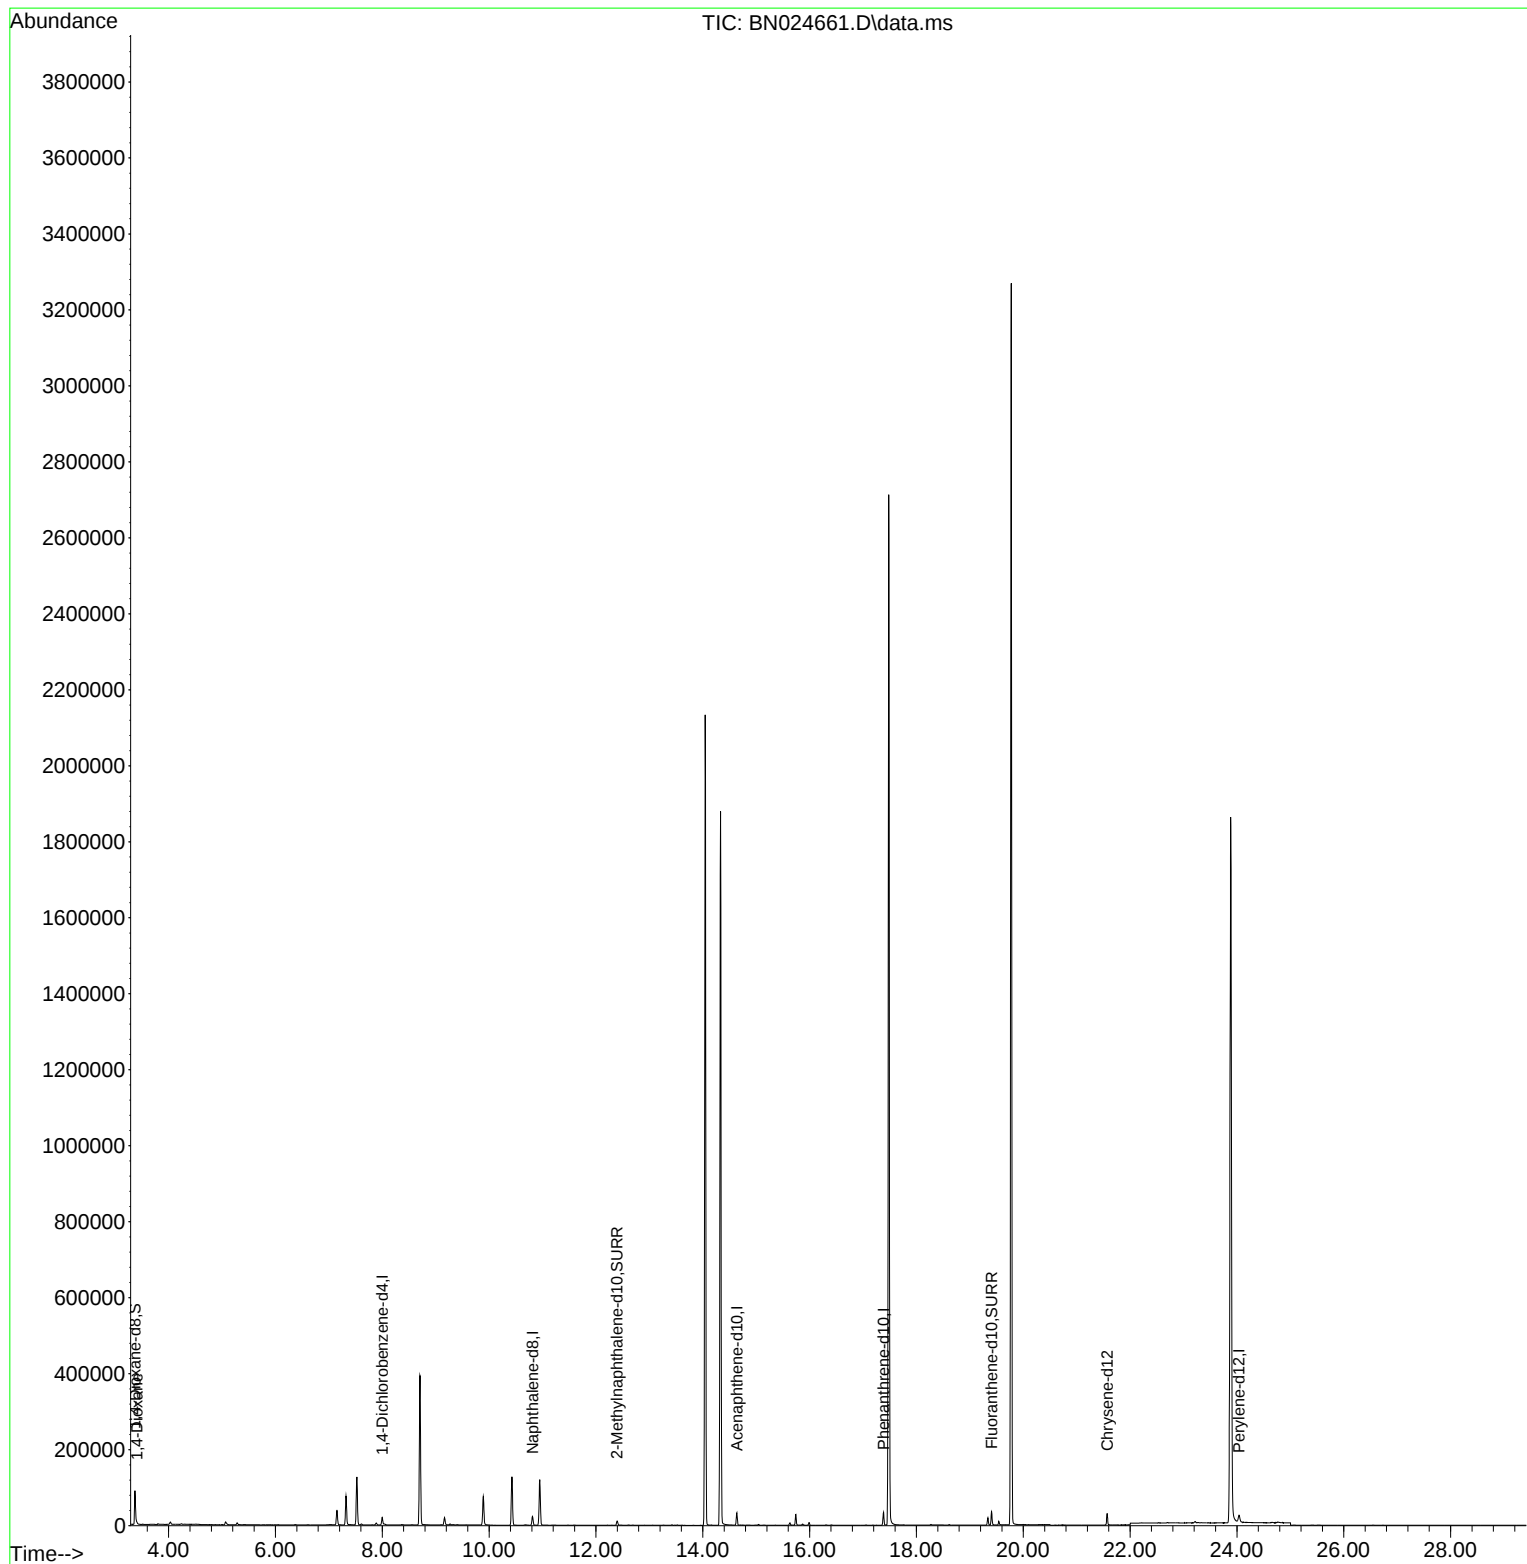

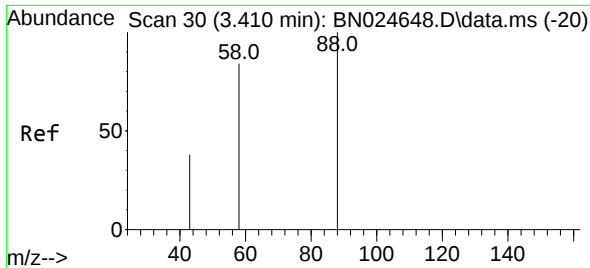

#2
 1,4-Dioxane
 Concen: 0.095 ng/ul
 RT: 3.409 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN024661.D
 Acq: 31 Mar 2023 02:14

Instrument :
 BNA_N
 ClientSampleId :
 BFZ78

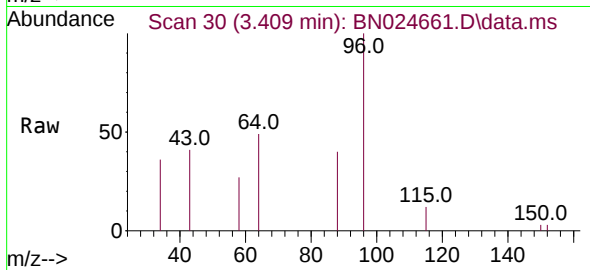

Tgt Ion: 88	Resp: 1009
Ion Ratio	Lower Upper
88	100
43	102.5 37.2 55.8#
58	66.7 61.5 92.3

