

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024662.D
 Acq On : 31 Mar 2023 02:50
 Operator : CG/JU
 Sample : 02067-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ85

Quant Time: Mar 31 04:00:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	8640	0.400	ng/u1	0.00
4) Naphthalene-d8	10.812	136	26185	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.638	164	15438	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.384	188	33066	0.400	ng/u1	0.00
17) Chrysene-d12	21.571	240	25193	0.400	ng/u1	0.00
23) Perylene-d12	24.041	264	24765	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	51721	5.832	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.396	152	14366	0.445	ng/u1	0.00
18) Fluoranthene-d10	19.408	212	39133	0.635	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.405	88	597	0.064	ng/u1#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024662.D
Acq On : 31 Mar 2023 02:50
Operator : CG/JU
Sample : 02067-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ85


Quant Time: Mar 31 04:00:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration

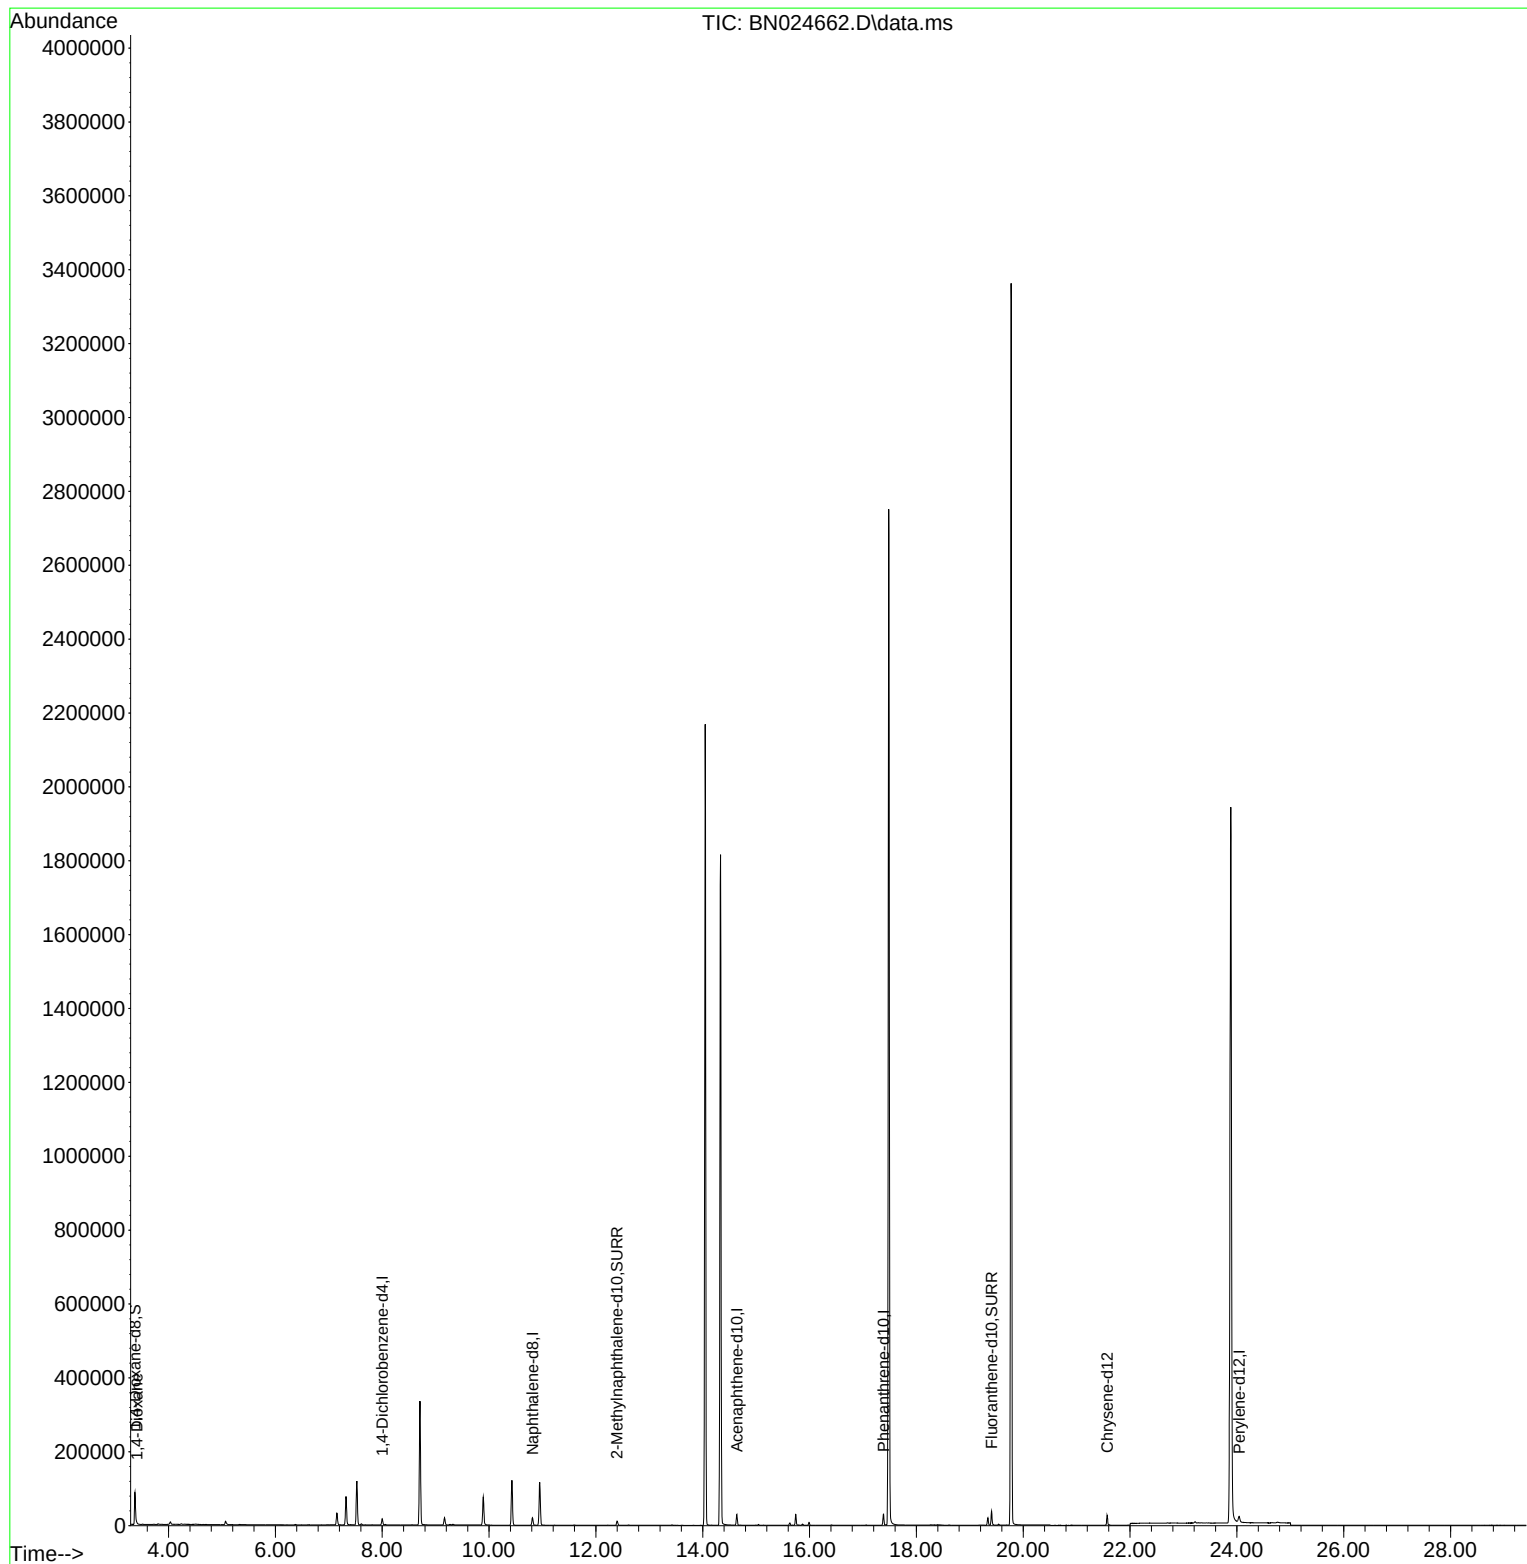

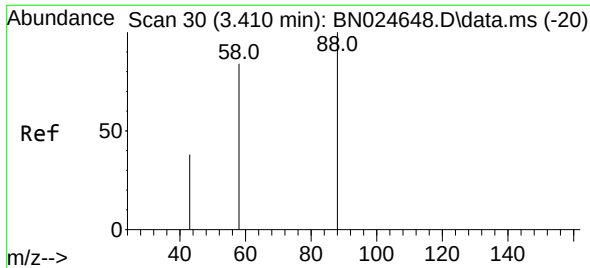

#2
 1,4-Dioxane
 Concen: 0.064 ng/ul
 RT: 3.405 min Scan# 29
 Delta R.T. -0.004 min
 Lab File: BN024662.D
 Acq: 31 Mar 2023 02:50

Instrument :
 BNA_N
 ClientSampleId :
 BFZ85

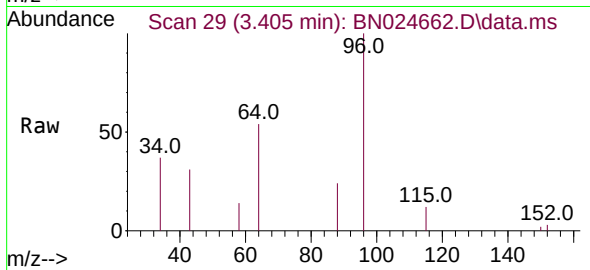

Tgt Ion: 88 Resp: 597

Ion	Ratio	Lower	Upper
88	100		
43	127.2	37.2	55.8#
58	56.0	61.5	92.3#

