

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024667.D
 Acq On : 31 Mar 2023 06:27
 Operator : CG/JU
 Sample : 02042-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB954

Quant Time: Mar 31 07:05:49 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 31 02:10:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	11554	0.400	ng/u1	0.00
4) Naphthalene-d8	10.812	136	36021	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.638	164	36038	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.384	188	45586	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.571	240	32792	0.400	ng/u1	# 0.00
23) Perylene-d12	24.062	264	26932	0.400	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	67553	5.696	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.396	152	23074	0.519	ng/u1	0.00
18) Fluoranthene-d10	19.408	212	51331	0.640	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.405	88	36165	2.898	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024667.D
Acq On : 31 Mar 2023 06:27
Operator : CG/JU
Sample : 02042-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB954


Quant Time: Mar 31 07:05:49 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 02:10:21 2023
Response via : Initial Calibration

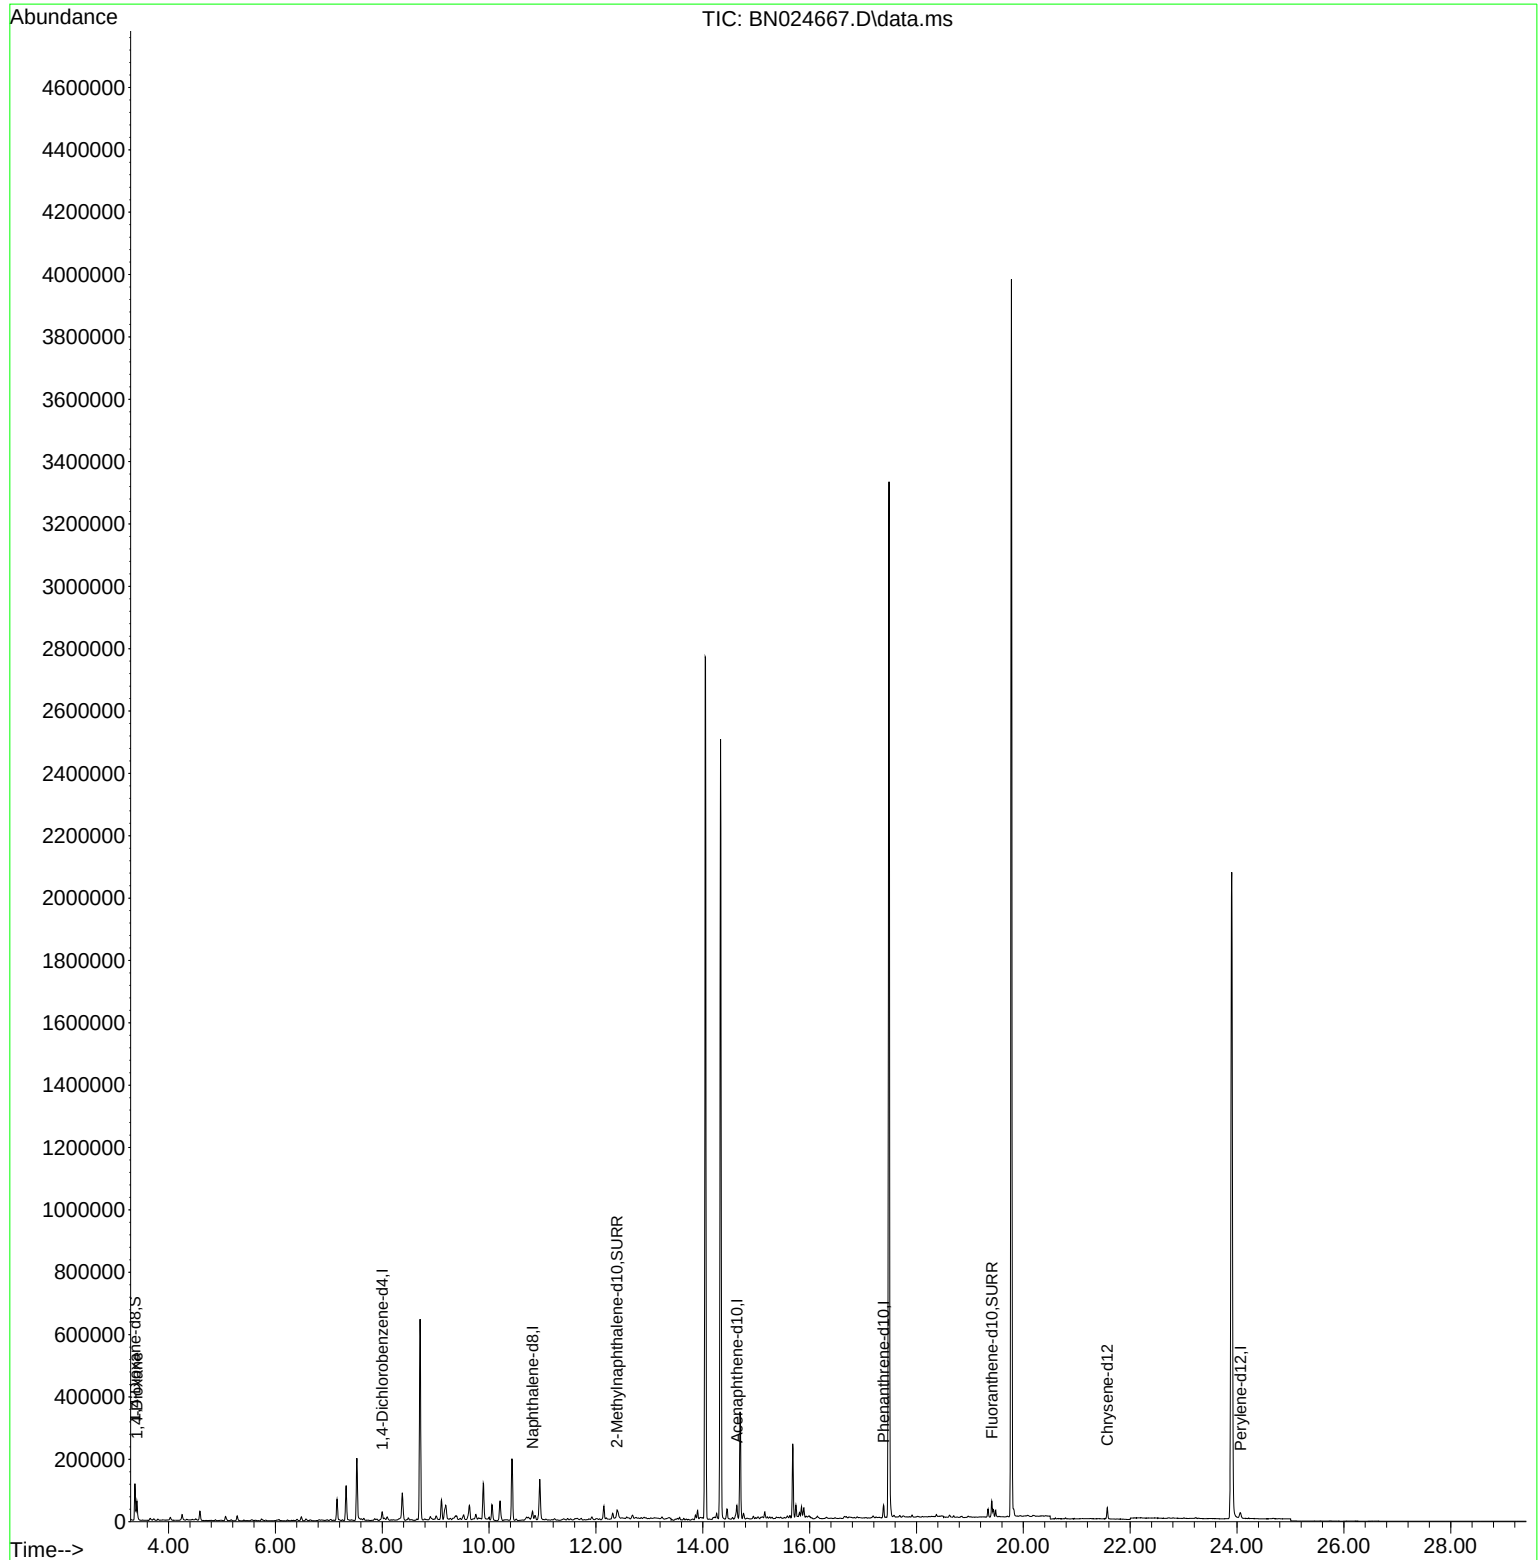

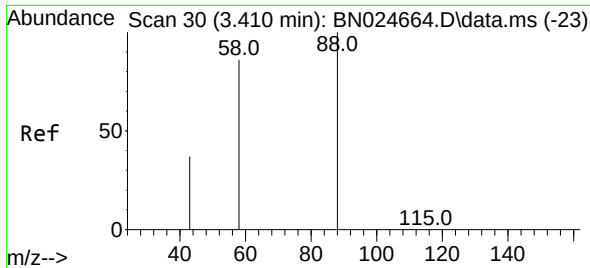

#2
 1,4-Dioxane
 Concen: 2.898 ng/ul
 RT: 3.405 min Scan# 29
 Delta R.T. -0.004 min
 Lab File: BN024667.D
 Acq: 31 Mar 2023 06:27

Instrument :
 BNA_N
 ClientSampleId :
 CB954

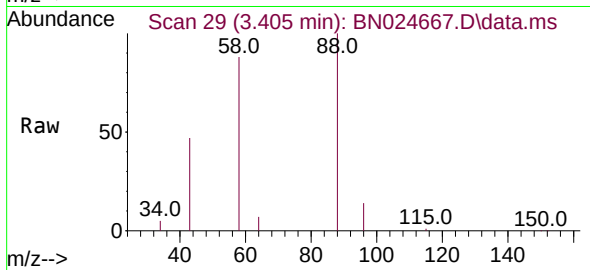

Tgt Ion: 88	Resp: 36165
Ion Ratio	Lower Upper
88	100
43	47.3 37.2 55.8
58	88.0 61.5 92.3

