

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024688.D
 Acq On : 31 Mar 2023 20:31
 Operator : CG/JU
 Sample : 02010-02
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB945

Quant Time: Apr 01 01:03:09 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.000	152	9020	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	27662	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	16550	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.384	188	34569	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	26262	0.400	ng/ul	0.00
23) Perylene-d12	24.056	264	24579	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	41815	4.516	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	12068	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	30155	0.469	ng/ul	0.00
Target Compounds						
11) Acenaphthene	14.698	153	1055	0.021	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024688.D
Acq On : 31 Mar 2023 20:31
Operator : CG/JU
Sample : 02010-02
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB945

Quant Time: Apr 01 01:03:09 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 01:00:20 2023
Response via : Initial Calibration

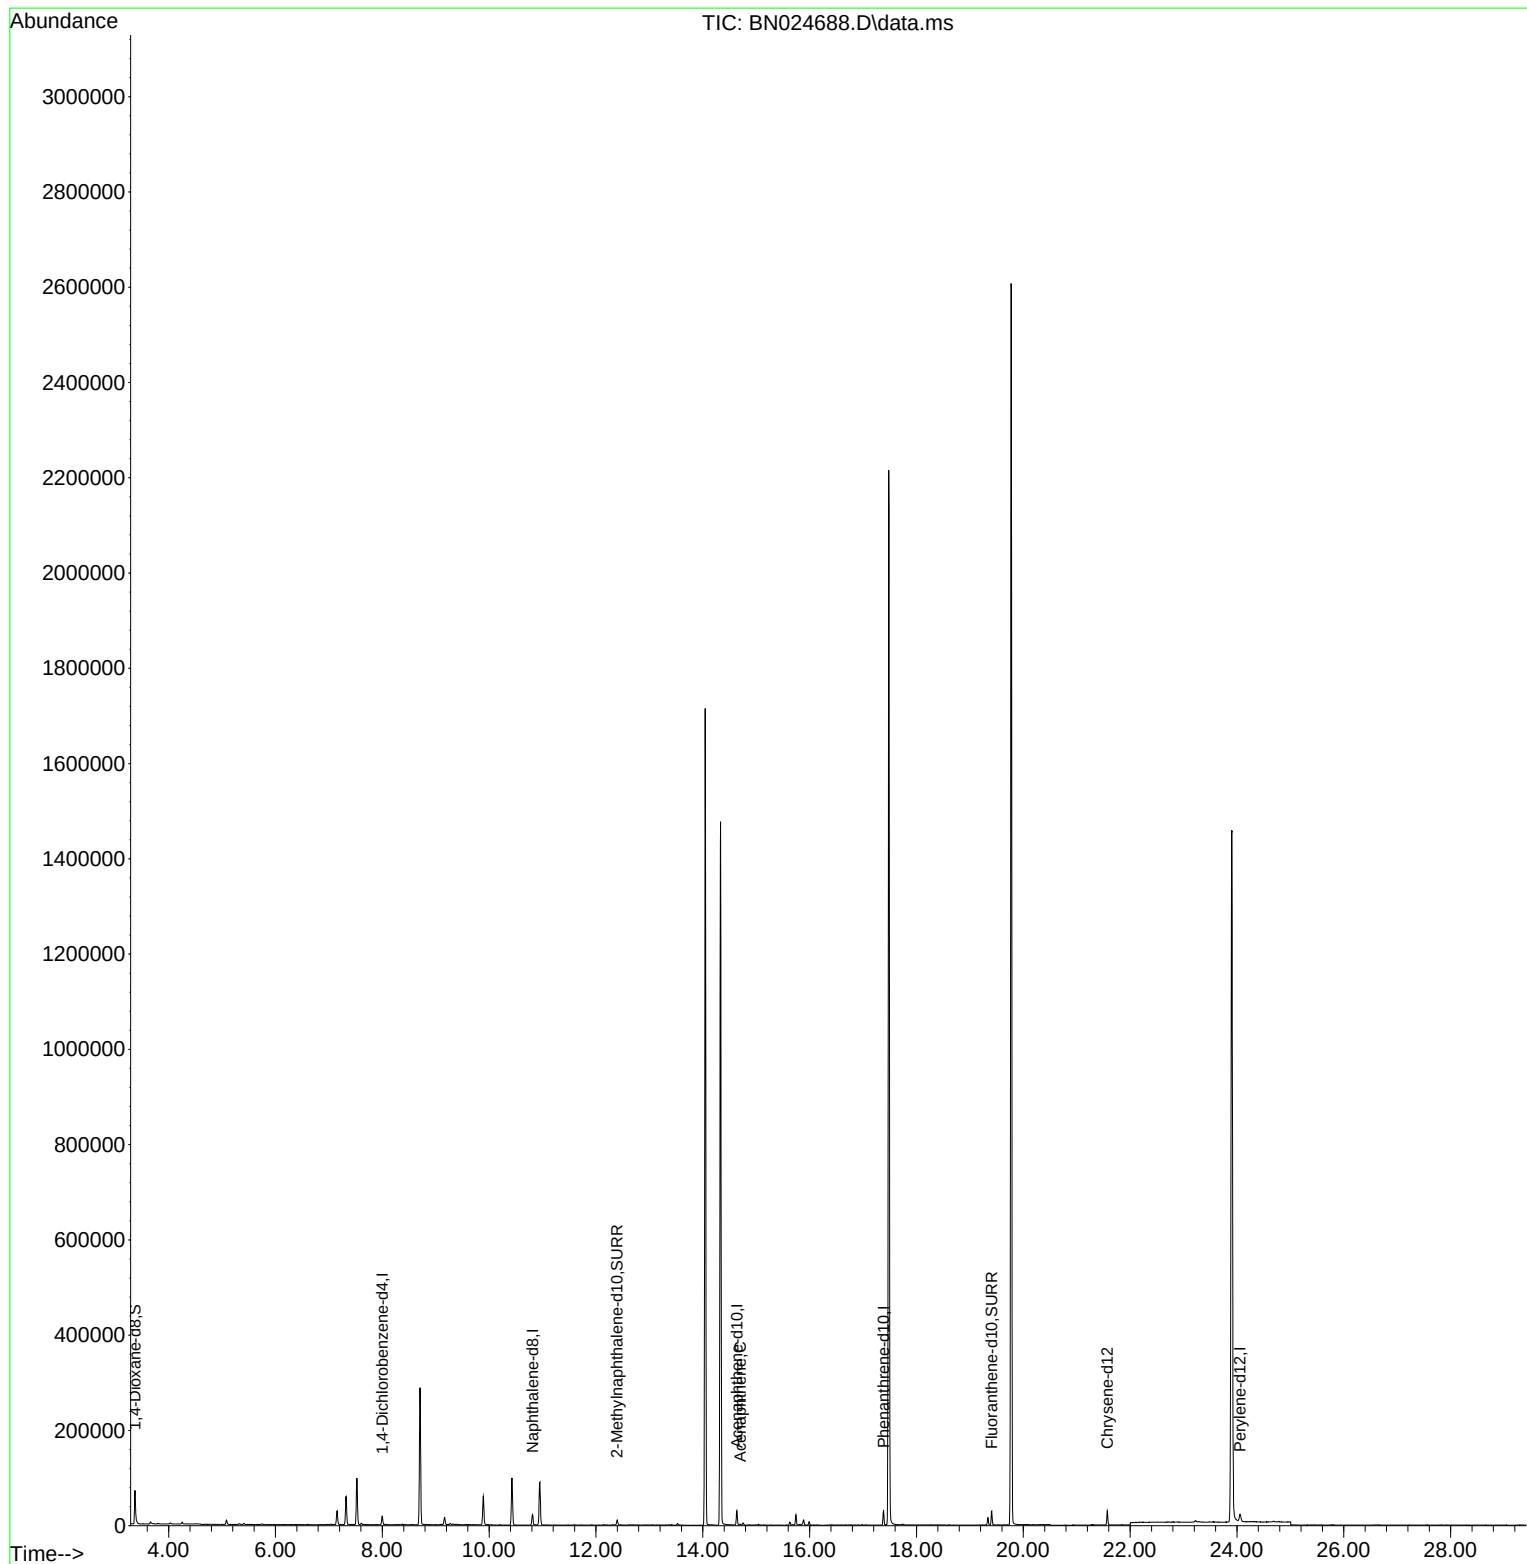

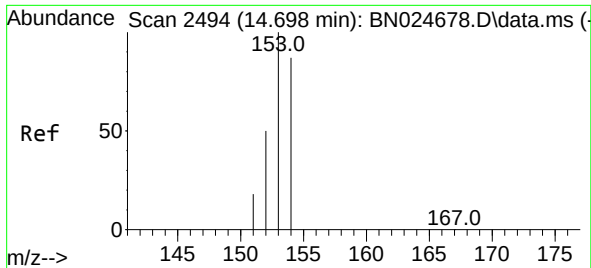

#11
 Acenaphthene
 Concen: 0.021 ng/ul
 RT: 14.698 min Scan# 2494
 Delta R.T. -0.000 min
 Lab File: BN024688.D
 Acq: 31 Mar 2023 20:31

Instrument :
 BNA_N
 ClientSampleId :
 CB945

Tgt Ion	Ratio	Lower	Upper
153	100		
152	55.7	40.3	60.5
154	89.8	71.0	106.4

