

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024691.D
 Acq On : 31 Mar 2023 22:21
 Operator : CG/JU
 Sample : 02067-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ69

Quant Time: Apr 01 01:03:30 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 01:00:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	9233	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	28442	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	17166	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	35342	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	26805	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	26926	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	50853	5.366	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	16128	0.460	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	39059	0.595	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.410	88	4059	0.407	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024691.D
Acq On : 31 Mar 2023 22:21
Operator : CG/JU
Sample : 02067-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ69


Quant Time: Apr 01 01:03:30 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 01:00:20 2023
Response via : Initial Calibration

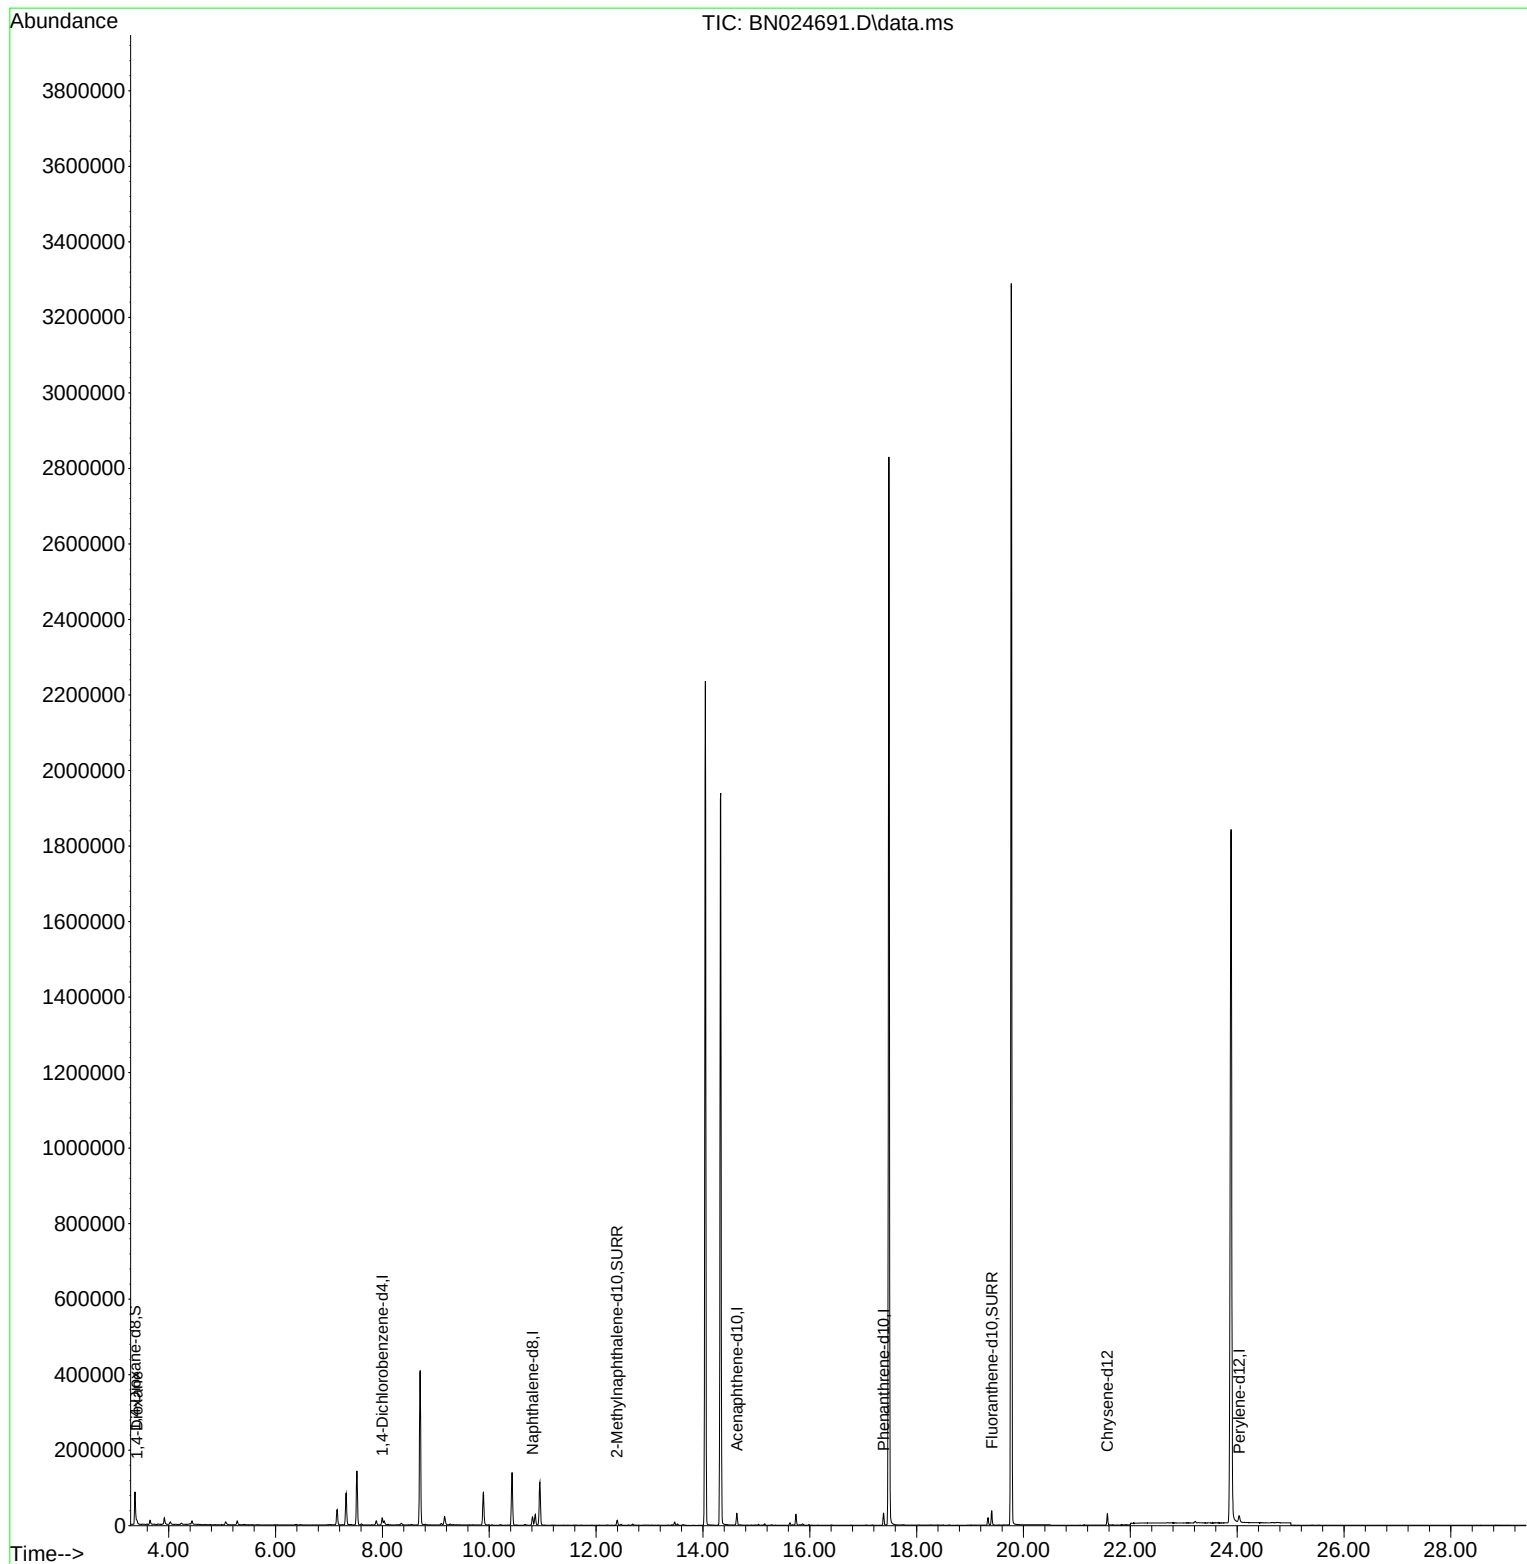

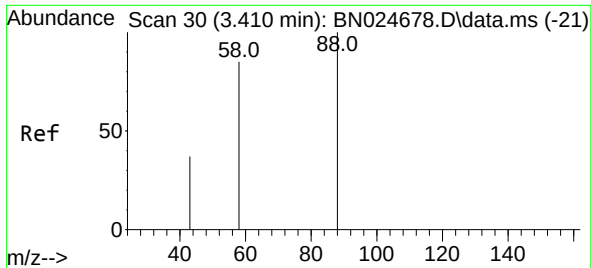

#2
 1,4-Dioxane
 Concen: 0.407 ng/ul
 RT: 3.410 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN024691.D
 Acq: 31 Mar 2023 22:21

Instrument :
 BNA_N
 ClientSampleId :
 BFZ69

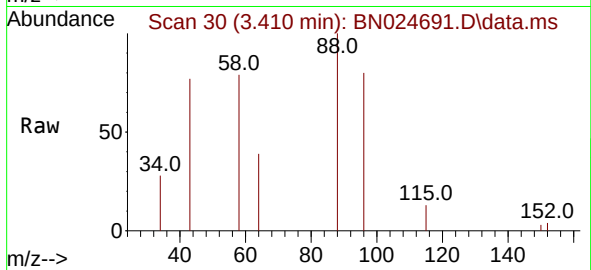

Tgt Ion: 88 Resp: 4059

Ion	Ratio	Lower	Upper
88	100		
43	77.3	37.2	55.8#
58	79.1	61.5	92.3

