

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024700.D
 Acq On : 01 Apr 2023 04:27
 Operator : CG/JU
 Sample : 02067-13
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ71

Quant Time: Apr 01 05:26:14 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	9062	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	27695	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.634	164	16234	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.380	188	33859	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	25390	0.400	ng/ul	0.00
23) Perylene-d12	24.038	264	24096	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	44564	4.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	12205	0.357	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	32960	0.530	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	3710	0.379	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024700.D
Acq On : 01 Apr 2023 04:27
Operator : CG/JU
Sample : 02067-13
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ71

Quant Time: Apr 01 05:26:14 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration

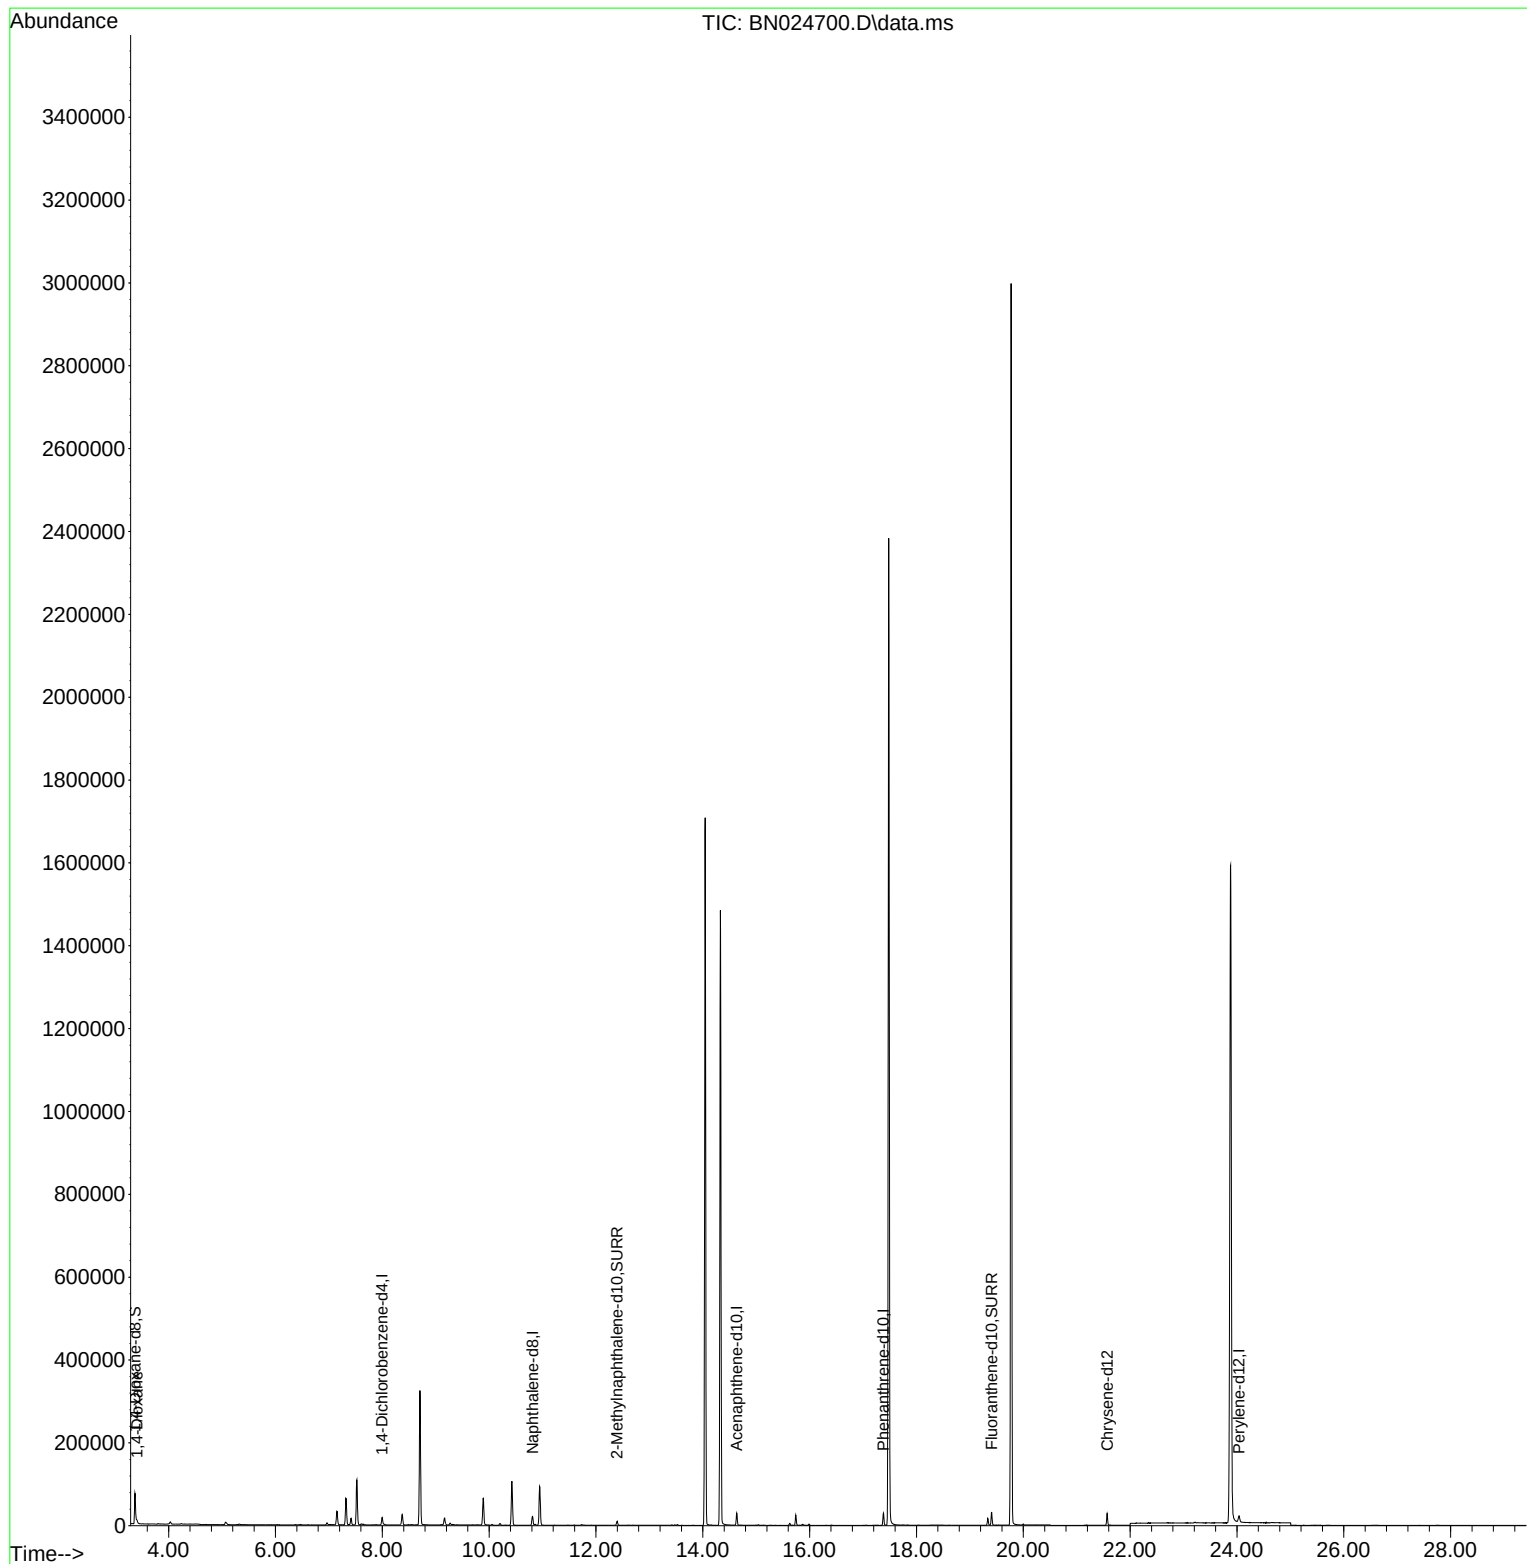

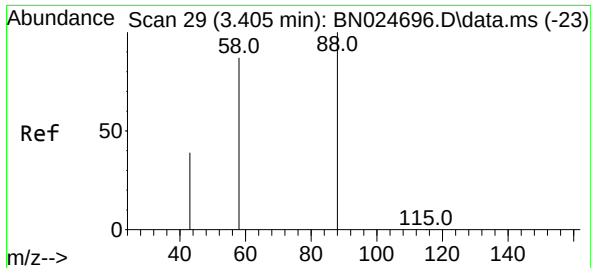

#2
 1,4-Dioxane
 Concen: 0.379 ng/ul
 RT: 3.406 min Scan# 29
 Delta R.T. 0.000 min
 Lab File: BN024700.D
 Acq: 01 Apr 2023 04:27

Instrument :
 BNA_N
 ClientSampleId :
 BFZ71

Tgt Ion:	88	Resp:	3710
Ion	Ratio	Lower	Upper
88	100		
43	47.6	37.2	55.8
58	59.2	61.5	92.3

