

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024701.D
 Acq On : 01 Apr 2023 05:04
 Operator : CG/JU
 Sample : 02067-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ72

Quant Time: Apr 01 05:36:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	8567	0.400	ng/ul	0.00
4) Naphthalene-d8	10.811	136	26374	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.638	164	15562	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.383	188	32442	0.400	ng/ul	0.00
17) Chrysene-d12	21.568	240	24775	0.400	ng/ul	0.00
23) Perylene-d12	24.047	264	22995	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.367	96	45275	5.149	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	13072	0.402	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	32919	0.543	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	4249	0.459	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024701.D
Acq On : 01 Apr 2023 05:04
Operator : CG/JU
Sample : 02067-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ72

Quant Time: Apr 01 05:36:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration

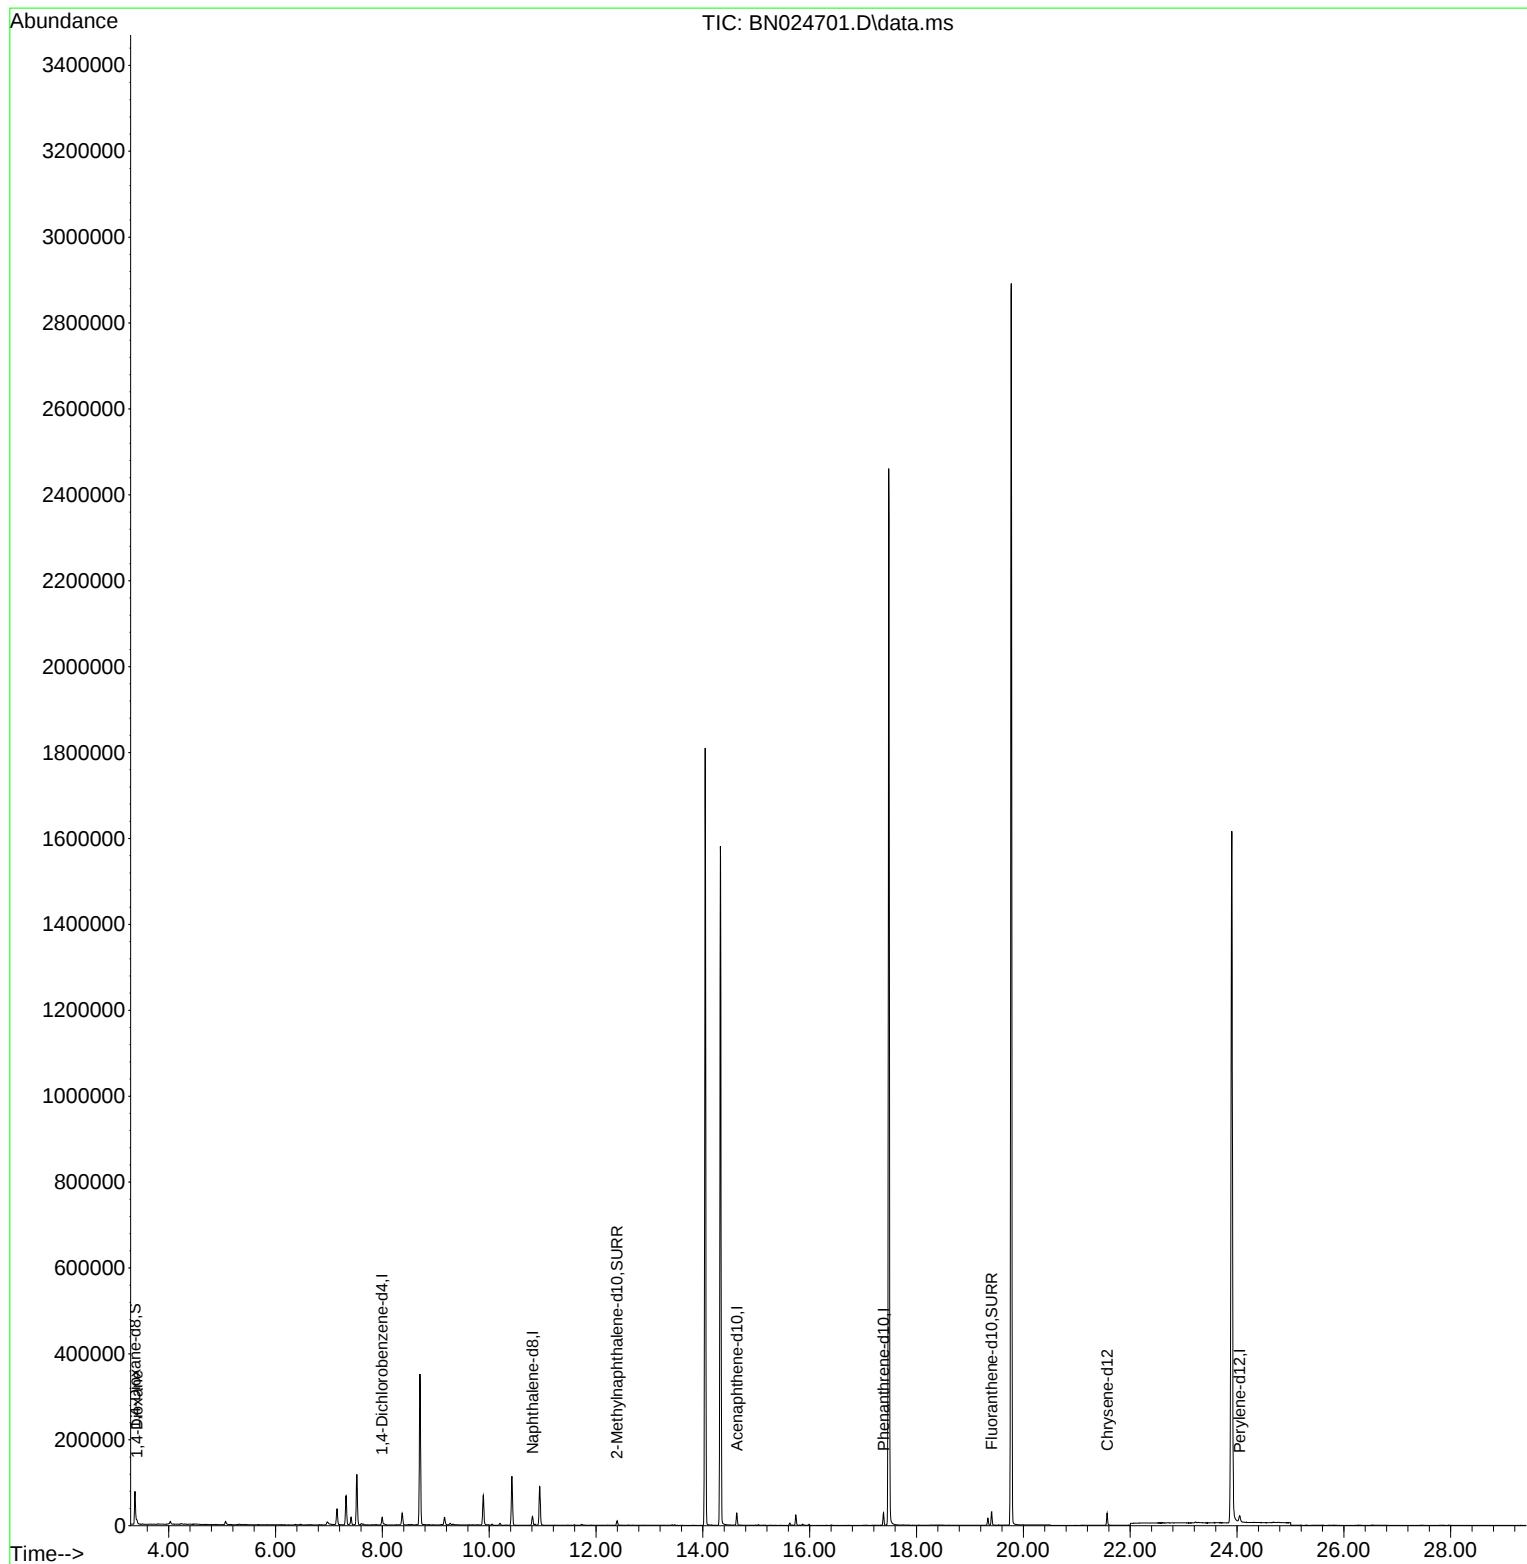

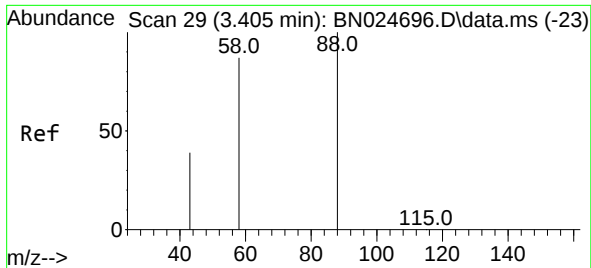

#2
 1,4-Dioxane
 Concen: 0.459 ng/ul
 RT: 3.405 min Scan# 24
 Delta R.T. -0.000 min
 Lab File: BN024701.D
 Acq: 01 Apr 2023 05:04

Instrument :
 BNA_N
 ClientSampleId :
 BFZ72

Tgt Ion: 88 Resp: 4249
 Ion Ratio Lower Upper
 88 100
 43 61.5 37.2 55.8#
 58 80.9 61.5 92.3

