

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024702.D
 Acq On : 01 Apr 2023 05:40
 Operator : CG/JU
 Sample : 02067-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ87

Quant Time: Apr 01 06:09:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8974	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	27687	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.633	164	16143	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	34168	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	24733	0.400	ng/ul	0.00
23) Perylene-d12	24.044	264	22971	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	44571	4.839	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13978	0.409	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	32842	0.543	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	1418	0.146	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024702.D
Acq On : 01 Apr 2023 05:40
Operator : CG/JU
Sample : 02067-15
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ87

Quant Time: Apr 01 06:09:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration

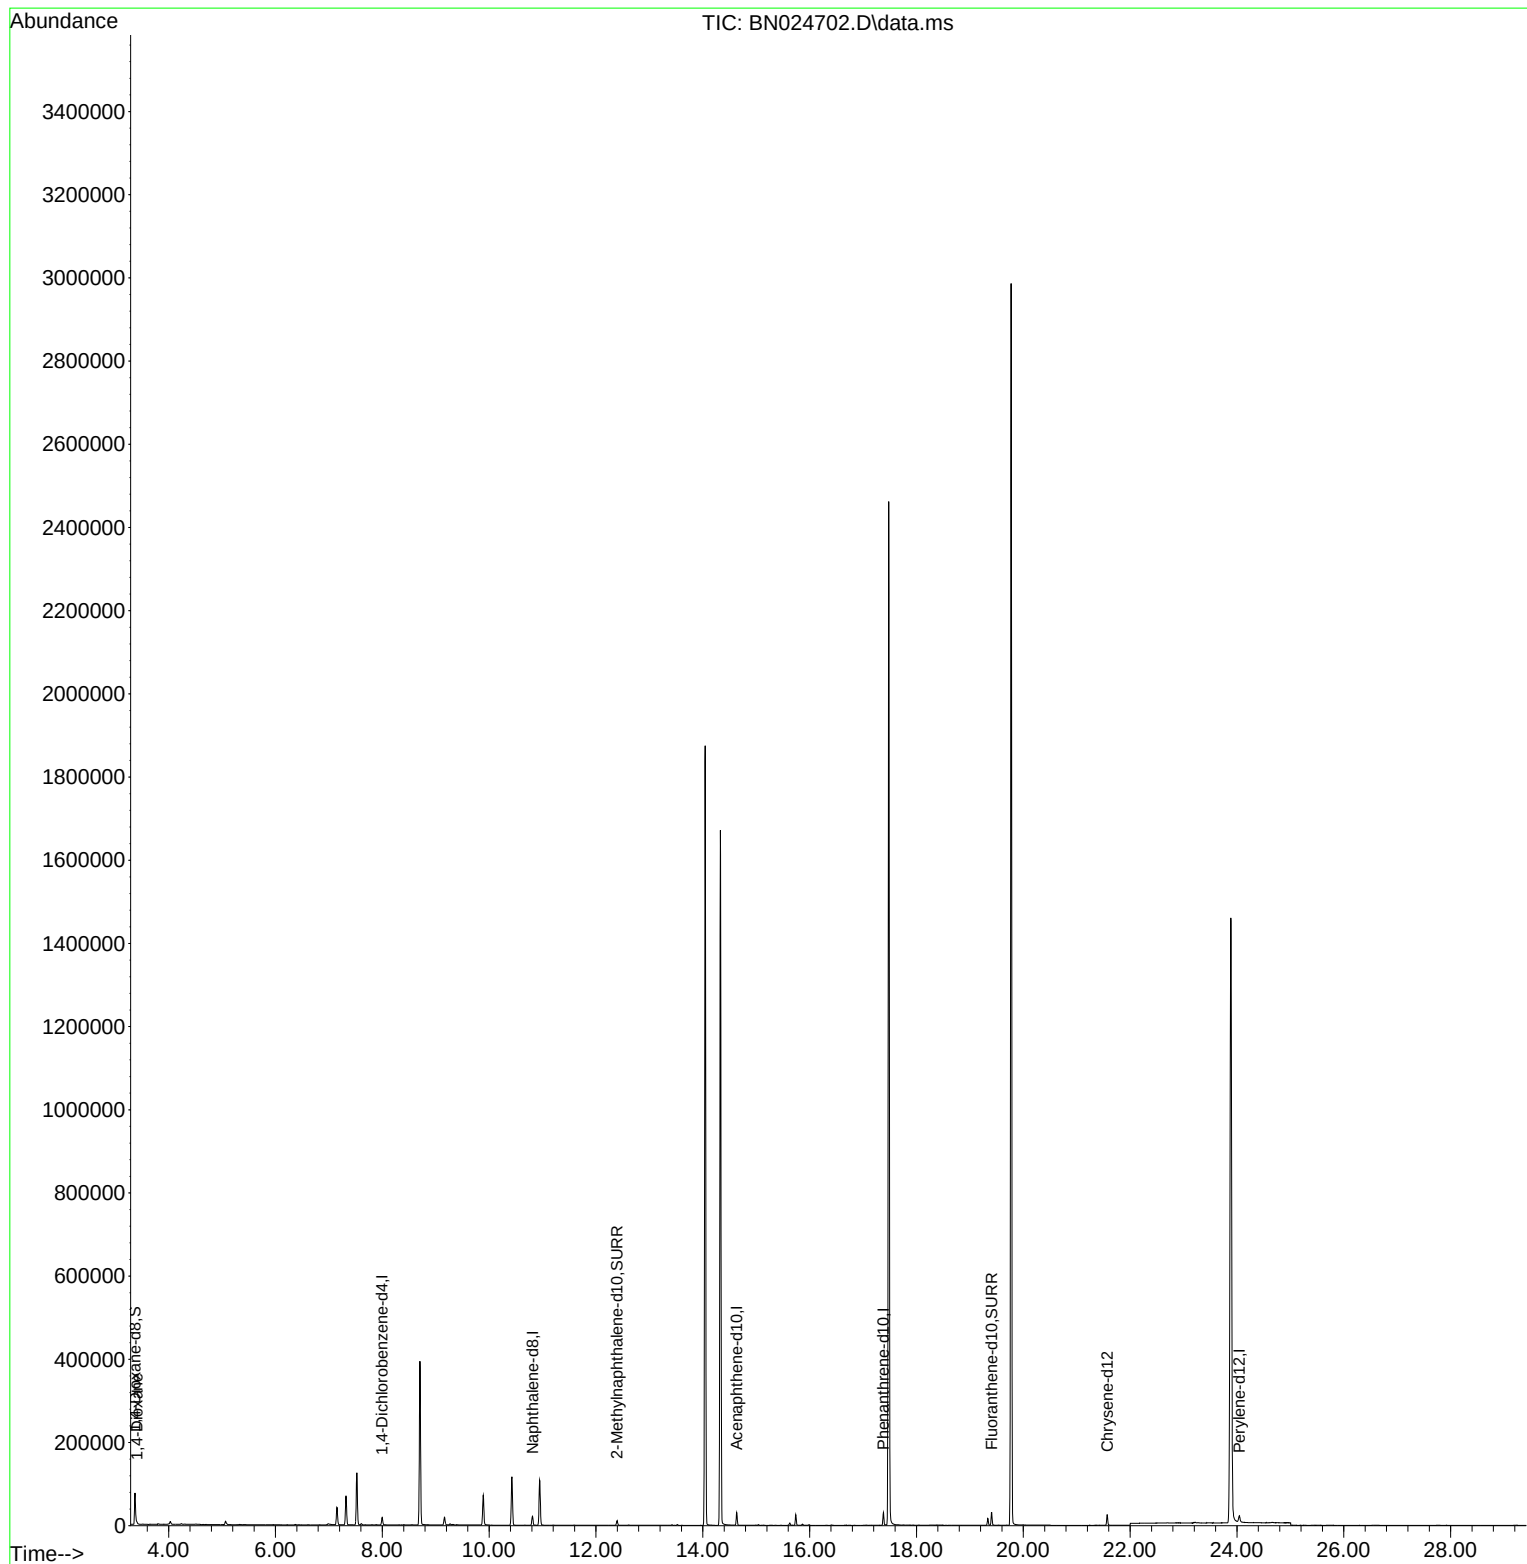

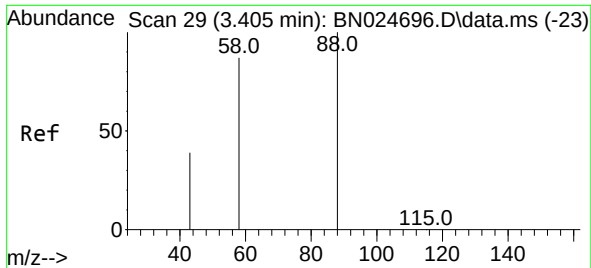

#2
 1,4-Dioxane
 Concen: 0.146 ng/ul
 RT: 3.405 min Scan# 29
 Delta R.T. 0.000 min
 Lab File: BN024702.D
 Acq: 01 Apr 2023 05:40

Instrument :
 BNA_N
 ClientSampleId :
 BFZ87

Tgt Ion: 88 Resp: 1418

Ion	Ratio	Lower	Upper
88	100		
43	82.2	37.2	55.8#
58	71.4	61.5	92.3

