

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024703.D
 Acq On : 01 Apr 2023 06:17
 Operator : CG/JU
 Sample : 02067-16
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ88

Quant Time: Apr 01 06:46:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8193	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	25293	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.633	164	14817	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.379	188	32341	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	24422	0.400	ng/ul	0.00
23) Perylene-d12	24.041	264	22463	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	39128	4.653	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	12194	0.391	ng/ul	0.00
18) Fluoranthene-d10	19.408	212	34078	0.570	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	6019	0.680	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024703.D
Acq On : 01 Apr 2023 06:17
Operator : CG/JU
Sample : 02067-16
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ88


Quant Time: Apr 01 06:46:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration

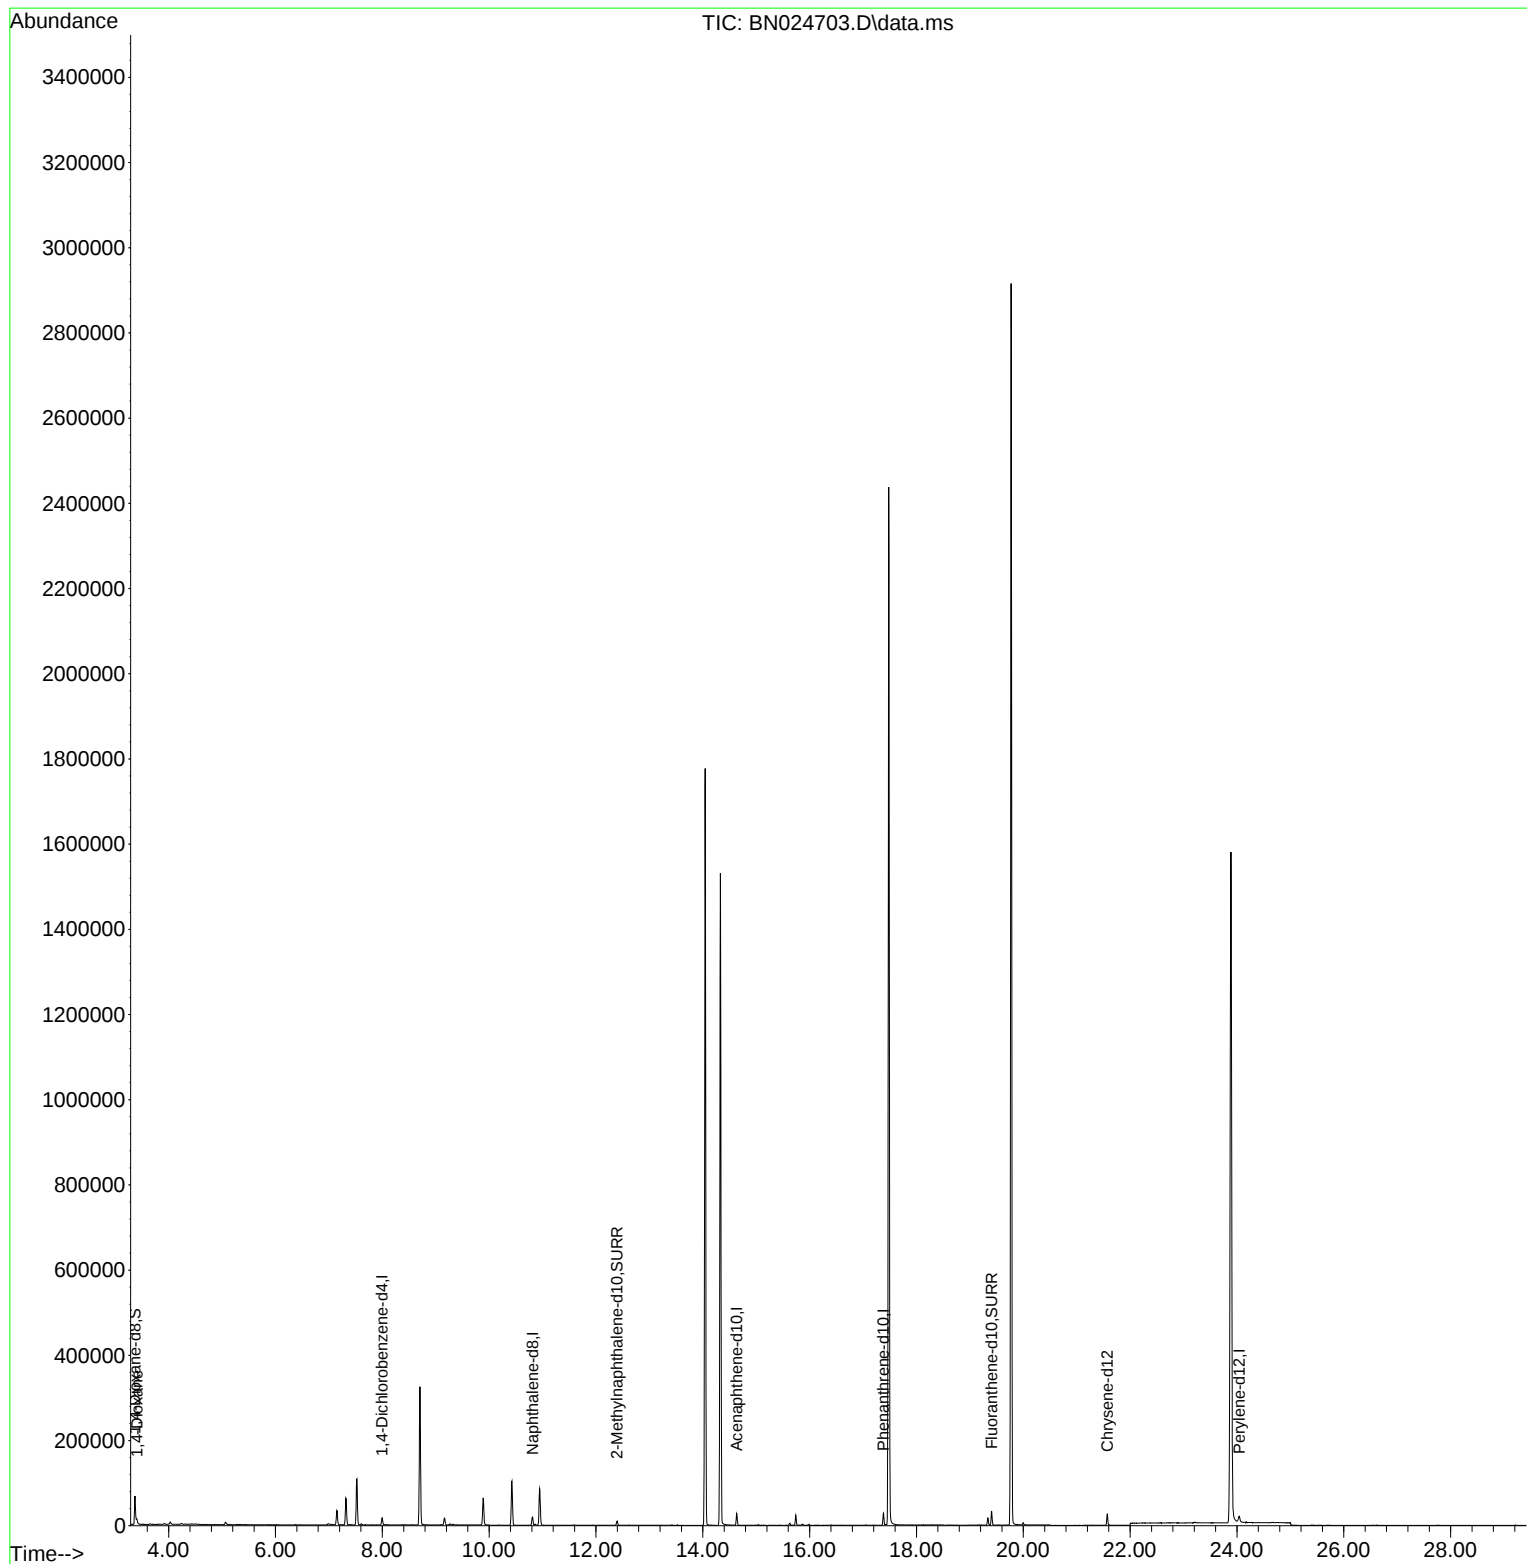

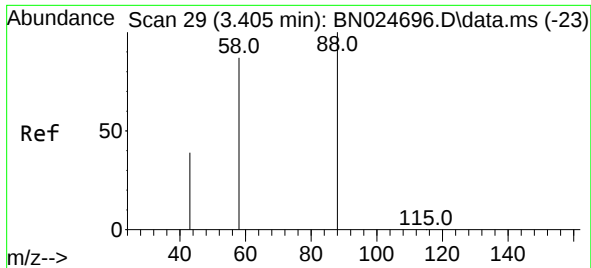

#2
 1,4-Dioxane
 Concen: 0.680 ng/ul
 RT: 3.405 min Scan# 29
 Delta R.T. 0.000 min
 Lab File: BN024703.D
 Acq: 01 Apr 2023 06:17

Instrument :
 BNA_N
 ClientSampleId :
 BFZ88

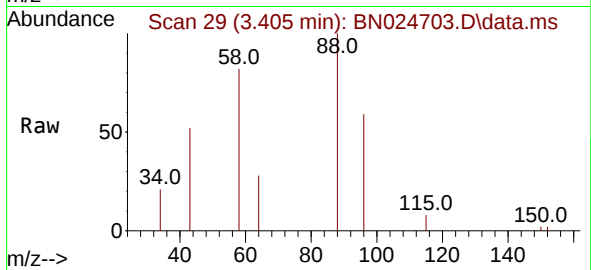

Tgt Ion: 88	Resp: 6019
Ion Ratio	Lower Upper
88 100	
43 52.1	37.2 55.8
58 81.7	61.5 92.3

