

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
 Data File : BN024718.D
 Acq On : 01 Apr 2023 16:03
 Operator : CG/JU
 Sample : 02086-05
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ75

Quant Time: Apr 03 01:37:47 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 01 04:05:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.996	152	8661	0.400	ng/u1	0.00
4) Naphthalene-d8	10.806	136	26656	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.633	164	15467	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.379	188	32459	0.400	ng/u1	0.00
17) Chrysene-d12	21.568	240	25794	0.400	ng/u1	0.00
23) Perylene-d12	24.038	264	23596	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	48491	5.455	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13091	0.398	ng/u1	0.00
18) Fluoranthene-d10	19.408	212	31995	0.507	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.405	88	17855	1.909	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033023\
Data File : BN024718.D
Acq On : 01 Apr 2023 16:03
Operator : CG/JU
Sample : 02086-05
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ75


Quant Time: Apr 03 01:37:47 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 01 04:05:52 2023
Response via : Initial Calibration

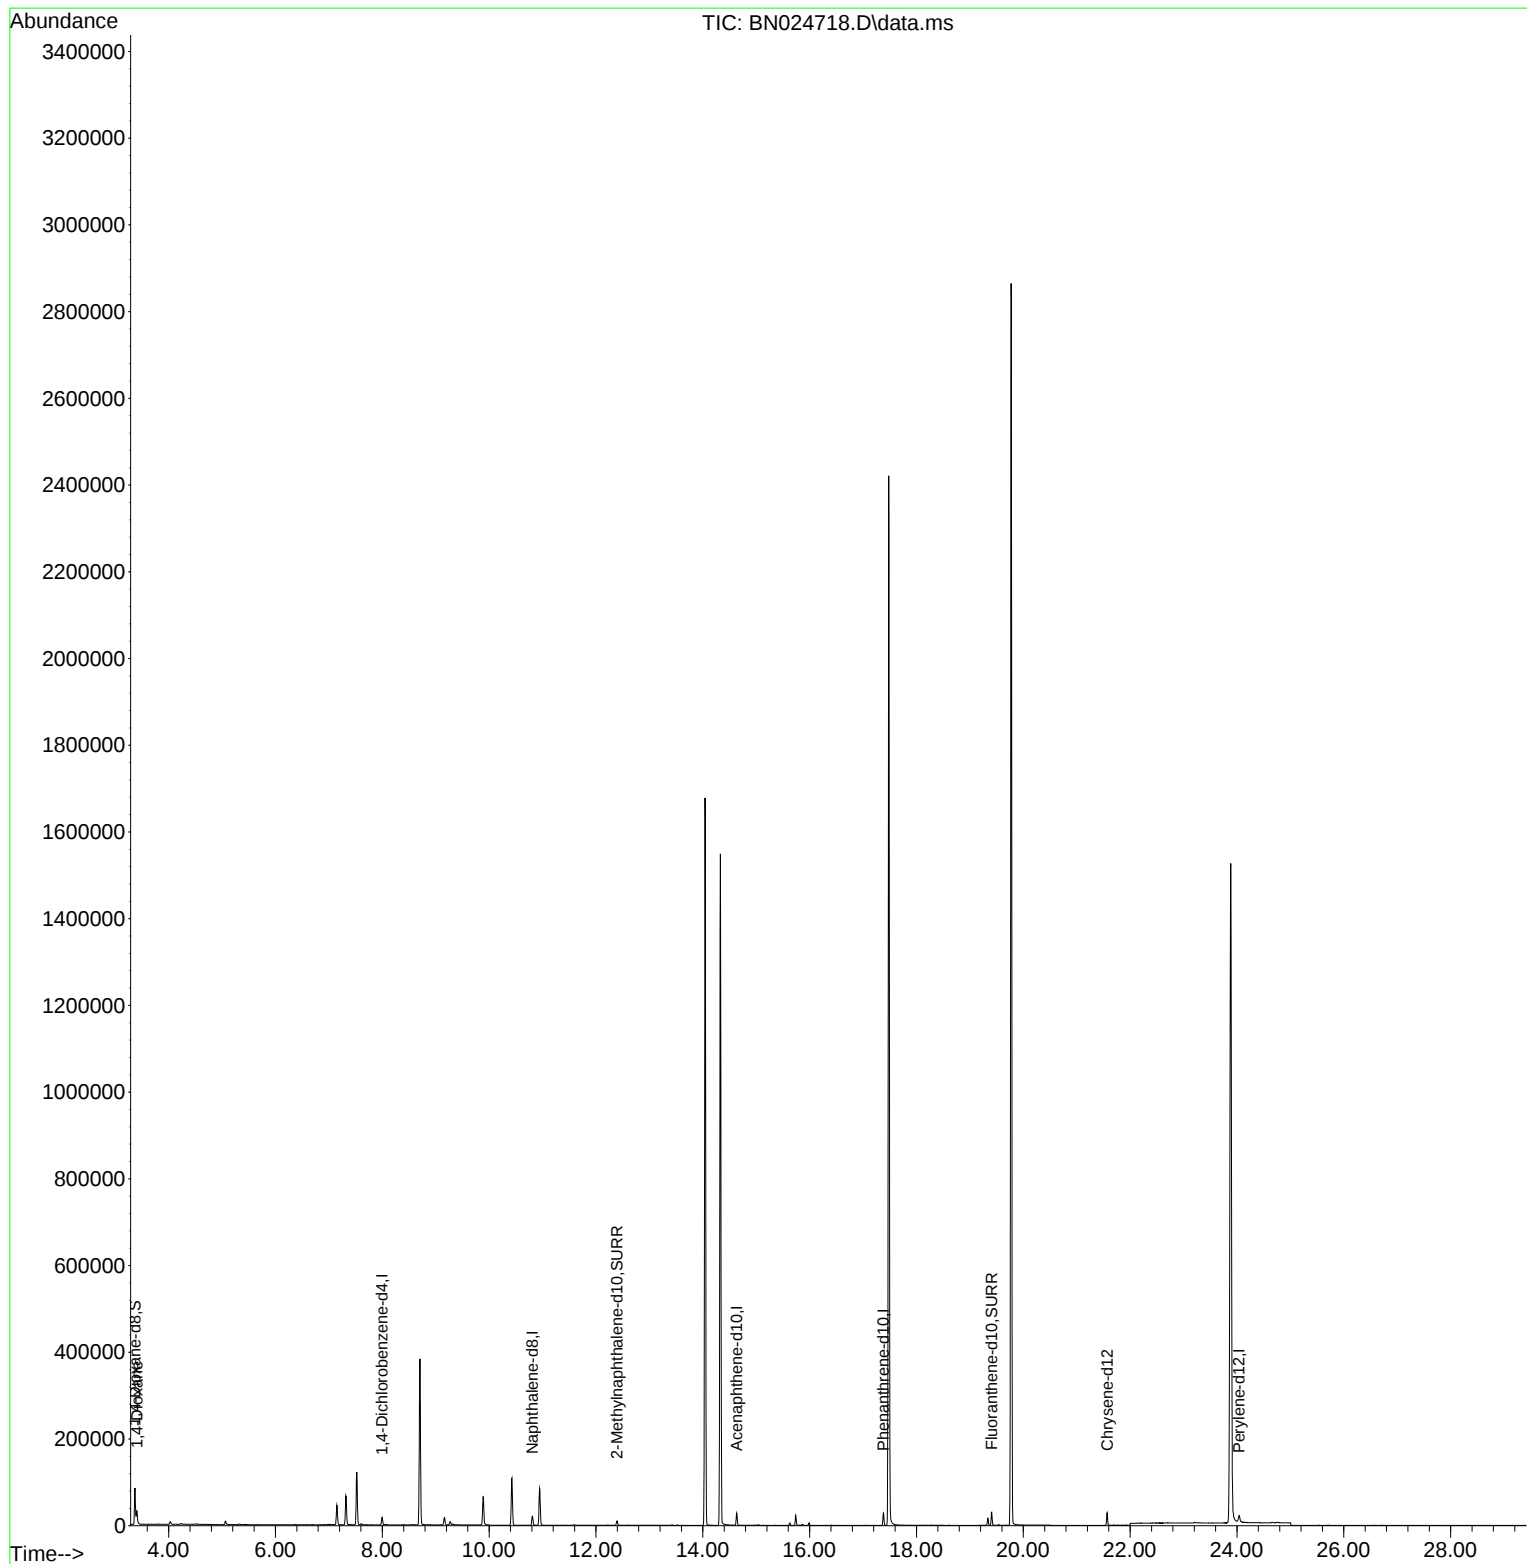

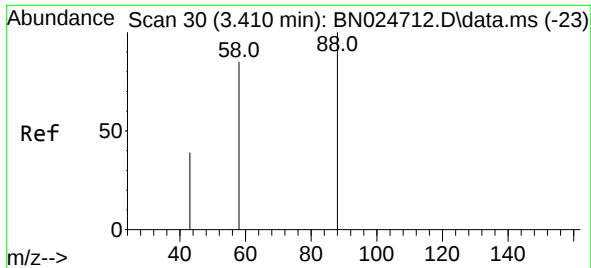

#2
 1,4-Dioxane
 Concen: 1.909 ng/ul
 RT: 3.405 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BN024718.D
 Acq: 01 Apr 2023 16:03

Instrument :
 BNA_N
 ClientSampleId :
 BFZ75

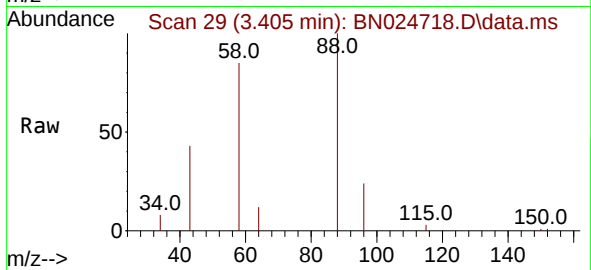

Tgt Ion:	88	Resp:	17855
Ion	Ratio	Lower	Upper
88	100		
43	42.8	37.2	55.8
58	84.7	61.5	92.3

