
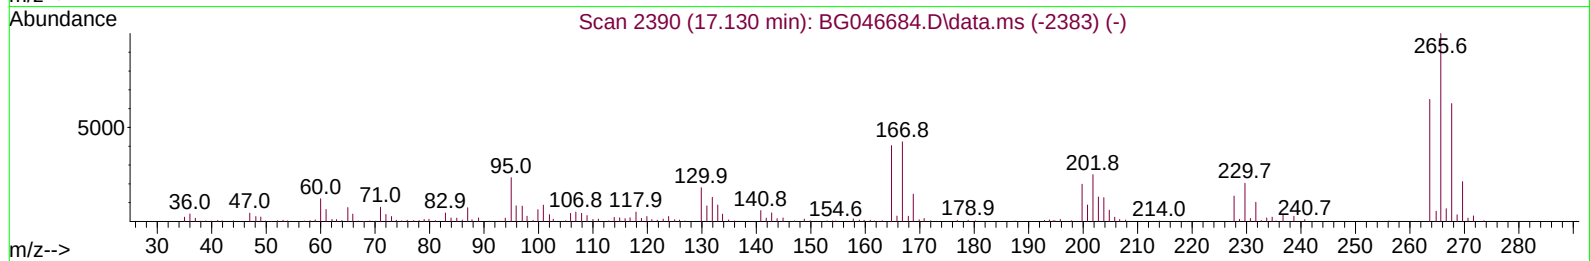
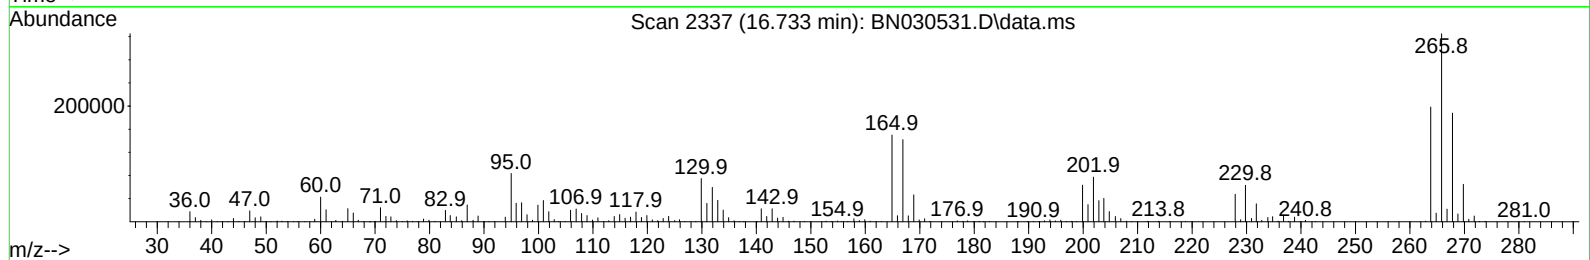


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033024\
Data File : BN030531.D
Acq On : 29 Mar 2024 15:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 00:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

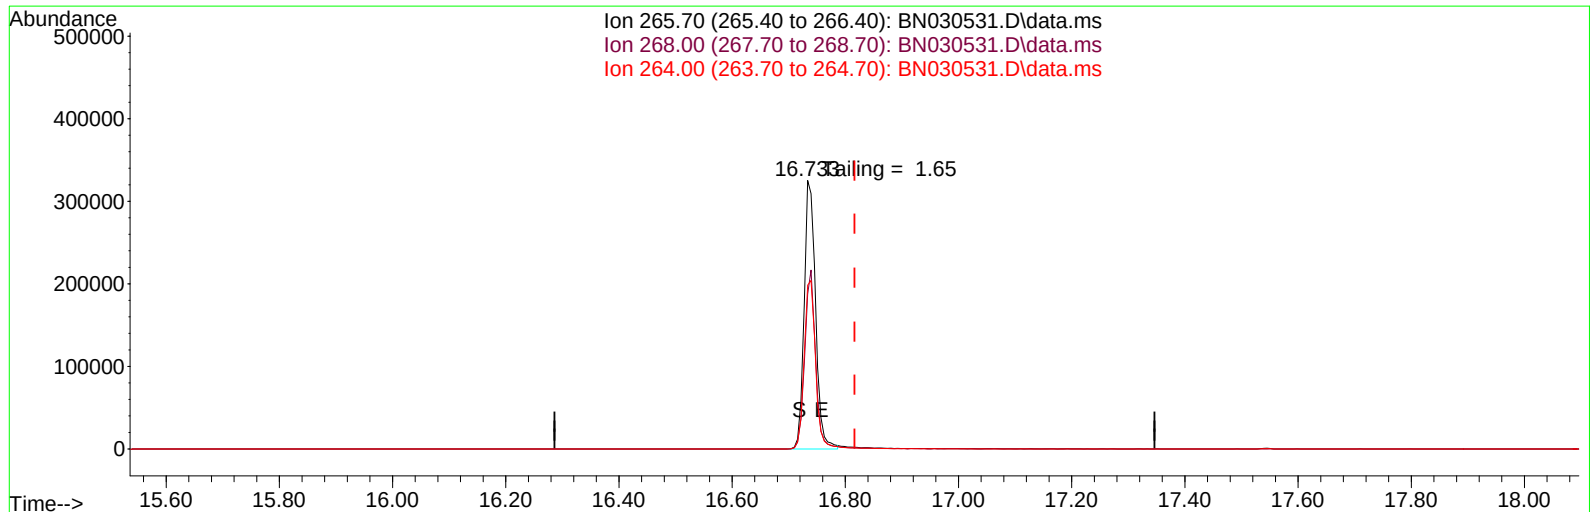

TIC: BN030531.D\data.ms

(70) Pentachlorophenol (C)




16.733min (-0.083) 25334.01 ng

response 464034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	61.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033024\
Data File : BN030531.D
Acq On : 29 Mar 2024 15:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 00:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

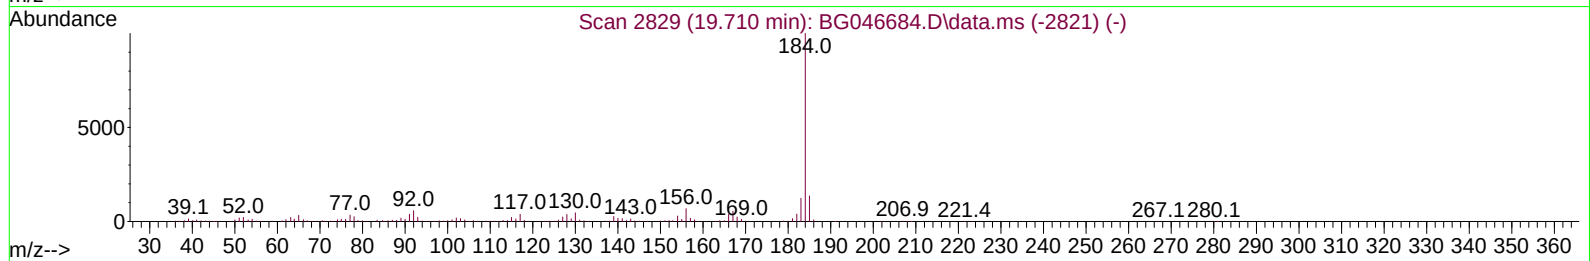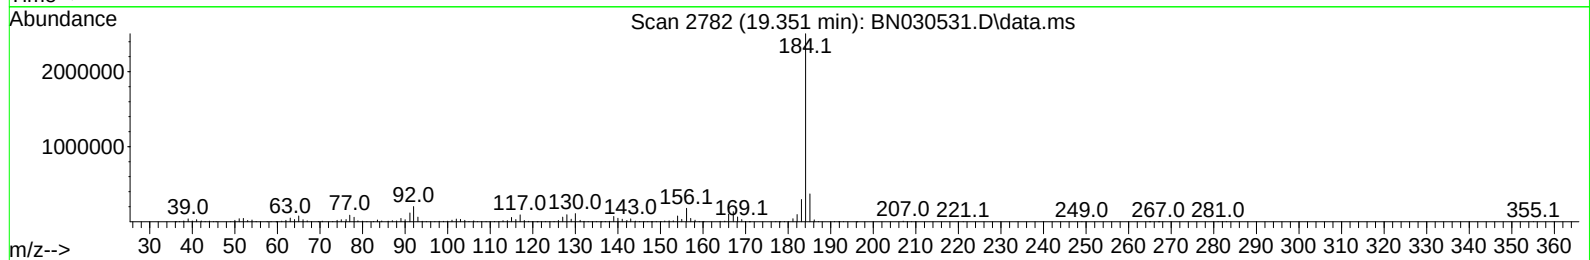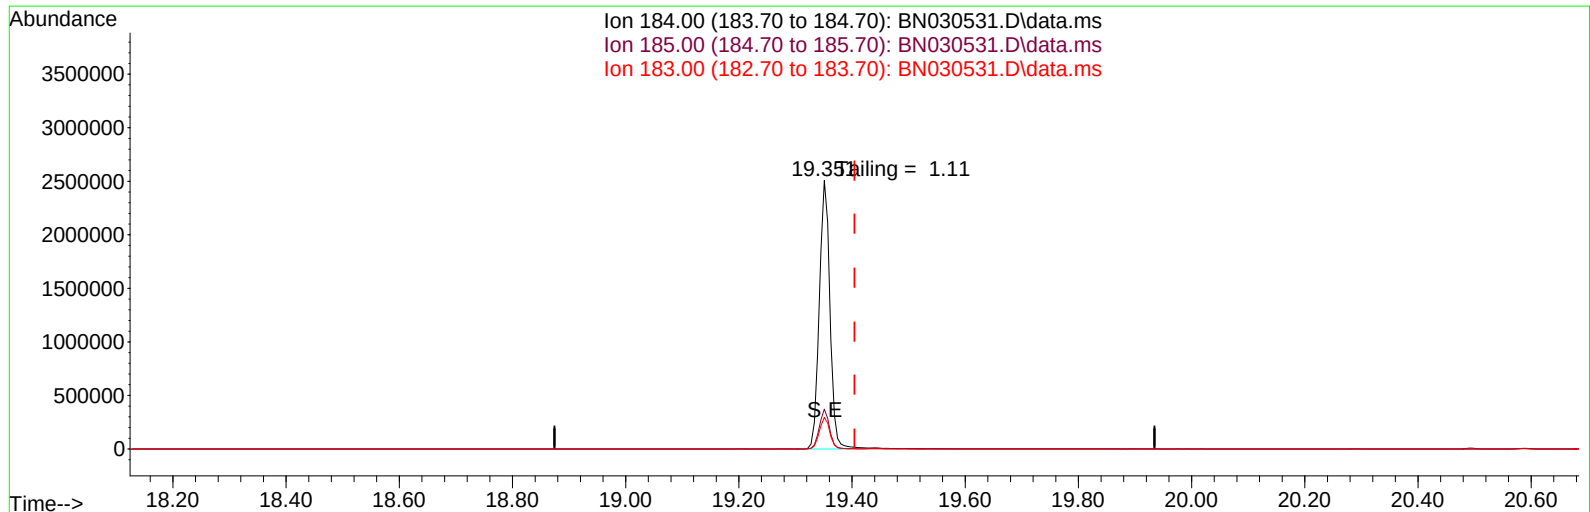

TIC: BN030531.D\data.ms

(77) Benzidine

19.351min (-0.053) 0.00 ng

response 3307936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	11.76
0.00	0.00	0.00