


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033024\
Data File : BN030531.D
Acq On : 29 Mar 2024 15:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN033024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 00:04:36 2024

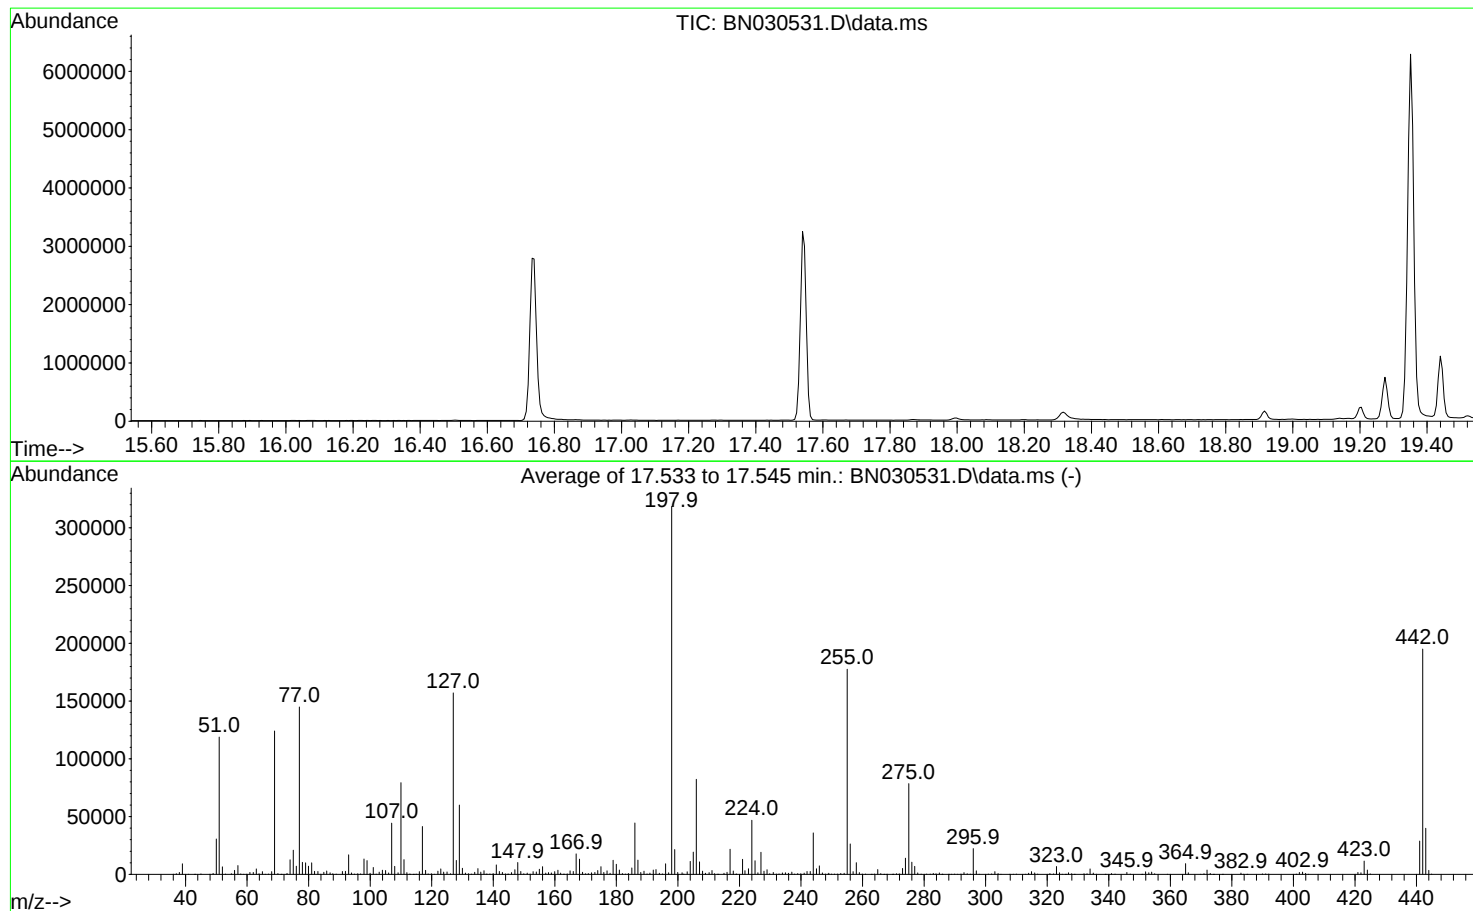




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	118825	PASS
68	69	0.00	2	1.9	2414	PASS
69	198	0.00	100	39.0	124052	PASS
70	69	0.00	2	0.6	734	PASS
127	198	10	80	49.3	157101	PASS
197	198	0.00	2	0.5	1436	PASS
198	198	100	100	100.0	318464	PASS
199	198	5	9	6.8	21530	PASS
275	198	10	60	24.7	78528	PASS
365	198	1	100	2.9	9300	PASS
441	198	0.01	100	9.1	28845	PASS
442	442	50	100	100.0	195069	PASS
443	442	15	24	20.4	39864	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033024\
Data File : BN030531.D
Acq On : 29 Mar 2024 15:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 30 00:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

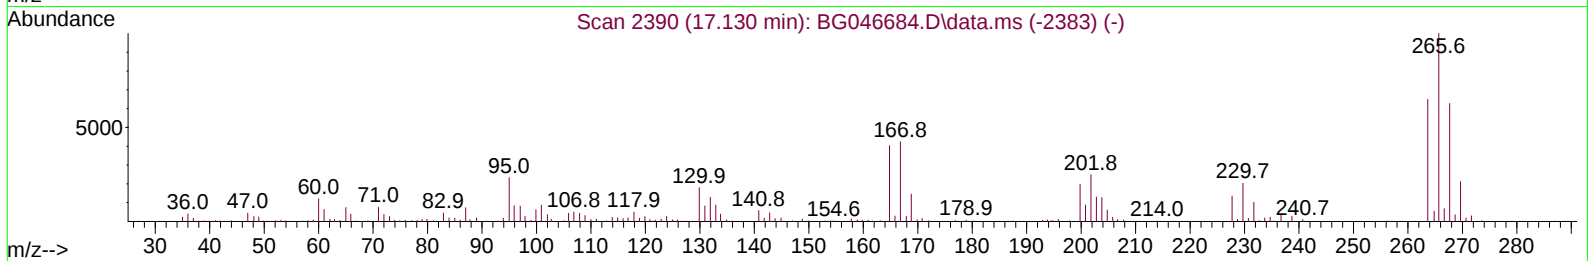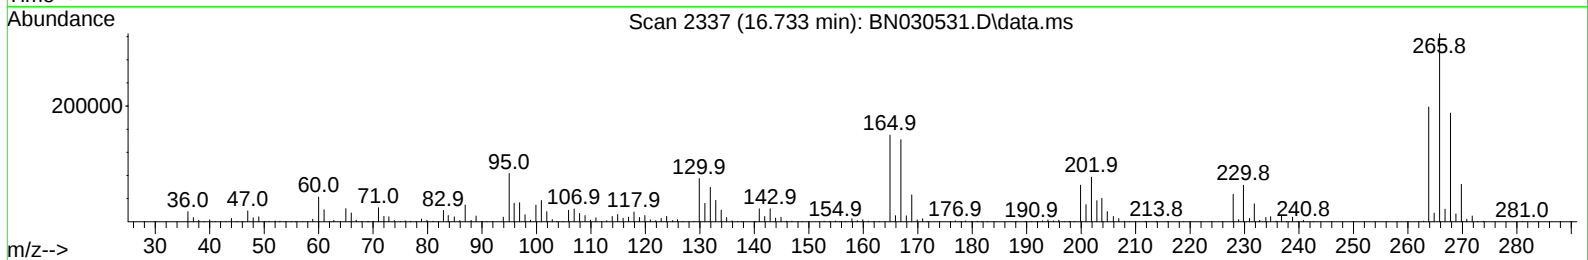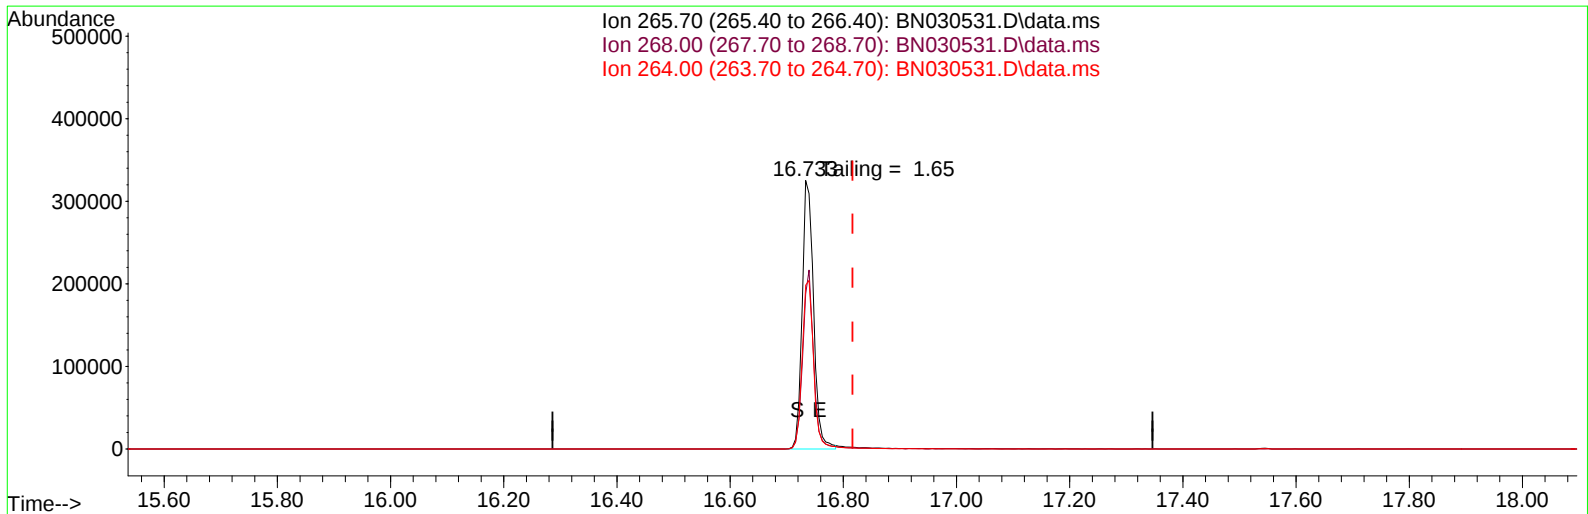

TIC: BN030531.D\data.ms

(70) Pentachlorophenol (C)

16.733min (-0.083) 25334.01 ng




response 464034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	61.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033024\
Data File : BN030531.D
Acq On : 29 Mar 2024 15:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 30 00:45:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 22 02:28:35 2024
Response via : Initial Calibration

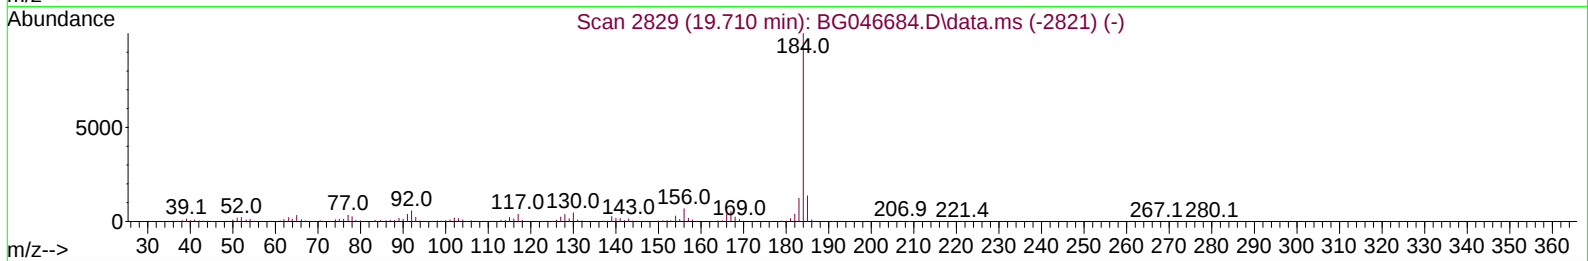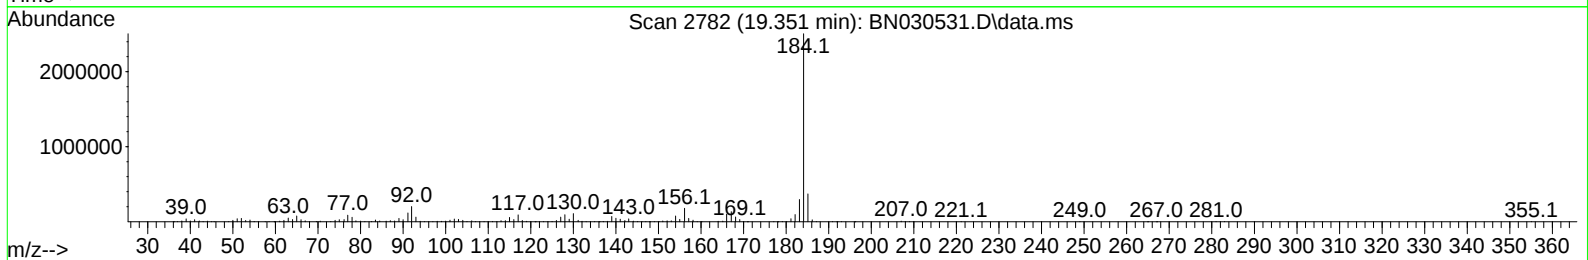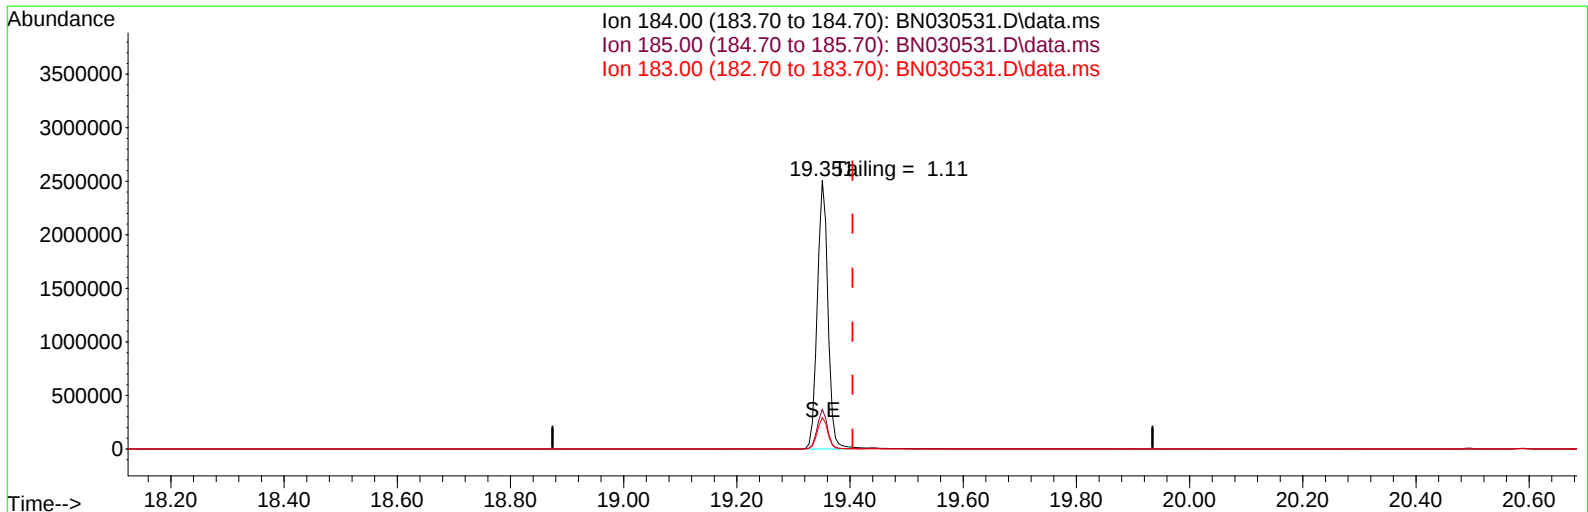

TIC: BN030531.D\data.ms

(77) Benzidine

19.351min (-0.053) 0.00 ng

response 3307936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2024	BNA_N	<u>BN030531.D</u>
Compound Name	Response	Retention Time
DDT	1354385	20.586
DDD	20976	20.198
DDE	461	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21437	1375822	1.56

Instrument :
BNA_N
ClientSampleId :
DFTPP