
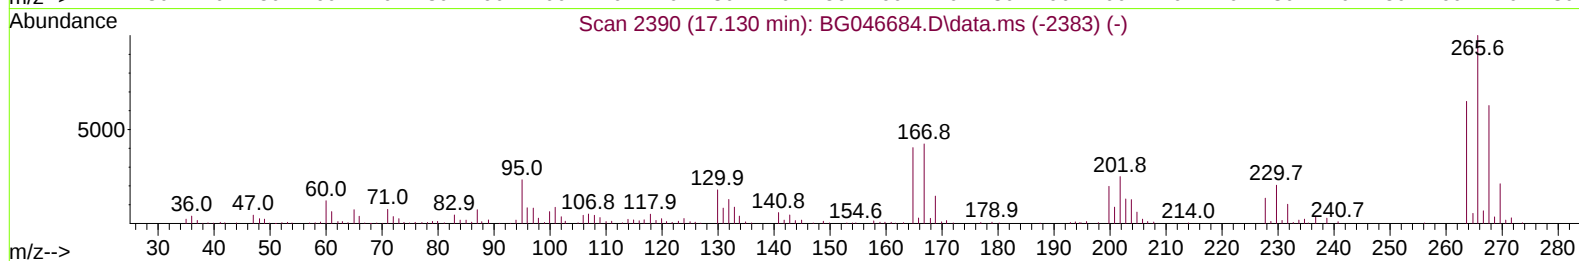
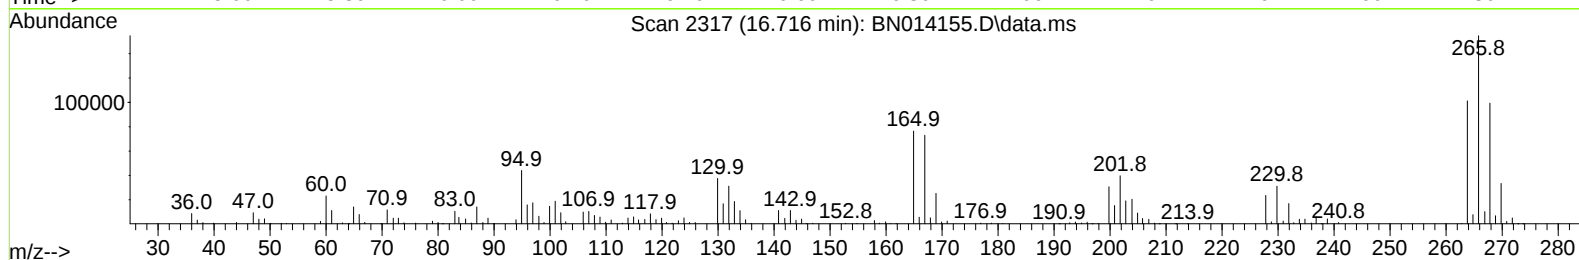


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033121\
 Data File : BN014155.D
 Acq On : 01 Apr 2021 00:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 08:31:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 09:00:06 2021
 Response via : Initial Calibration

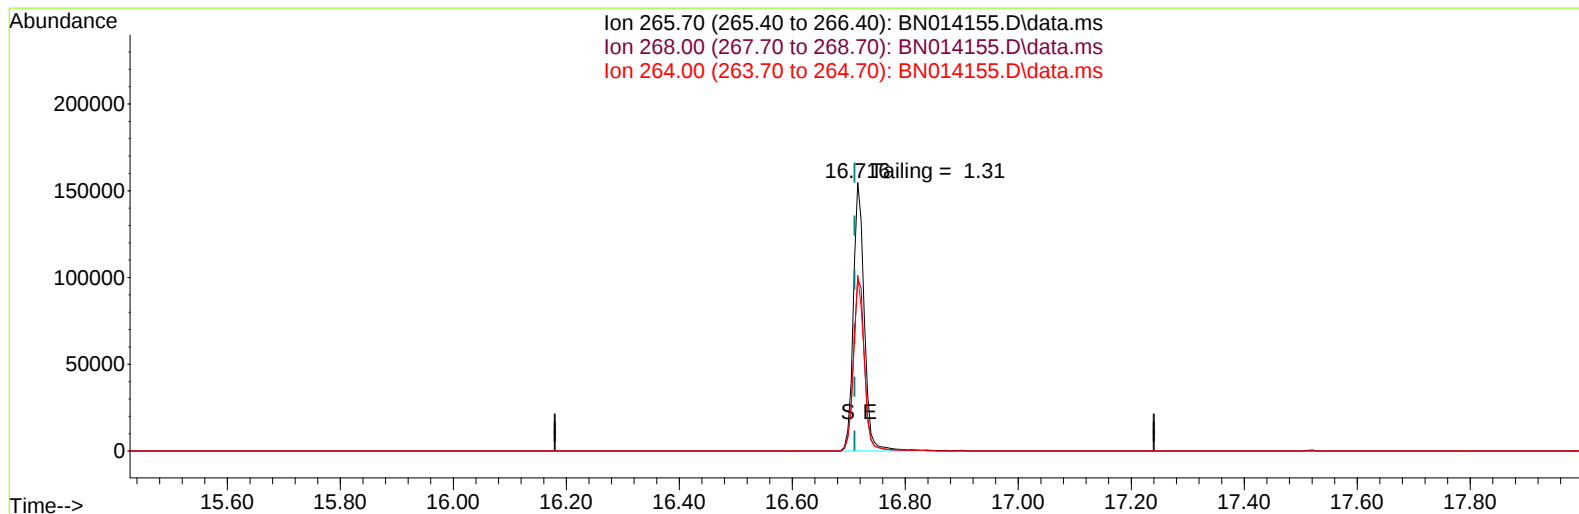

TIC: BN014155.D\data.ms

(70) Pentachlorophenol (C)




16.716min (+ 0.006) 18093.49 ng

response 208162

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033121\
Data File : BN014155.D
Acq On : 01 Apr 2021 00:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 08:31:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

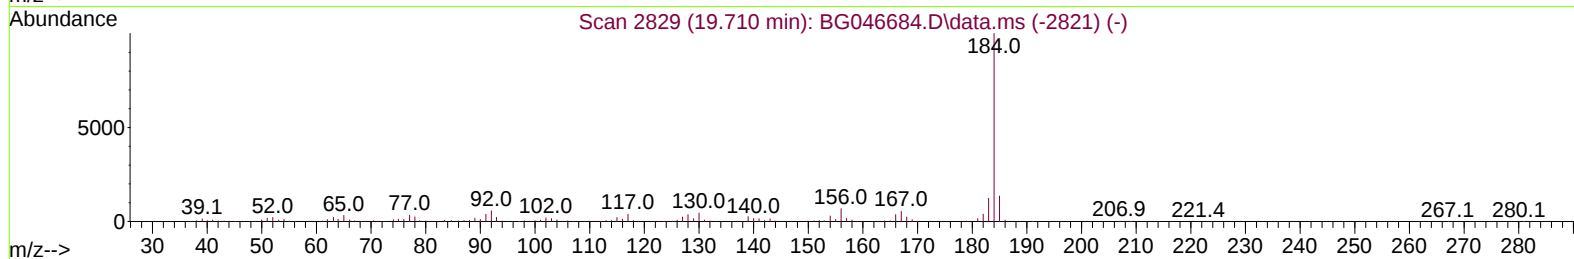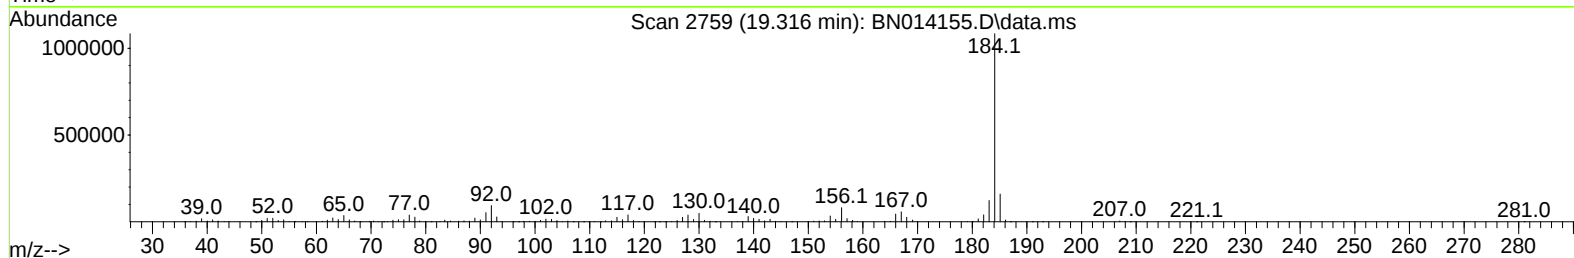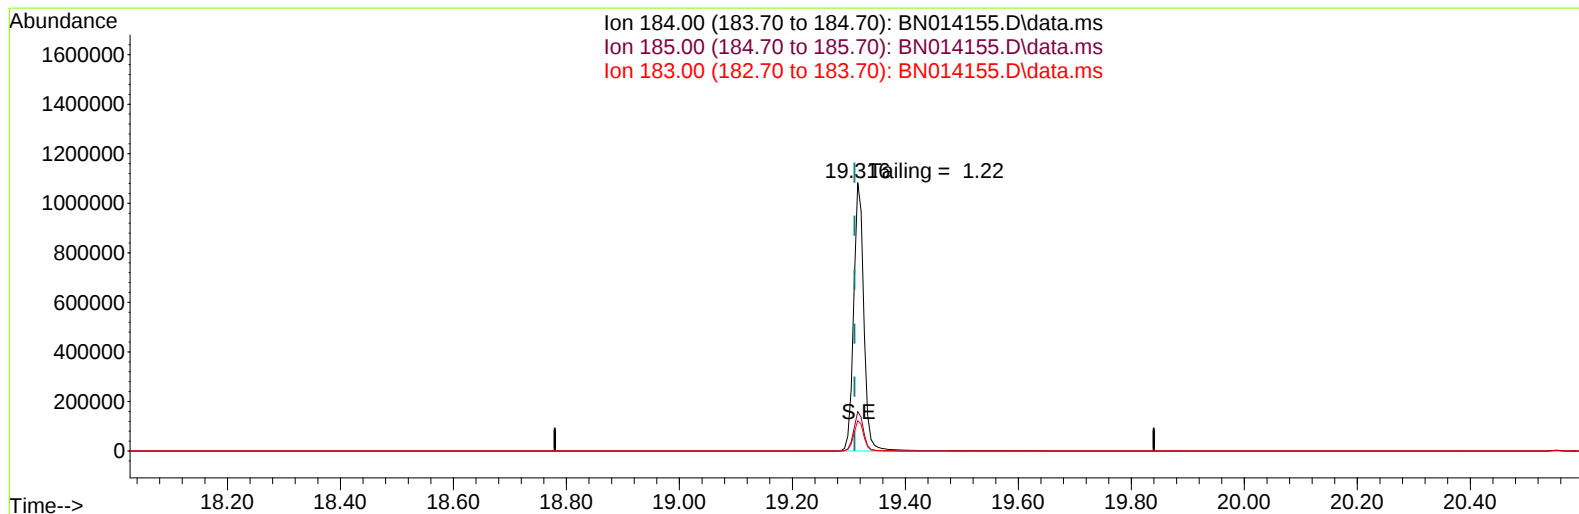

TIC: BN014155.D\data.ms

(77) Benzidine

19.316min (+ 0.006) 0.00 ng

response 1359312

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.76
183.00	13.20	11.32
0.00	0.00	0.00